

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB031219\
 Data File : FB020151.D
 Signal(s) : FID2B.CH
 Acq On : 12 Mar 2019 10:33
 Operator : MJ/SJ
 Sample : K1830-01
 Misc : 5.02gm/5.00ml DI WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BALLFIELD-SS-03072019

Integration File: Calibration.e
 Quant Time: Mar 13 02:27:35 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB031119.M
 Quant Title :
 QLast Update : Mon Mar 11 13:44:46 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.039	479531	18.266 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.891	3752	0.111 ng/ml
2) t 2,2,4-Trimethylpentane	7.654	19872	0.606 ng/ml
6) t Toluene	10.903	11272	0.305 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB031219\
Data File : FB020151.D
Signal(s) : FID2B.CH
Acq On : 12 Mar 2019 10:33
Operator : MJ/SJ
Sample : K1830-01
Misc : 5.02gm/5.00ml DI WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BALLFIELD-SS-03072019

Integration File: Calibration.e
Quant Time: Mar 13 02:27:35 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB031119.M
Quant Title :
QLast Update : Mon Mar 11 13:44:46 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

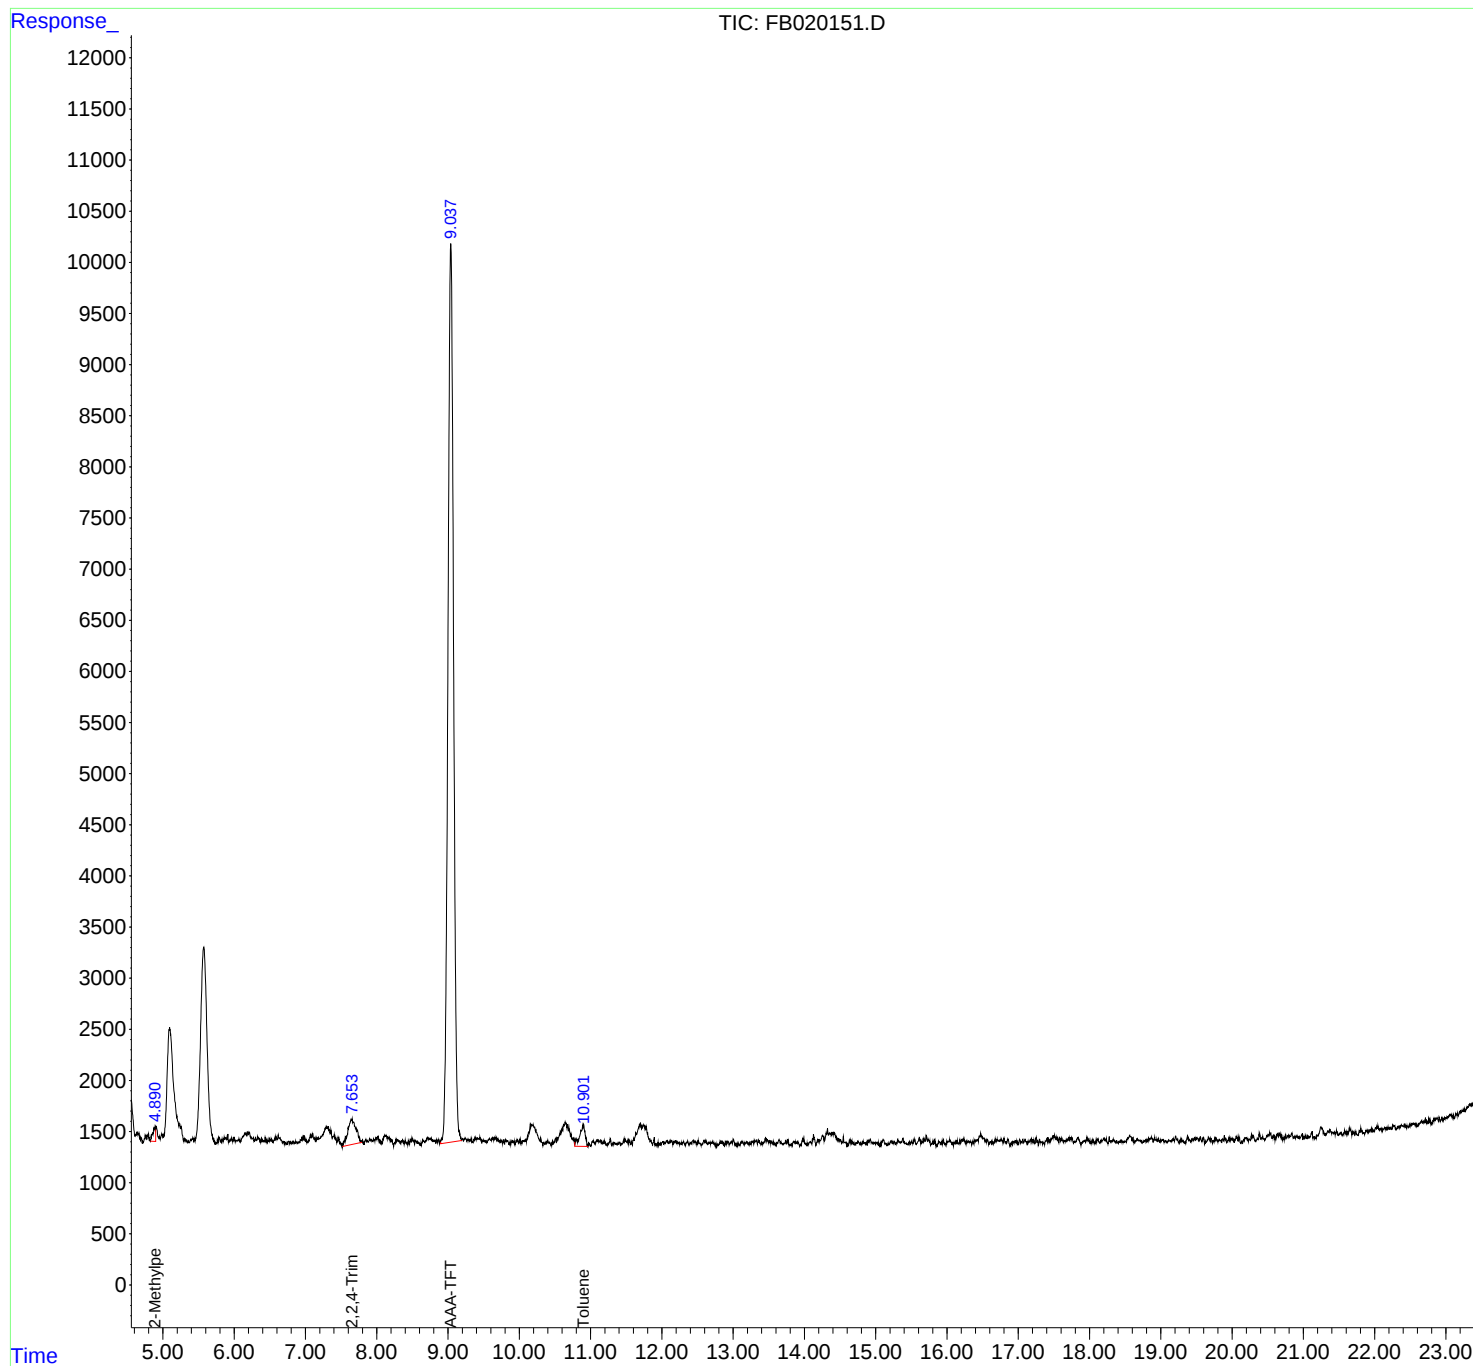


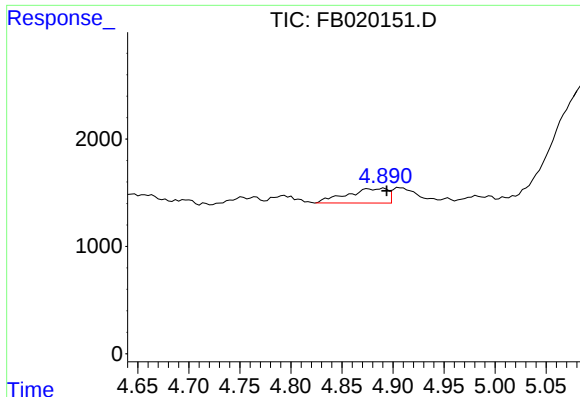

#1 2-Methylpentane


R.T.: 4.891 min
Delta R.T.: -0.003 min
Response: 3752
Conc: 0.11 ng/ml

Instrument :
FID_B
ClientSampleId :
BALLFIELD-SS-03072019

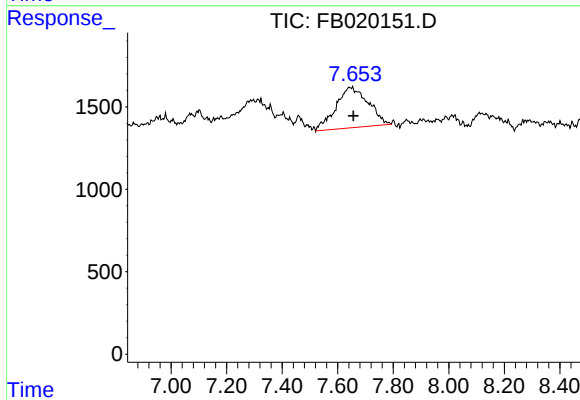


#2 2,2,4-Trimethylpentane

R.T.: 7.654 min
Delta R.T.: -0.004 min
Response: 19872
Conc: 0.61 ng/ml

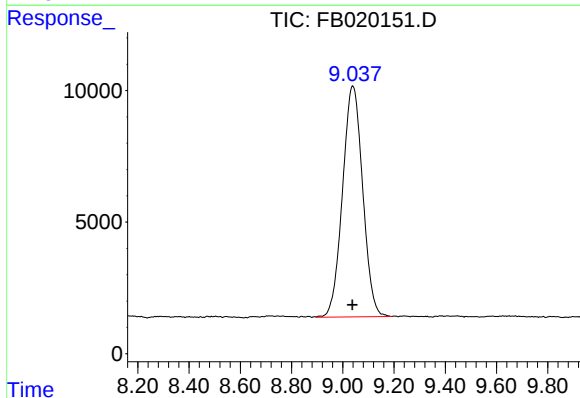

#5 AAA-TFT

R.T.: 9.039 min
Delta R.T.: 0.001 min
Response: 479531
Conc: 18.27 ng/ml

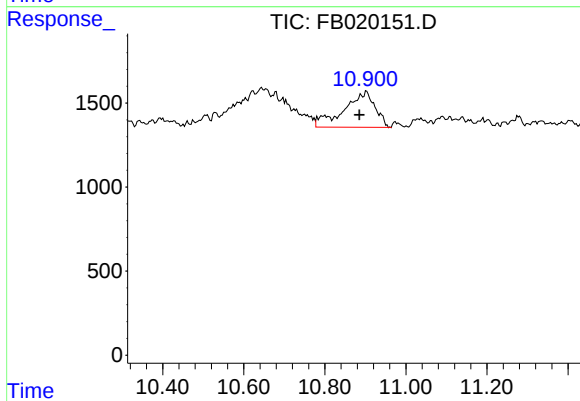

#6 Toluene

R.T.: 10.903 min
Delta R.T.: 0.017 min
Response: 11272
Conc: 0.31 ng/ml