

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB031219\
 Data File : FB020159.D
 Signal(s) : FID2B.CH
 Acq On : 12 Mar 2019 14:36
 Operator : MJ/SJ
 Sample : K1830-01MSD
 Misc : 5.04g/5.00ml DI WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BALLFIELD-SS-03072019MSD

Integration File: Calibration.e
 Quant Time: Mar 13 02:28:47 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB031119.M
 Quant Title :
 QLast Update : Mon Mar 11 13:44:46 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.040	501994	19.122 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.899	866141	25.676 ng/ml
2) t 2,2,4-Trimethylpentane	7.664	758965	23.143 ng/ml
3) t n-Heptane	7.995	335197	8.054 ng/ml
4) t Benzene	8.133	403816	8.674 ng/ml
6) t Toluene	10.887	907599	24.561 ng/ml
7) t Ethylbenzene	13.340	198429	8.434 ng/ml
8) t m-Xylene	13.474	380631	17.843 ng/ml
9) t O-Xylene	14.206	370136	19.539 ng/ml
10) t 1,2,4-Trimethylbenzene	16.492	379467	19.134 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB031219\
Data File : FB020159.D
Signal(s) : FID2B.CH
Acq On : 12 Mar 2019 14:36
Operator : MJ/SJ
Sample : K1830-01MSD
Misc : 5.04g/5.00ml DI WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BALLFIELD-SS-03072019MSD

Integration File: Calibration.e
Quant Time: Mar 13 02:28:47 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB031119.M
Quant Title :
QLast Update : Mon Mar 11 13:44:46 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

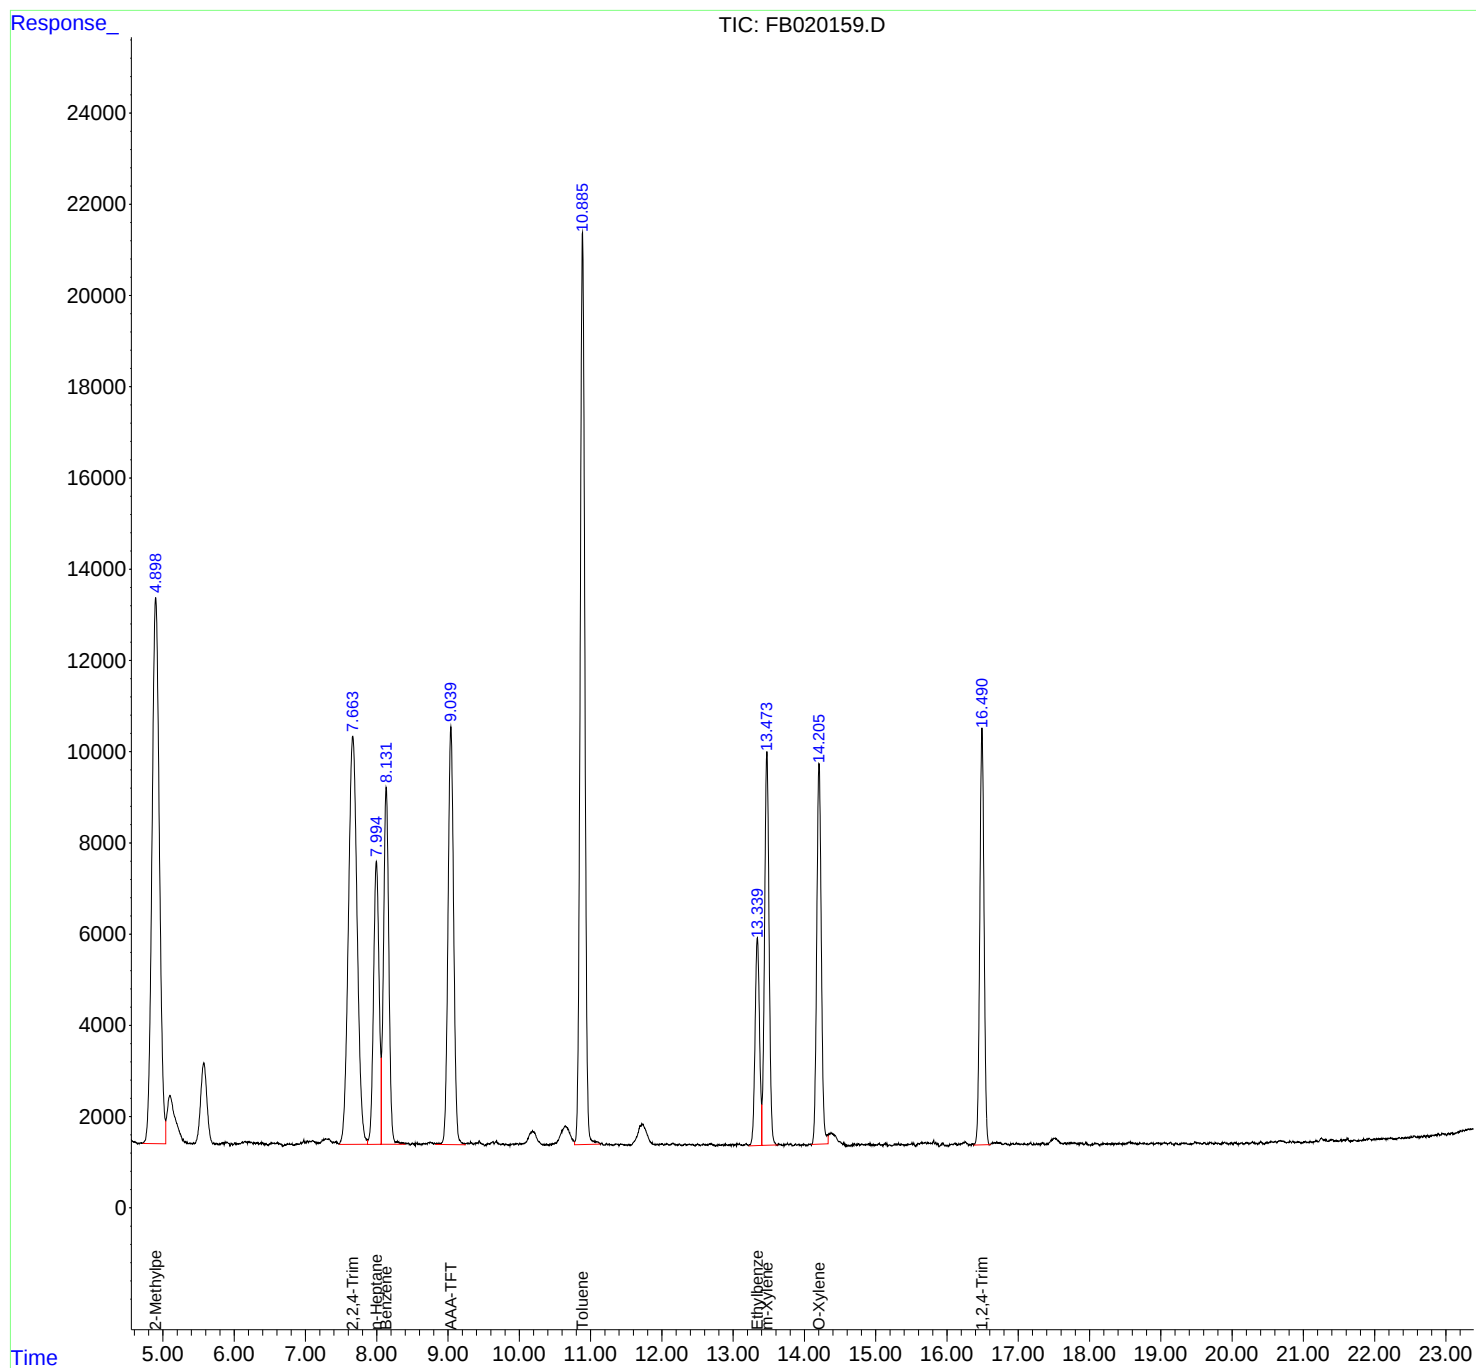


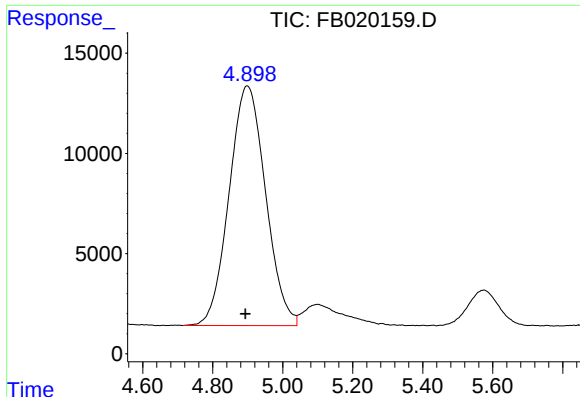

#1 2-Methylpentane


R.T.: 4.899 min
Delta R.T.: 0.005 min
Response: 866141
Conc: 25.68 ng/ml

Instrument :
FID_B
ClientSampleId :
BALLFIELD-SS-03072019MSD

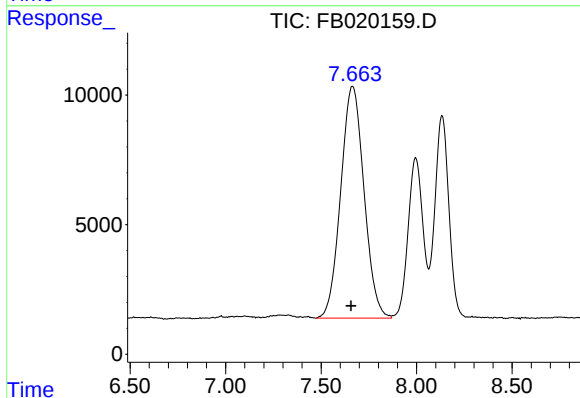


#2 2,2,4-Trimethylpentane

R.T.: 7.664 min
Delta R.T.: 0.007 min
Response: 758965
Conc: 23.14 ng/ml

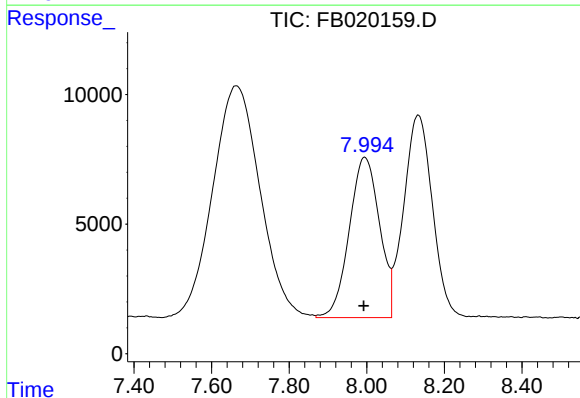


#3 n-Heptane

R.T.: 7.995 min
Delta R.T.: 0.003 min
Response: 335197
Conc: 8.05 ng/ml

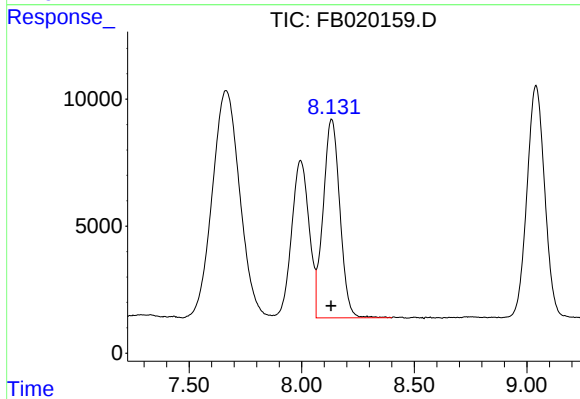


#4 Benzene

R.T.: 8.133 min
Delta R.T.: 0.003 min
Response: 403816
Conc: 8.67 ng/ml

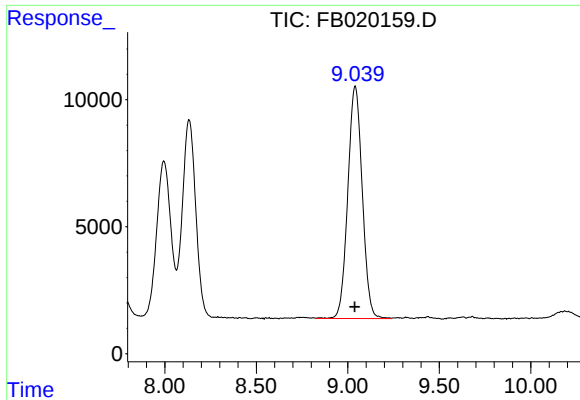


#5 AAA-TFT
 R.T.: 9.040 min
 Delta R.T.: 0.002 min
 Response: 501994
 Conc: 19.12 ng/ml


Instrument :
 FID_B
 ClientSampleId :
 BALLFIELD-SS-03072019MSD

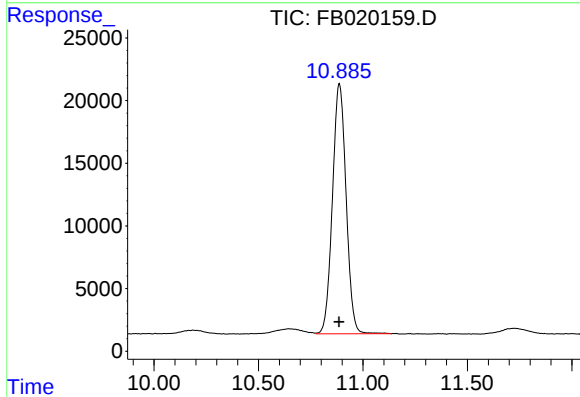


#6 Toluene
 R.T.: 10.887 min
 Delta R.T.: 0.002 min
 Response: 907599
 Conc: 24.56 ng/ml

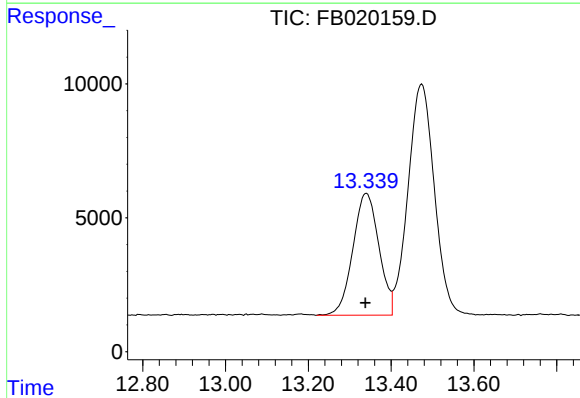

#7 Ethylbenzene
 R.T.: 13.340 min
 Delta R.T.: 0.002 min
 Response: 198429
 Conc: 8.43 ng/ml

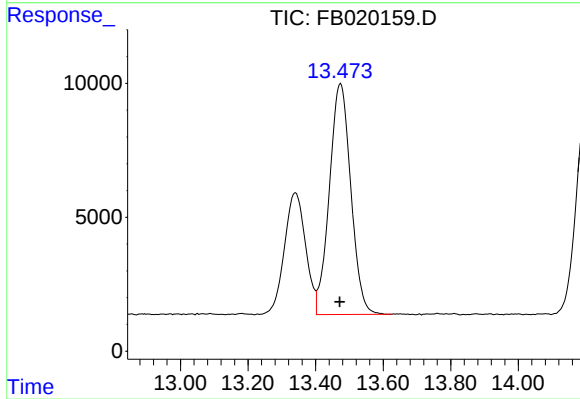


#8 m-Xylene
 R.T.: 13.474 min
 Delta R.T.: 0.002 min
 Response: 380631
 Conc: 17.84 ng/ml

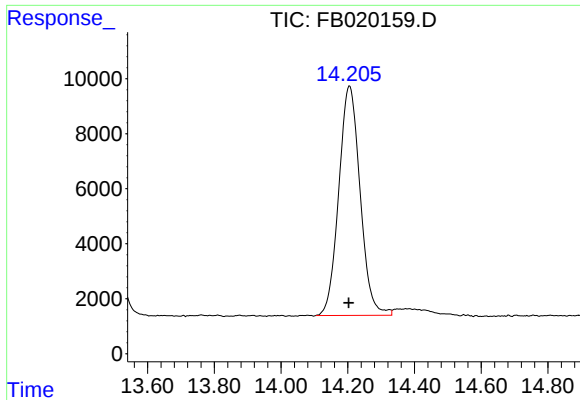

#9 O-Xylene

R.T.: 14.206 min
Delta R.T.: 0.003 min
Response: 370136
Conc: 19.54 ng/ml

Instrument :
FID_B
ClientSampleId :
BALLFIELD-SS-03072019MSD

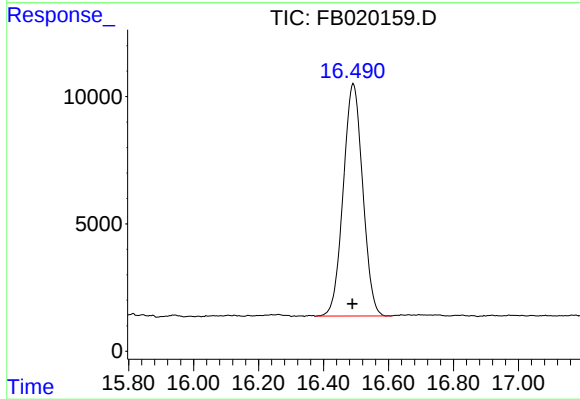

#10 1,2,4-Trimethylbenzene

R.T.: 16.492 min
Delta R.T.: 0.003 min
Response: 379467
Conc: 19.13 ng/ml