

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB031219\
 Data File : FB020167.D
 Signal(s) : FID2B.CH
 Acq On : 12 Mar 2019 18:38
 Operator : MJ/SJ
 Sample : K1687-05
 Misc : 5.03g/5.00ml DI WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 HR-06-031119-C

Integration File: Calibration.e
 Quant Time: Mar 13 02:30:16 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB031119.M
 Quant Title :
 QLast Update : Mon Mar 11 13:44:46 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.040	431459	16.435 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.912	4537	0.134 ng/ml
2) t 2,2,4-Trimethylpentane	7.665	10597	0.323 ng/ml
6) t Toluene	10.894	6783	0.184 ng/ml
7) t Ethylbenzene	13.314	9614	0.409 ng/ml
8) t m-Xylene	13.475	9487	0.445 ng/ml
9) t O-Xylene	14.207	12632	0.667 ng/ml
10) t 1,2,4-Trimethylbenzene	16.492	69391	3.499 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB031219\
Data File : FB020167.D
Signal(s) : FID2B.CH
Acq On : 12 Mar 2019 18:38
Operator : MJ/SJ
Sample : K1687-05
Misc : 5.03g/5.00ml DI WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
HR-06-031119-C

Integration File: Calibration.e
Quant Time: Mar 13 02:30:16 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB031119.M
Quant Title :
QLast Update : Mon Mar 11 13:44:46 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

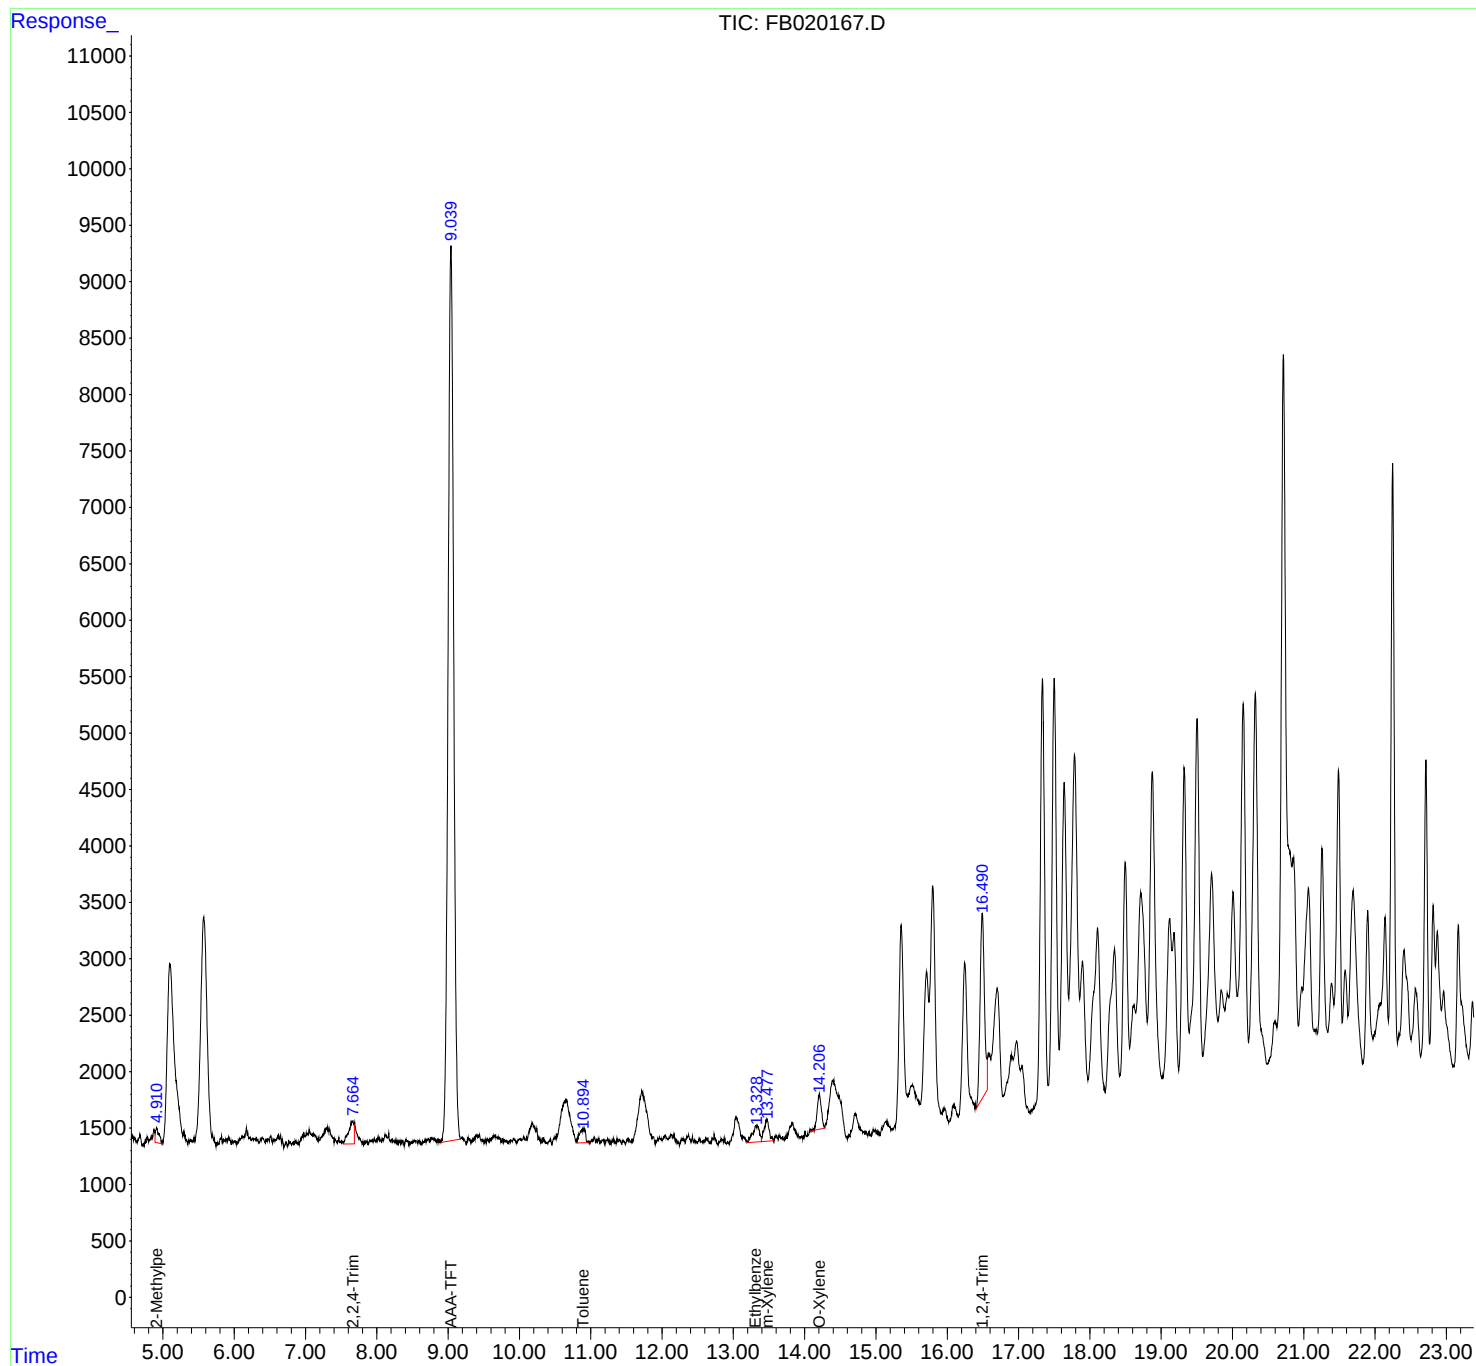


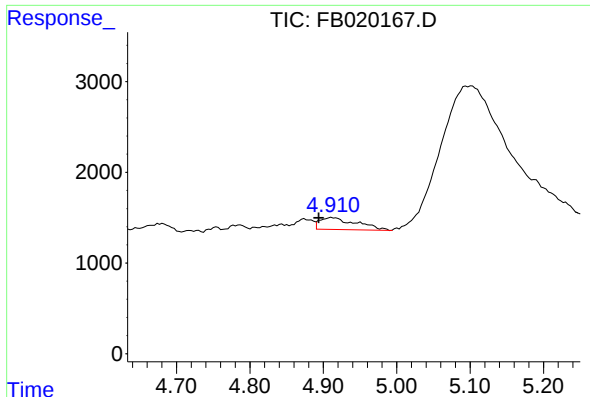

#1 2-Methylpentane


R.T.: 4.912 min
Delta R.T.: 0.018 min
Response: 4537
Conc: 0.13 ng/ml

Instrument :
FID_B
ClientSampleId :
HR-06-031119-C

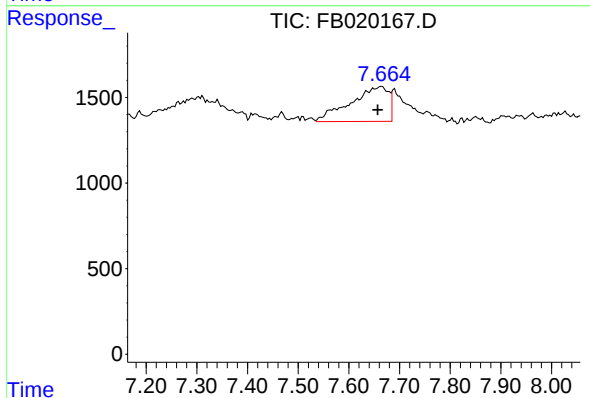


#2 2,2,4-Trimethylpentane

R.T.: 7.665 min
Delta R.T.: 0.008 min
Response: 10597
Conc: 0.32 ng/ml

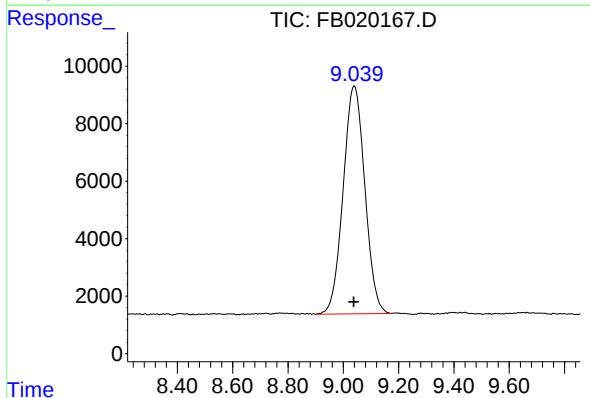


#5 AAA-TFT

R.T.: 9.040 min
Delta R.T.: 0.002 min
Response: 431459
Conc: 16.43 ng/ml

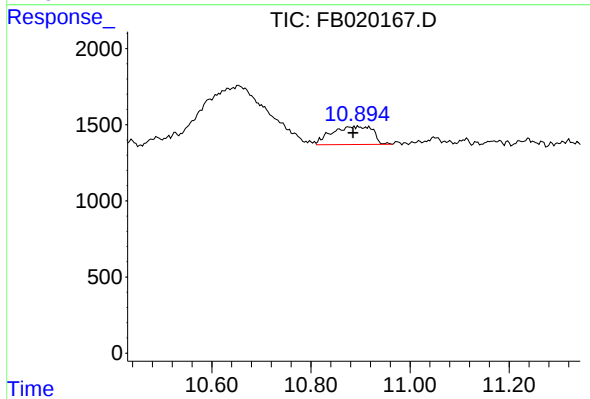

#6 Toluene


R.T.: 10.894 min
Delta R.T.: 0.009 min
Response: 6783
Conc: 0.18 ng/ml

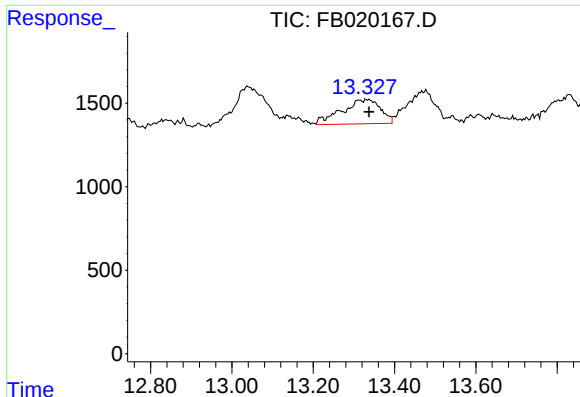

#7 Ethylbenzene


R.T.: 13.314 min
Delta R.T.: -0.024 min
Response: 9614
Conc: 0.41 ng/ml

Instrument :
FID_B
ClientSampleId :
HR-06-031119-C

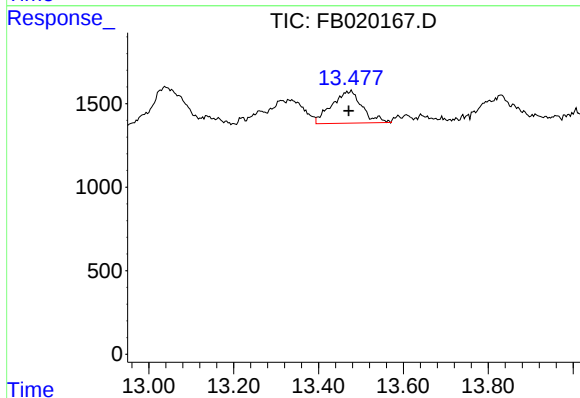


#8 m-Xylene

R.T.: 13.475 min
Delta R.T.: 0.004 min
Response: 9487
Conc: 0.44 ng/ml

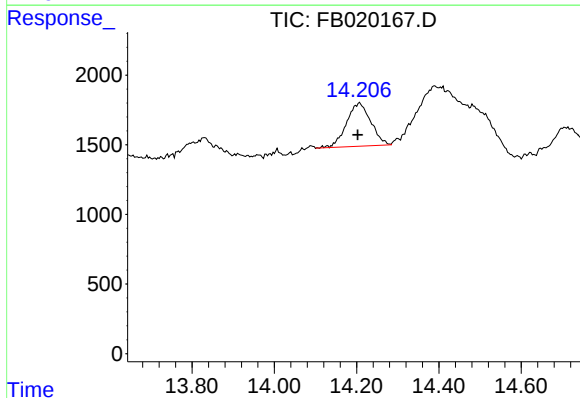

#9 O-Xylene

R.T.: 14.207 min
Delta R.T.: 0.004 min
Response: 12632
Conc: 0.67 ng/ml

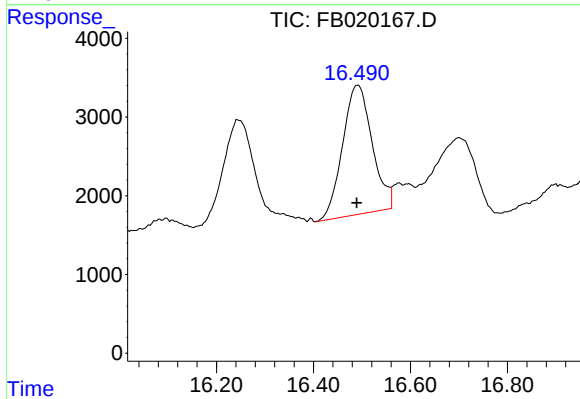

#10 1,2,4-Trimethylbenzene

R.T.: 16.492 min
Delta R.T.: 0.002 min
Response: 69391
Conc: 3.50 ng/ml