

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB031220\
 Data File : FB023899.D
 Signal(s) : FID2B.CH
 Acq On : 12 Mar 2020 18:56
 Operator : DD/AJ
 Sample : L1907-02MSD
 Misc : 5.03g/5.00ml DI WATER
 ALS Vial : 15 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Mar 13 03:36:08 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030520.M
 Quant Title :
 QLast Update : Thu Mar 05 11:03:12 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	8.800	457768	21.746 ng/ml
Target Compounds				
1) t	2-Methylpentane	4.690	927494	30.011 ng/ml
2) t	2,2,4-Trimethylpentane	7.418	977707	28.994 ng/ml
3) t	n-Heptane	7.758	321615	9.708 ng/ml
4) t	Benzene	7.893	429498	10.257 ng/ml
6) t	Toluene	10.631	1248587	30.623 ng/ml
7) t	Ethylbenzene	13.071	379436	9.931 ng/ml
8) t	m-Xylene	13.204	726081	19.721 ng/ml
9) t	O-Xylene	13.932	695798	19.564 ng/ml
10) t	1,2,4-Trimethylbenzene	16.210	604252	19.945 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB031220\
Data File : FB023899.D
Signal(s) : FID2B.CH
Acq On : 12 Mar 2020 18:56
Operator : DD/AJ
Sample : L1907-02MSD
Misc : 5.03g/5.00ml DI WATER
ALS Vial : 15 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Mar 13 03:36:08 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030520.M
Quant Title :
QLast Update : Thu Mar 05 11:03:12 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

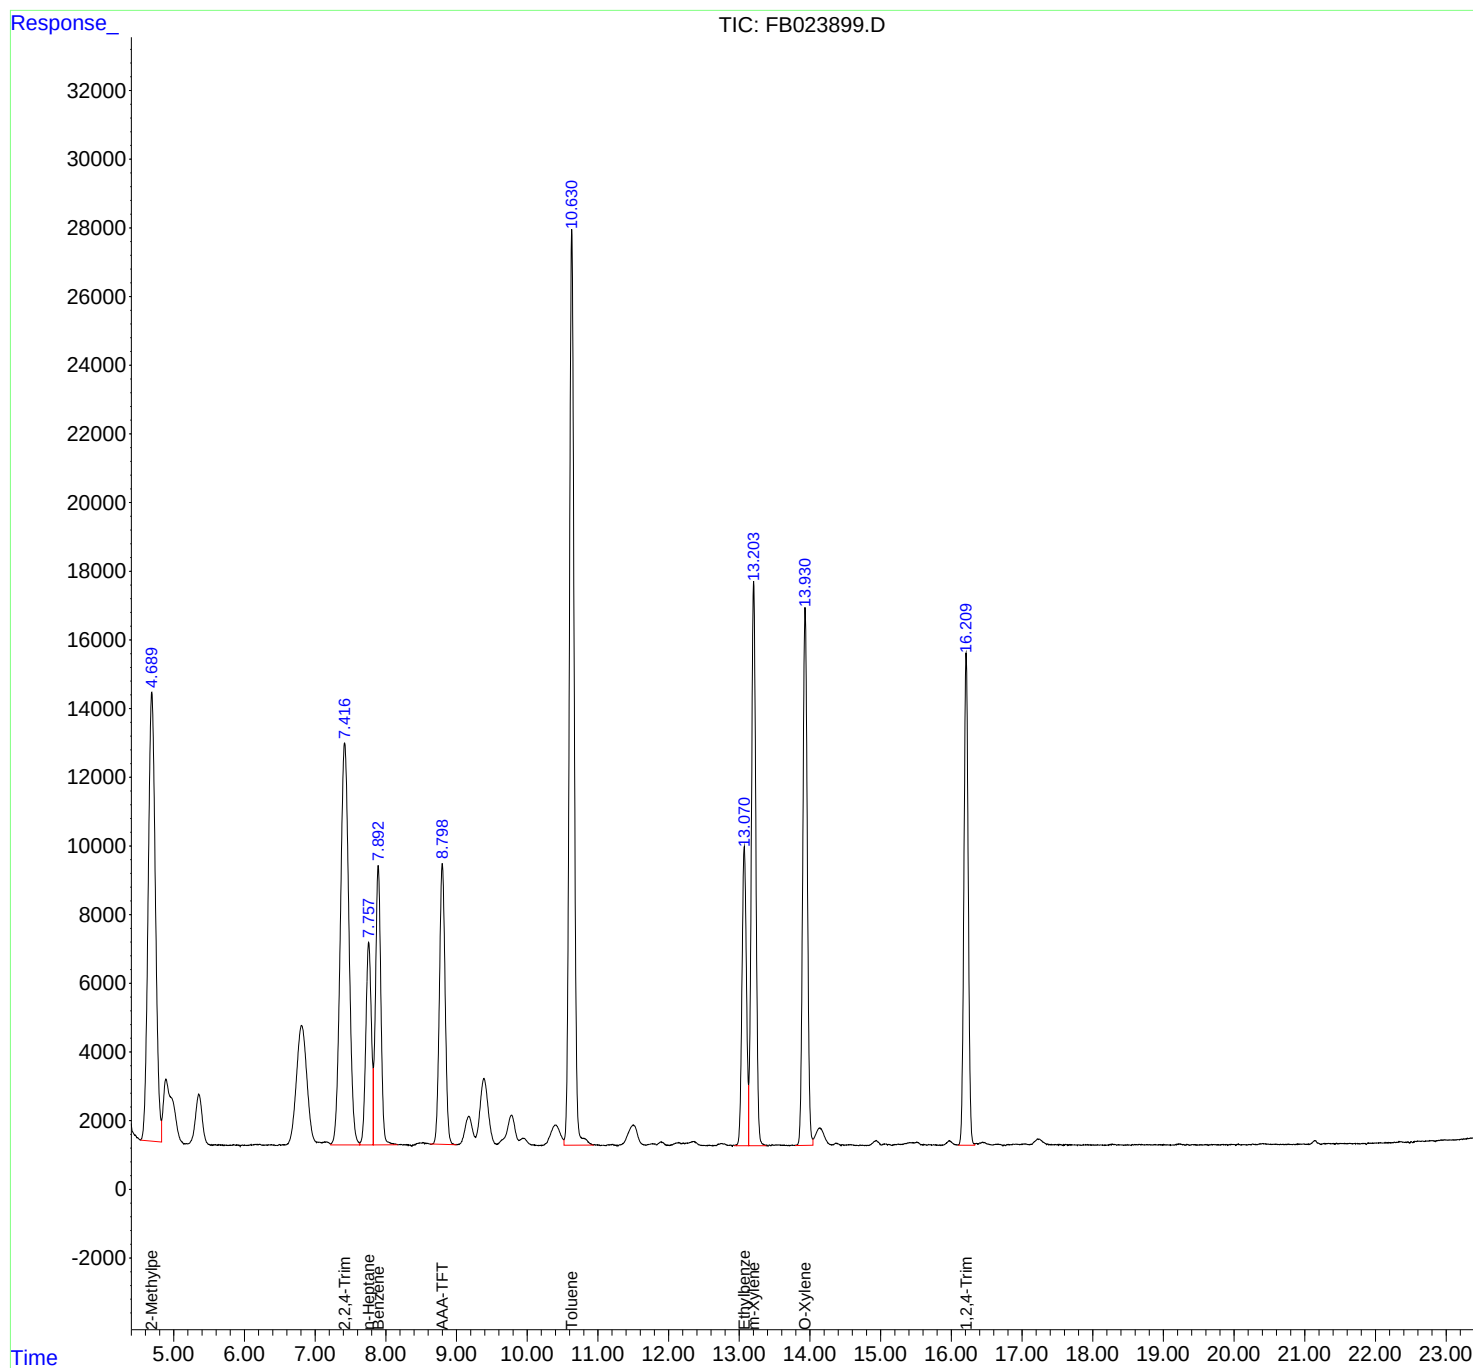

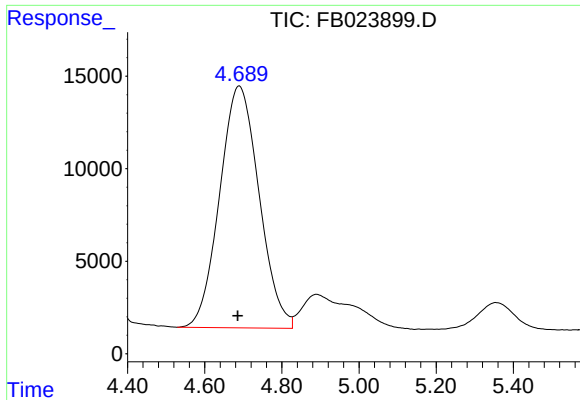


#1 2-Methylpentane

R.T.: 4.690 min
Delta R.T.: 0.004 min
Response: 927494
Conc: 30.01 ng/ml

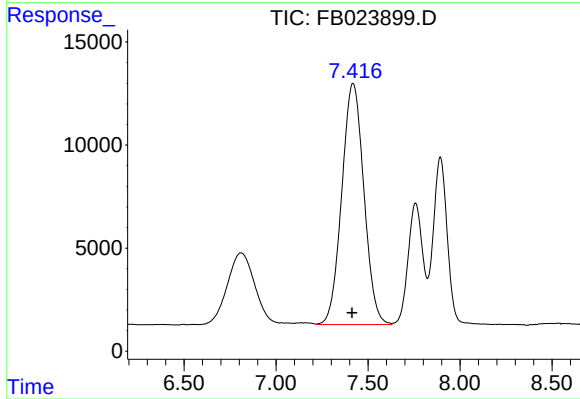


#2 2,2,4-Trimethylpentane

R.T.: 7.418 min
Delta R.T.: 0.005 min
Response: 977707
Conc: 28.99 ng/ml

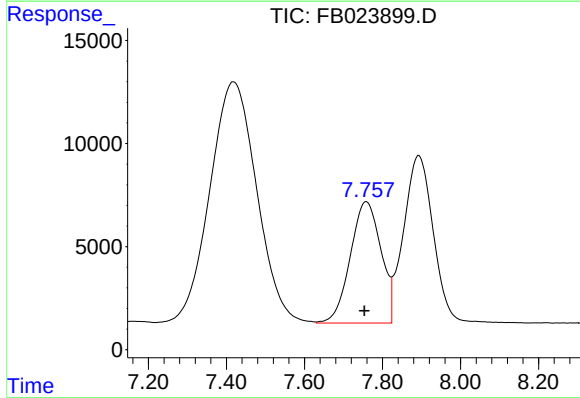


#3 n-Heptane

R.T.: 7.758 min
Delta R.T.: 0.005 min
Response: 321615
Conc: 9.71 ng/ml

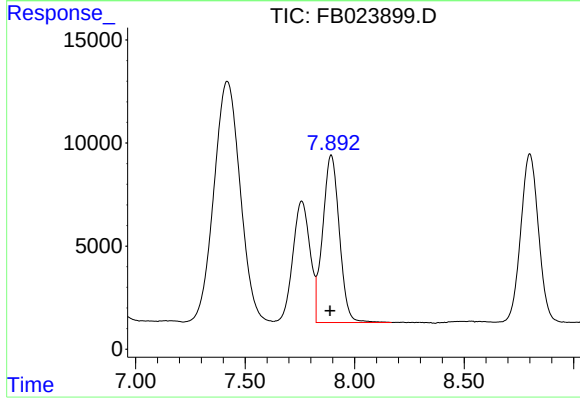


#4 Benzene

R.T.: 7.893 min
Delta R.T.: 0.005 min
Response: 429498
Conc: 10.26 ng/ml

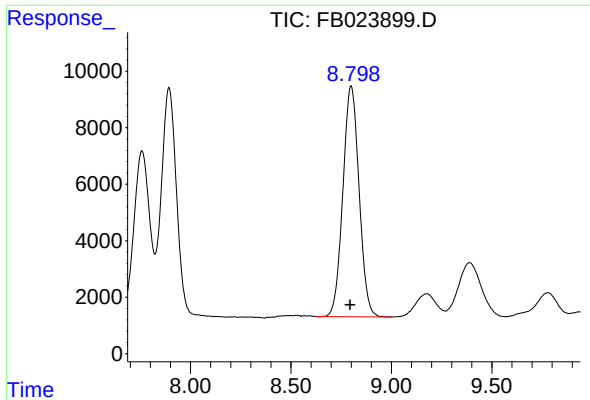


#5 AAA-TFT

R.T.: 8.800 min
Delta R.T.: 0.005 min
Response: 457768
Conc: 21.75 ng/ml

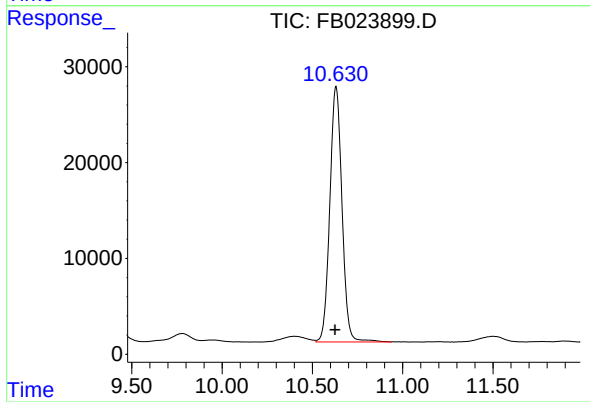


#6 Toluene

R.T.: 10.631 min
Delta R.T.: 0.005 min
Response: 1248587
Conc: 30.62 ng/ml

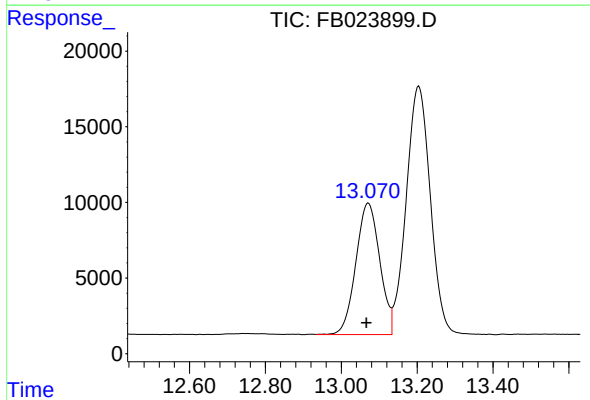


#7 Ethylbenzene

R.T.: 13.071 min
Delta R.T.: 0.005 min
Response: 379436
Conc: 9.93 ng/ml

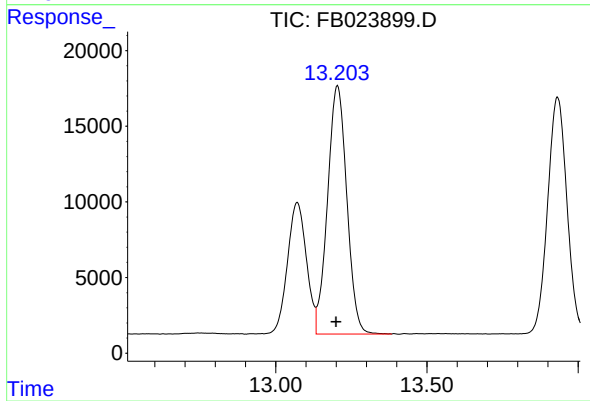


#8 m-Xylene

R.T.: 13.204 min
Delta R.T.: 0.005 min
Response: 726081
Conc: 19.72 ng/ml

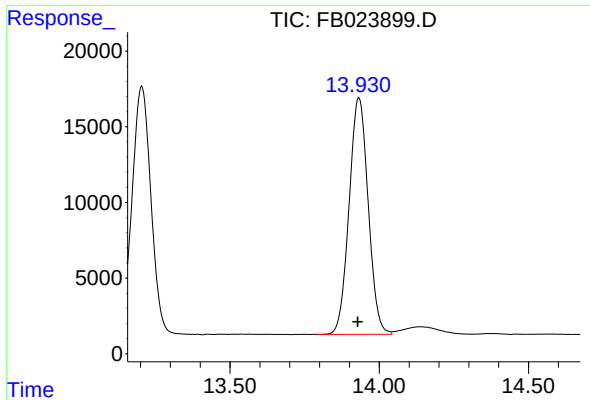

#9 O-Xylene

R.T.: 13.932 min
Delta R.T.: 0.004 min
Response: 695798
Conc: 19.56 ng/ml

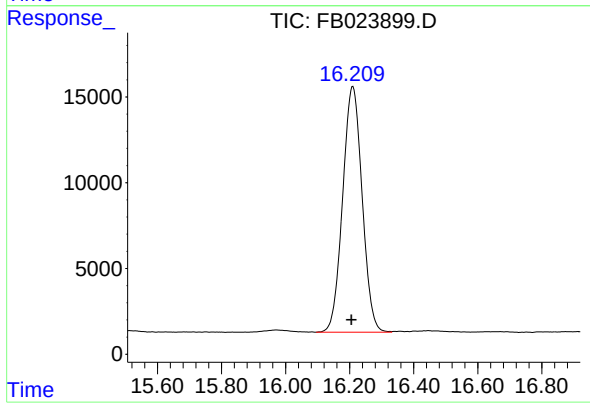

#10 1,2,4-Trimethylbenzene

R.T.: 16.210 min
Delta R.T.: 0.004 min
Response: 604252
Conc: 19.95 ng/ml