

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB031220\
Data File : FB023905.D
Signal(s) : FID2B.CH
Acq On : 12 Mar 2020 22:30
Operator : DD/AJ
Sample : L1912-07
Misc : 5.05g/5.00ml DI WATER
ALS Vial : 22 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Mar 13 03:36:35 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030520.M
Quant Title :
QLast Update : Thu Mar 05 11:03:12 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.799	375843	17.854 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.694	4296	0.139 ng/ml
6) t Toluene	10.559	90	0.002 ng/ml
8) t m-Xylene	13.198	3377	0.092 ng/ml
9) t O-Xylene	13.922	405	0.011 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB031220\
Data File : FB023905.D
Signal(s) : FID2B.CH
Acq On : 12 Mar 2020 22:30
Operator : DD/AJ
Sample : L1912-07
Misc : 5.05g/5.00ml DI WATER
ALS Vial : 22 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Mar 13 03:36:35 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030520.M
Quant Title :
QLast Update : Thu Mar 05 11:03:12 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

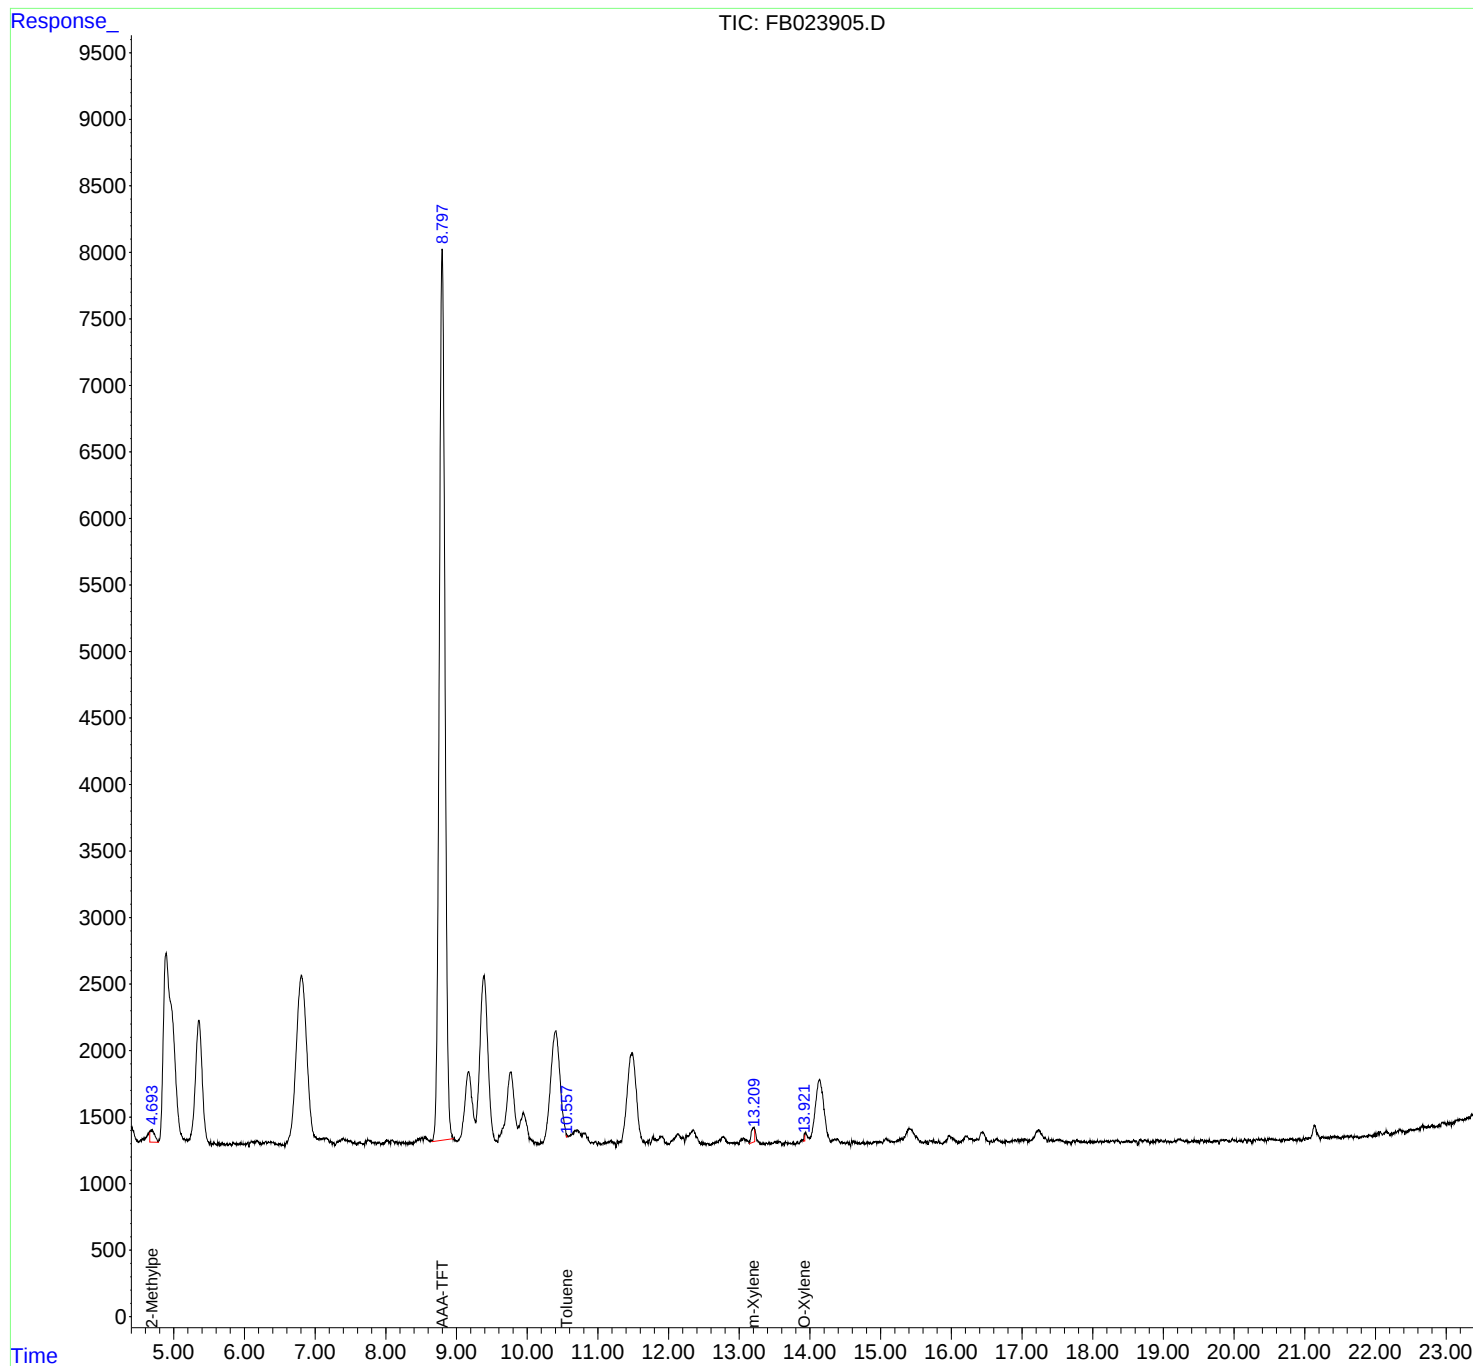

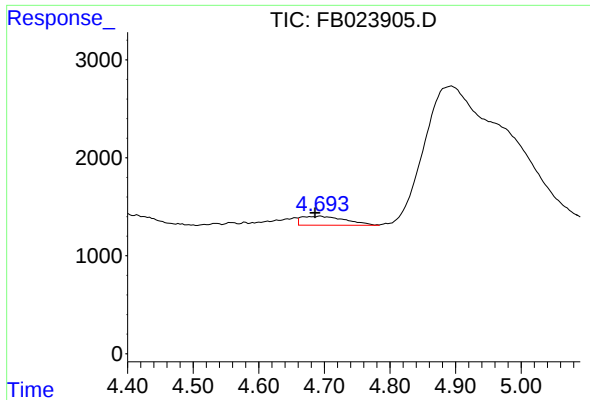


#1 2-Methylpentane

R.T.: 4.694 min
Delta R.T.: 0.008 min
Response: 4296
Conc: 0.14 ng/ml

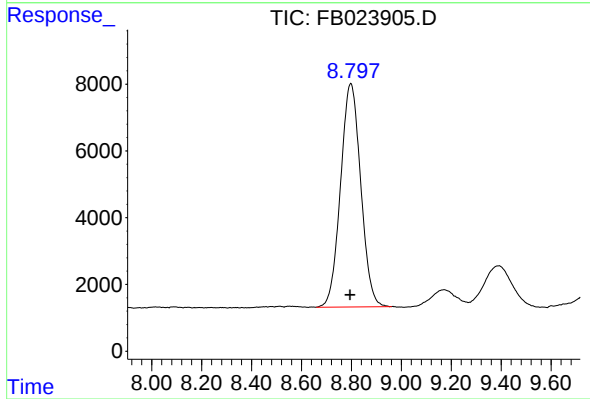


#5 AAA-TFT

R.T.: 8.799 min
Delta R.T.: 0.004 min
Response: 375843
Conc: 17.85 ng/ml

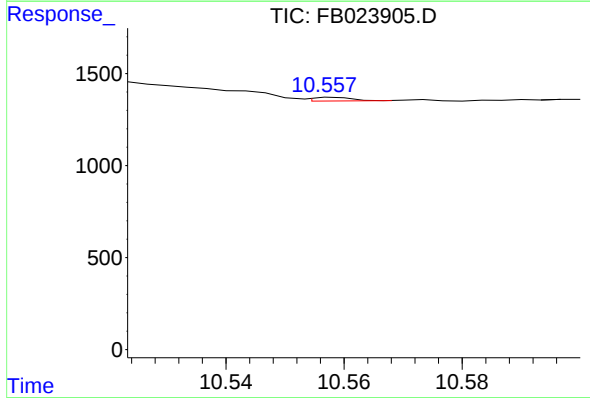


#6 Toluene

R.T.: 10.559 min
Delta R.T.: -0.067 min
Response: 90
Conc: 0.00 ng/ml

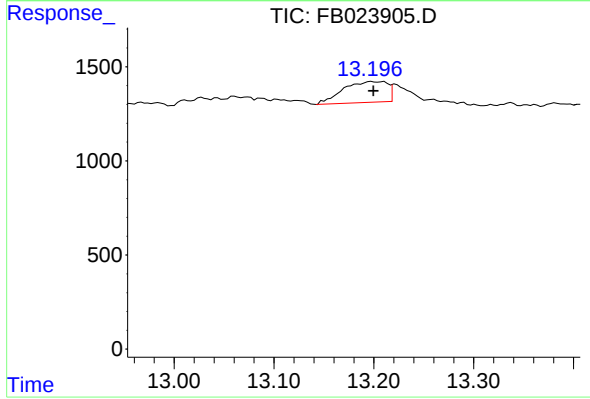

#8 m-Xylene

R.T.: 13.198 min
Delta R.T.: -0.002 min
Response: 3377
Conc: 0.09 ng/ml

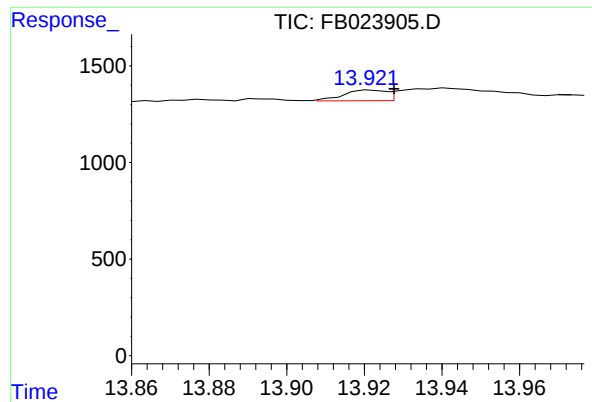

#9 O-Xylene

R.T.: 13.922 min
Delta R.T.: -0.005 min
Response: 405
Conc: 0.01 ng/ml