

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB031220\
 Data File : FB023890.D
 Signal(s) : FID2B.CH
 Acq On : 12 Mar 2020 14:20
 Operator : DD/AJ
 Sample : L1893-15MS
 Misc : 5.06g/5.00ml DI WATER
 ALS Vial : 6 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Mar 13 03:35:23 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030520.M
 Quant Title :
 QLast Update : Thu Mar 05 11:03:12 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.797	212271	10.084 ng/mlm
Target Compounds			
1) t 2-Methylpentane	4.694	408226	13.209 ng/ml
2) t 2,2,4-Trimethylpentane	7.420	438134	12.993 ng/ml
3) t n-Heptane	7.759	140360	4.237 ng/ml
4) t Benzene	7.892	188452	4.501 ng/ml
6) t Toluene	10.630	547943	13.439 ng/ml
7) t Ethylbenzene	13.070	156084	4.085 ng/ml
8) t m-Xylene	13.203	306214	8.317 ng/ml
9) t O-Xylene	13.931	292406	8.222 ng/ml
10) t 1,2,4-Trimethylbenzene	16.209	217162	7.168 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB031220\
Data File : FB023890.D
Signal(s) : FID2B.CH
Acq On : 12 Mar 2020 14:20
Operator : DD/AJ
Sample : L1893-15MS
Misc : 5.06g/5.00ml DI WATER
ALS Vial : 6 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Mar 13 03:35:23 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030520.M
Quant Title :
QLast Update : Thu Mar 05 11:03:12 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

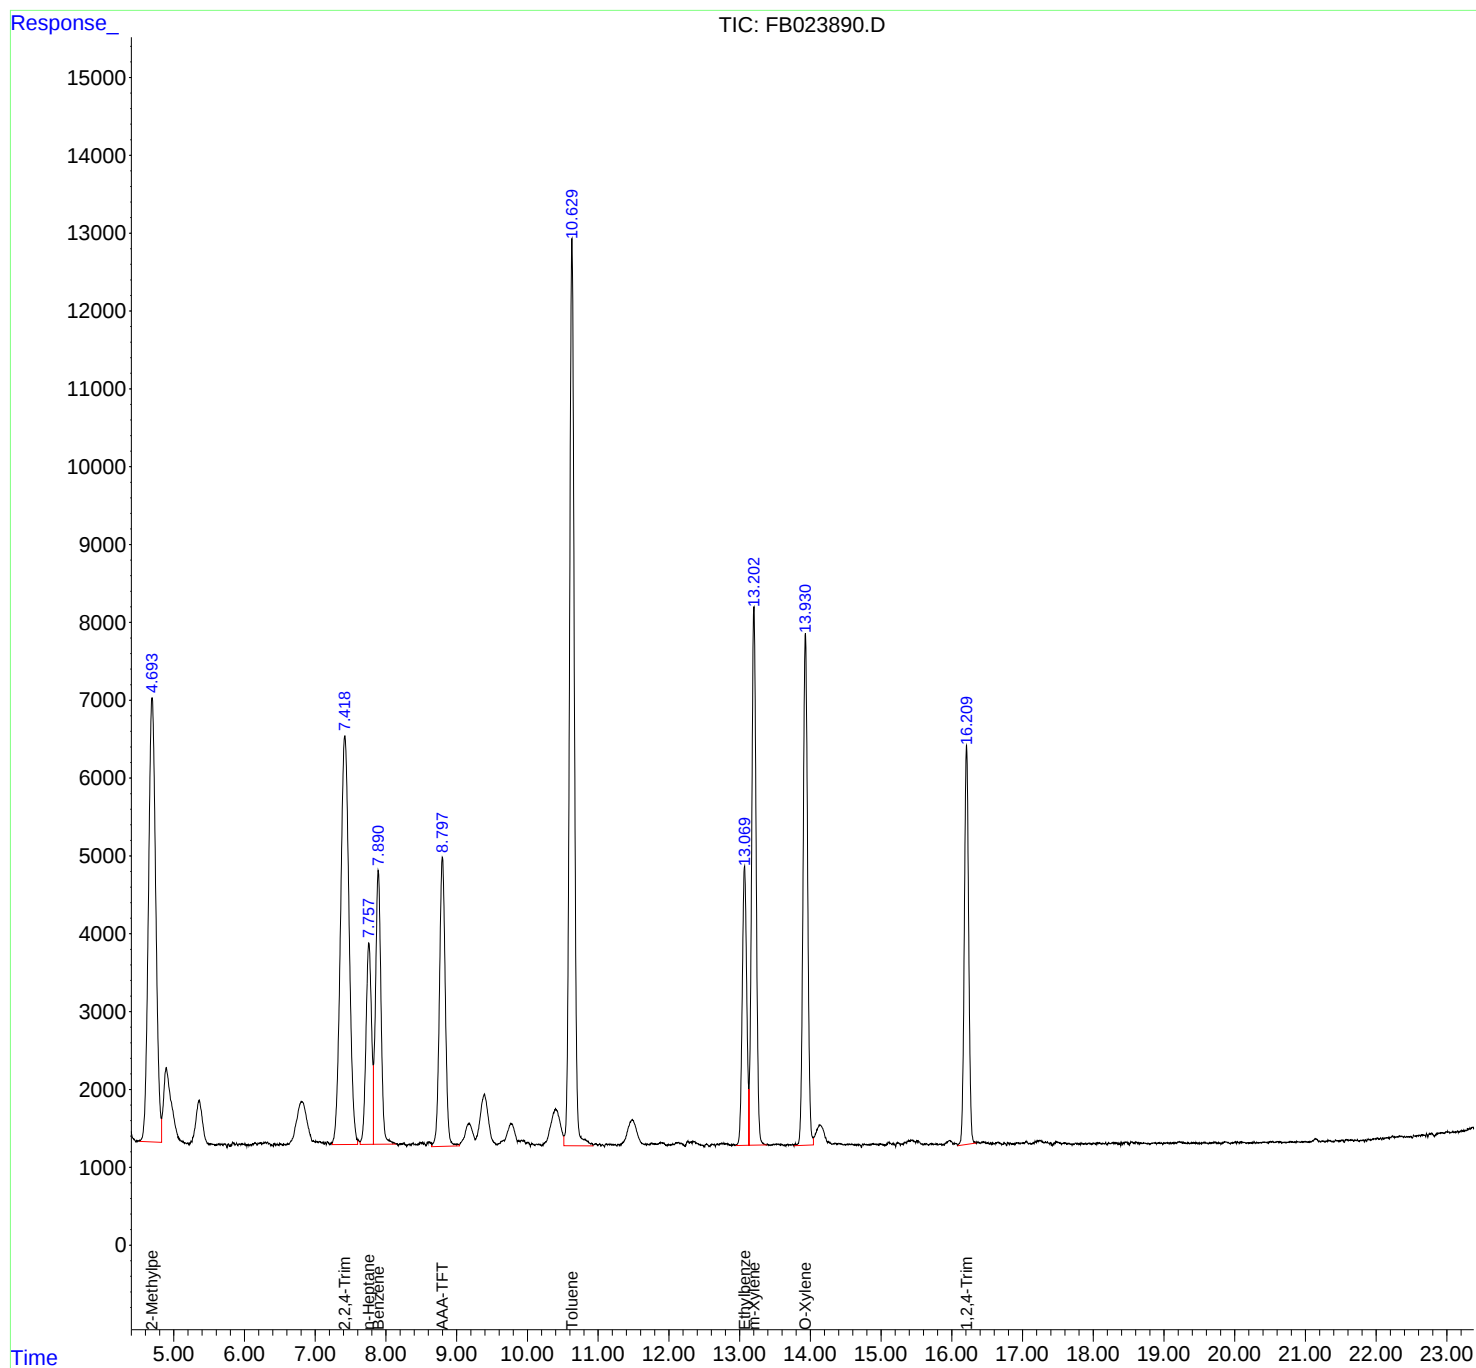

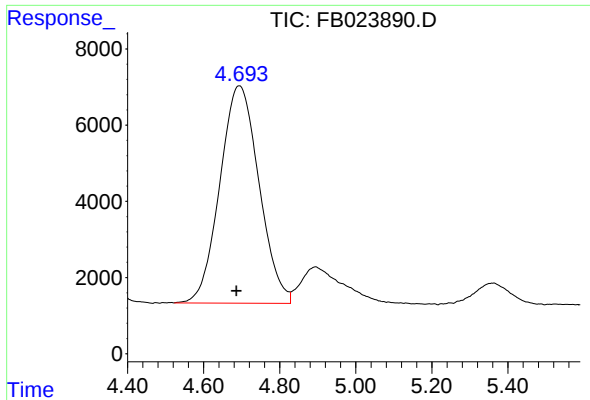


#1 2-Methylpentane

R.T.: 4.694 min
Delta R.T.: 0.008 min
Response: 408226
Conc: 13.21 ng/ml

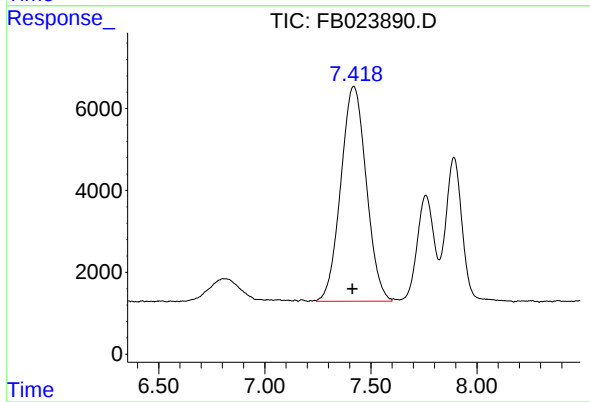


#2 2,2,4-Trimethylpentane

R.T.: 7.420 min
Delta R.T.: 0.007 min
Response: 438134
Conc: 12.99 ng/ml

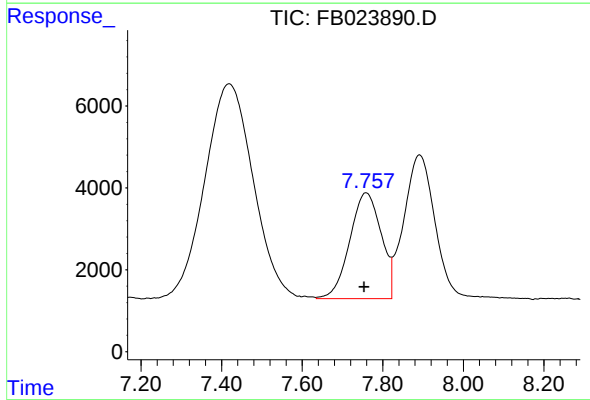


#3 n-Heptane

R.T.: 7.759 min
Delta R.T.: 0.006 min
Response: 140360
Conc: 4.24 ng/ml

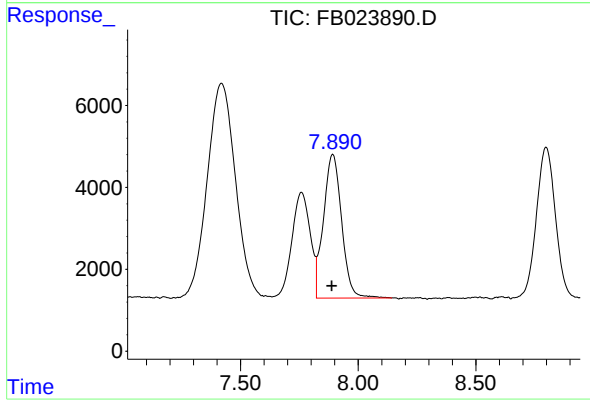


#4 Benzene

R.T.: 7.892 min
Delta R.T.: 0.004 min
Response: 188452
Conc: 4.50 ng/ml

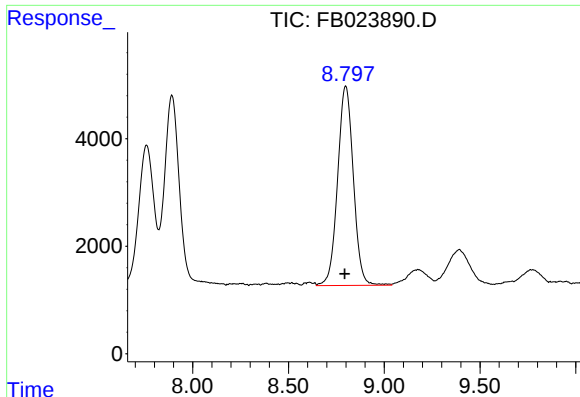


#5 AAA-TFT

R.T.: 8.797 min
Delta R.T.: 0.003 min
Response: 212271
Conc: 10.08 ng/ml m

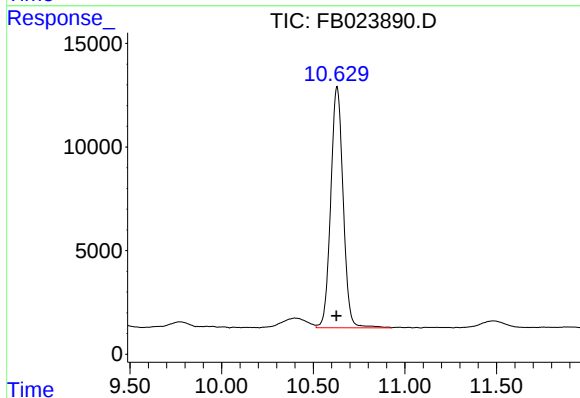


#6 Toluene

R.T.: 10.630 min
Delta R.T.: 0.004 min
Response: 547943
Conc: 13.44 ng/ml

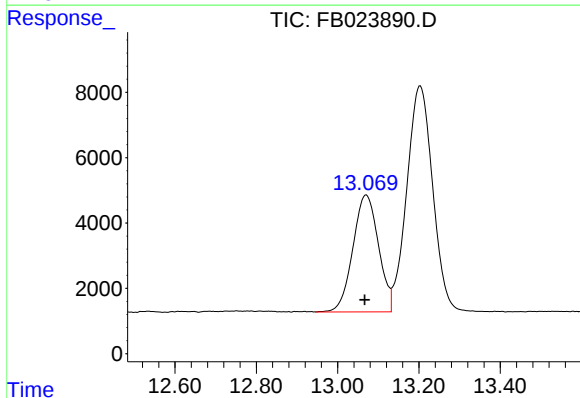


#7 Ethylbenzene

R.T.: 13.070 min
Delta R.T.: 0.004 min
Response: 156084
Conc: 4.09 ng/ml

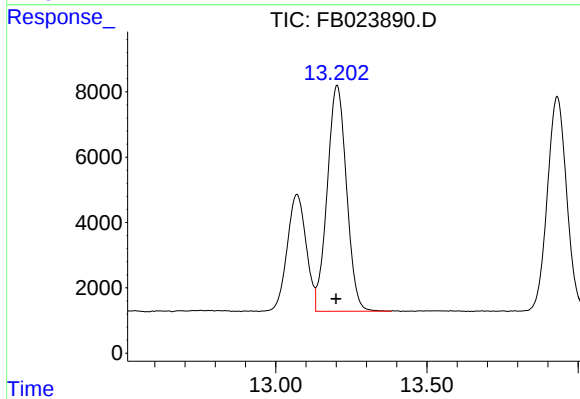


#8 m-Xylene

R.T.: 13.203 min
Delta R.T.: 0.003 min
Response: 306214
Conc: 8.32 ng/ml

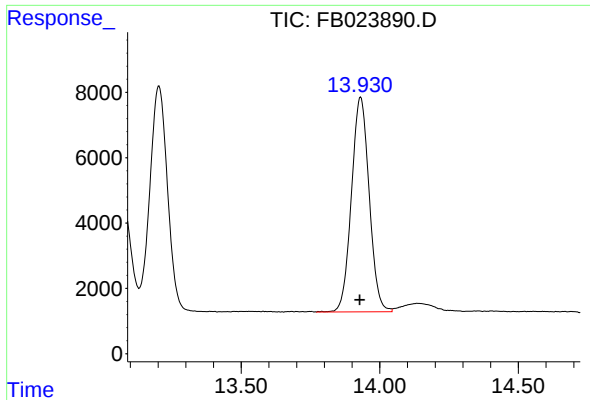

#9 O-Xylene

R.T.: 13.931 min
Delta R.T.: 0.003 min
Response: 292406
Conc: 8.22 ng/ml

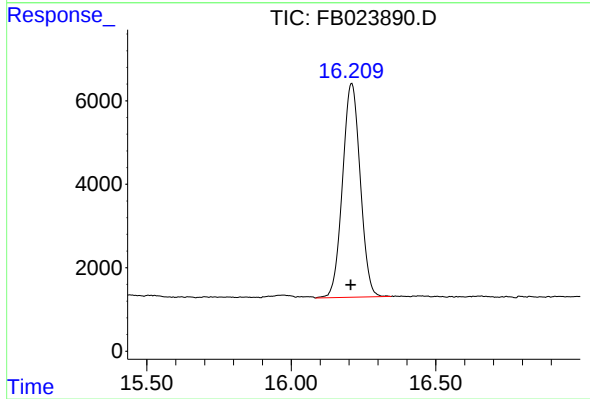

#10 1,2,4-Trimethylbenzene

R.T.: 16.209 min
Delta R.T.: 0.003 min
Response: 217162
Conc: 7.17 ng/ml