

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB031225\
Data File : FB031591.D
Signal(s) : FID2B.CH
Acq On : 12 Mar 2025 14:03
Operator : YP/AJ
Sample : VBF0312S1
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Mar 13 01:17:35 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030625.M
Quant Title :
QLast Update : Thu Mar 06 13:17:04 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.792	437261	19.310 ng/ml
Target Compounds			
6) t Toluene	10.613	8610	0.218 ng/ml
8) t m-Xylene	13.192	10598	0.275 ng/ml
9) t O-Xylene	13.921	10841	0.294 ng/ml
10) t 1,2,4-Trimethylbenzene	16.197	18273	0.647 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB031225\
Data File : FB031591.D
Signal(s) : FID2B.CH
Acq On : 12 Mar 2025 14:03
Operator : YP/AJ
Sample : VBF0312S1
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Mar 13 01:17:35 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030625.M
Quant Title :
QLast Update : Thu Mar 06 13:17:04 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

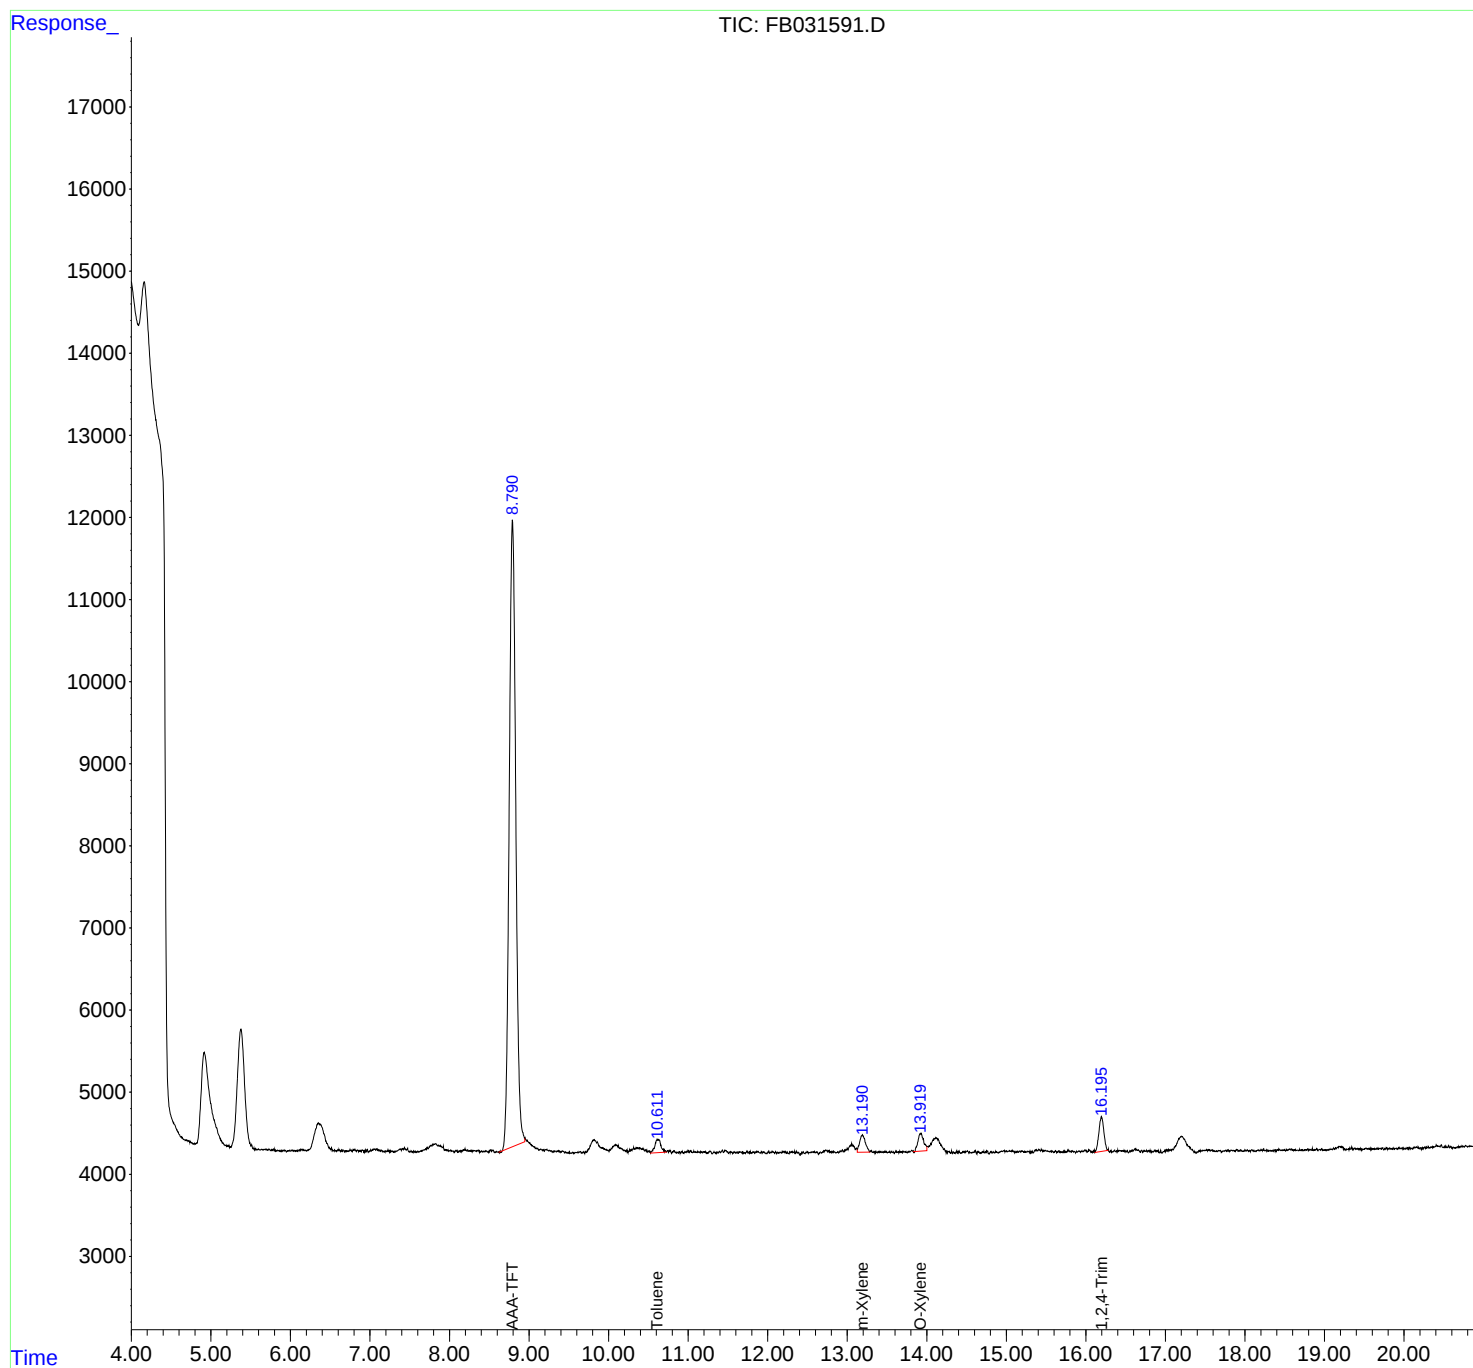


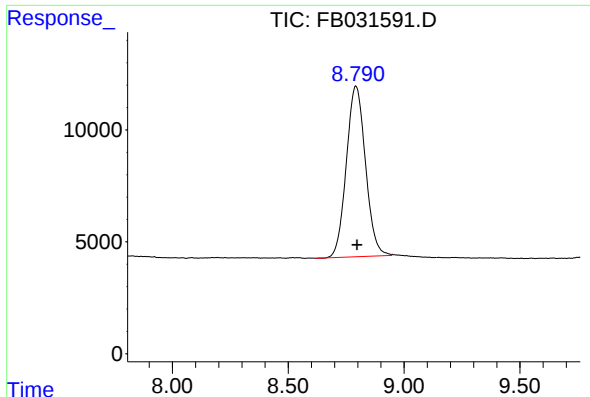

#5 AAA-TFT


R.T.: 8.792 min
Delta R.T.: -0.005 min
Response: 437261
Conc: 19.31 ng/ml

Instrument :
FID_B
ClientSampleId :

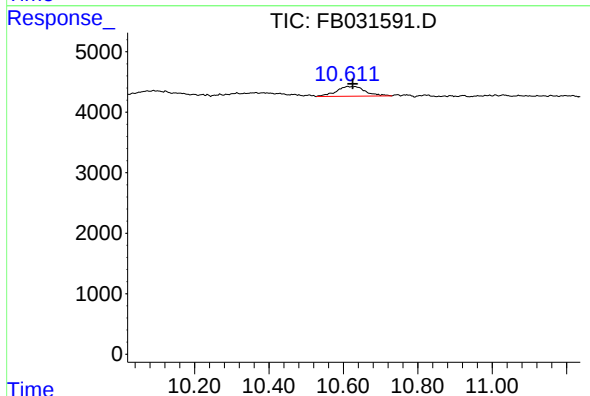


#6 Toluene

R.T.: 10.613 min
Delta R.T.: -0.013 min
Response: 8610
Conc: 0.22 ng/ml

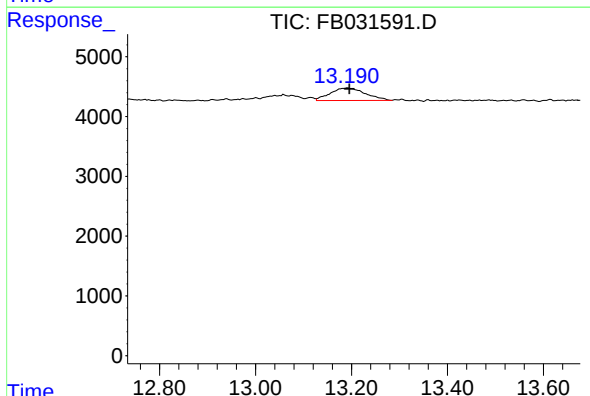


#8 m-Xylene

R.T.: 13.192 min
Delta R.T.: -0.004 min
Response: 10598
Conc: 0.27 ng/ml

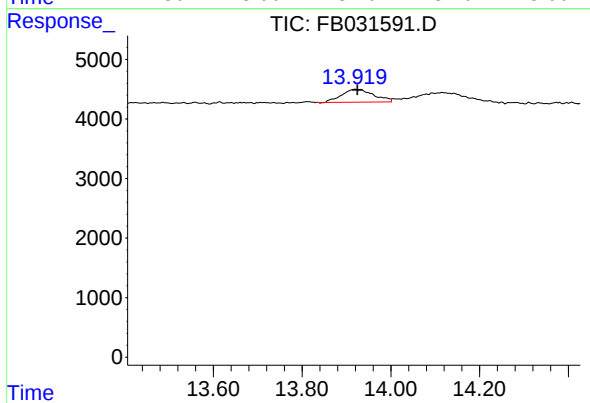

#9 O-Xylene

R.T.: 13.921 min
Delta R.T.: -0.004 min
Response: 10841
Conc: 0.29 ng/ml

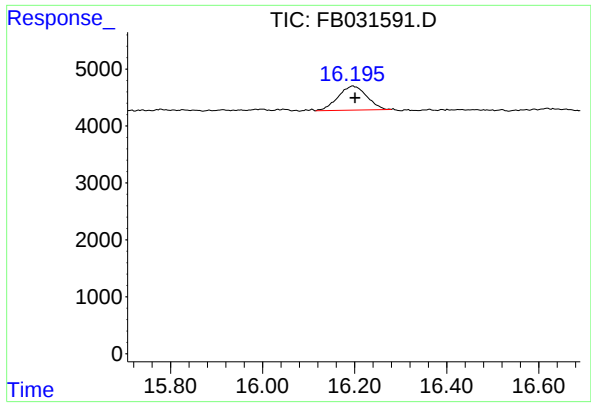

#10 1,2,4-Trimethylbenzene

R.T.: 16.197 min
Delta R.T.: -0.004 min
Response: 18273
Conc: 0.65 ng/ml

Instrument :
FID_B
ClientSampleId :