

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB031319\
 Data File : FB020180.D
 Signal(s) : FID2B.CH
 Acq On : 13 Mar 2019 10:07
 Operator : MJ/SJ
 Sample : K6193-05
 Misc : 5.04g/5.00ml DI WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 OR-02-031219-A

Integration File: Calibration.e
 Quant Time: Mar 14 01:52:09 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB031119.M
 Quant Title :
 QLast Update : Mon Mar 11 13:44:46 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.039	477929	18.205 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.894	5095	0.151 ng/ml
2) t 2,2,4-Trimethylpentane	7.659	22233	0.678 ng/ml
3) t n-Heptane	8.002	3983	0.096 ng/ml
6) t Toluene	10.888	28395	0.768 ng/ml
8) t m-Xylene	13.478	7041	0.330 ng/ml
9) t O-Xylene	14.218	5280	0.279 ng/ml
10) t 1,2,4-Trimethylbenzene	16.493	12796	0.645 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB031319\
Data File : FB020180.D
Signal(s) : FID2B.CH
Acq On : 13 Mar 2019 10:07
Operator : MJ/SJ
Sample : K6193-05
Misc : 5.04g/5.00ml DI WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
OR-02-031219-A

Integration File: Calibration.e
Quant Time: Mar 14 01:52:09 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB031119.M
Quant Title :
QLast Update : Mon Mar 11 13:44:46 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

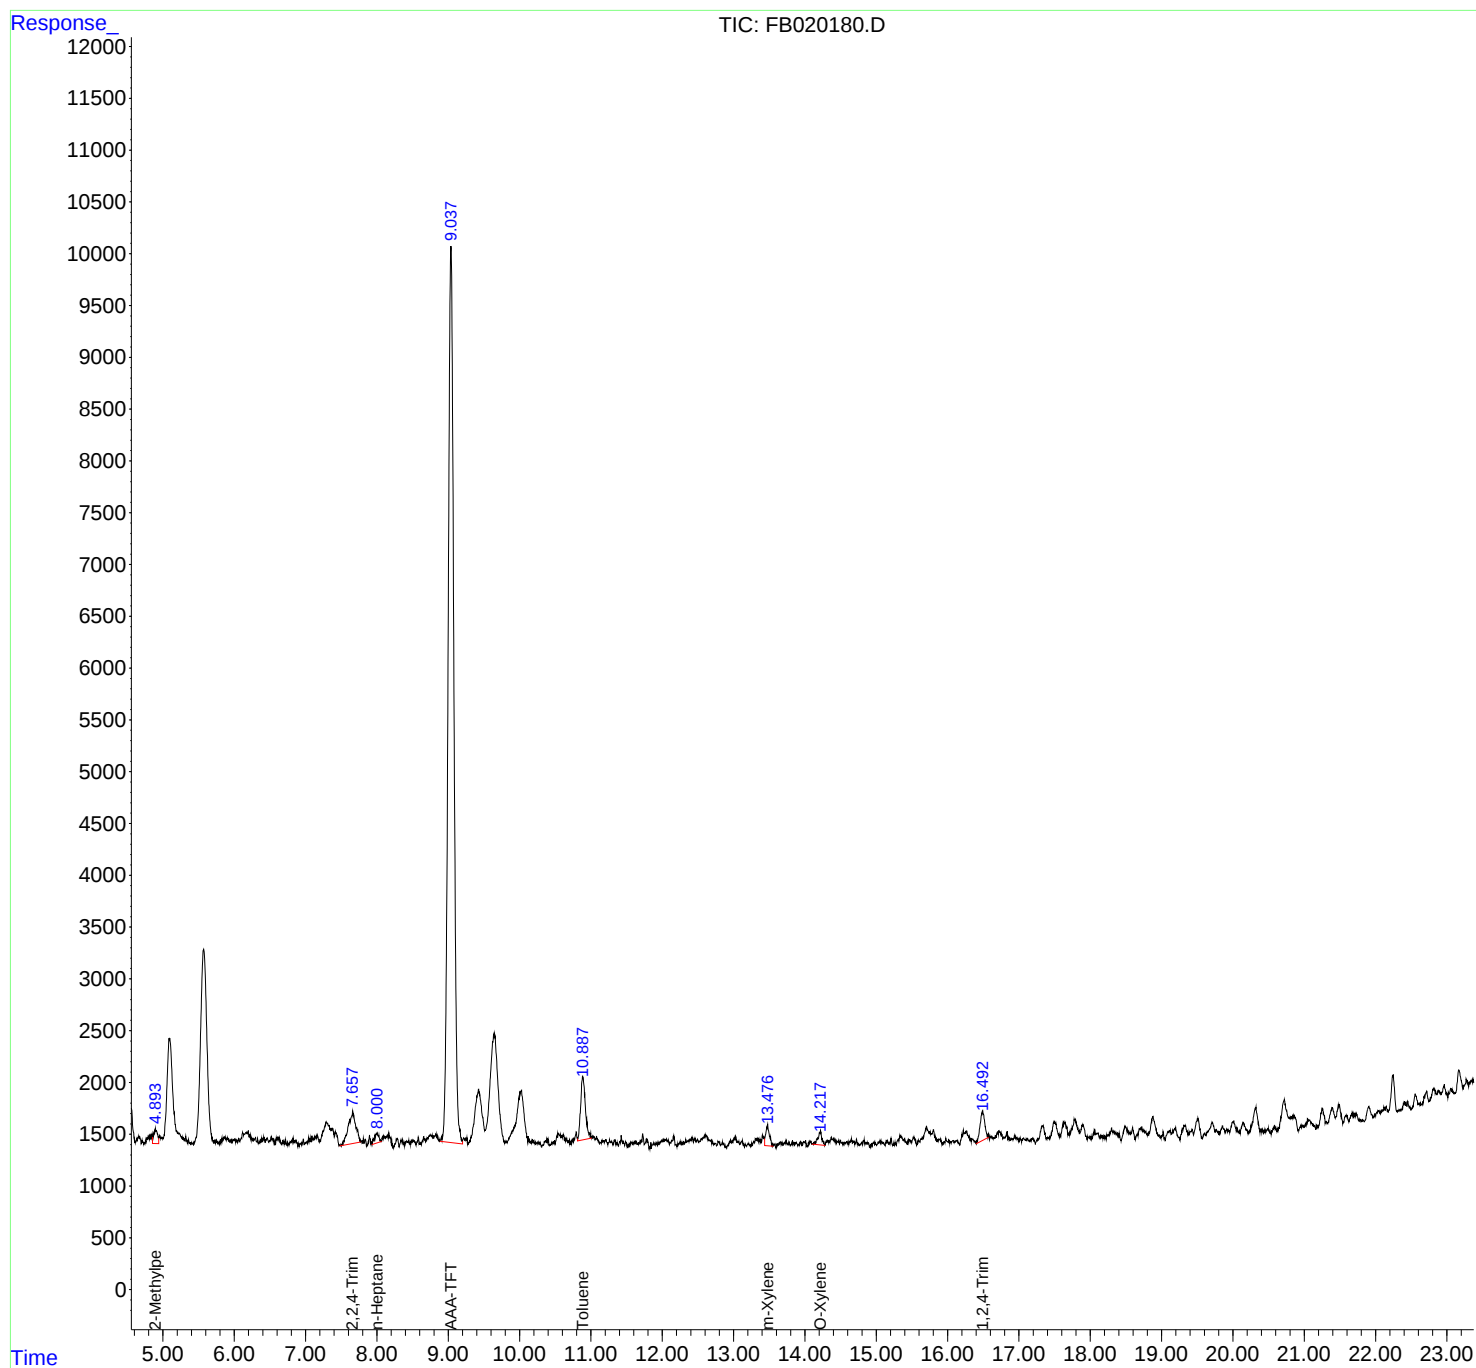


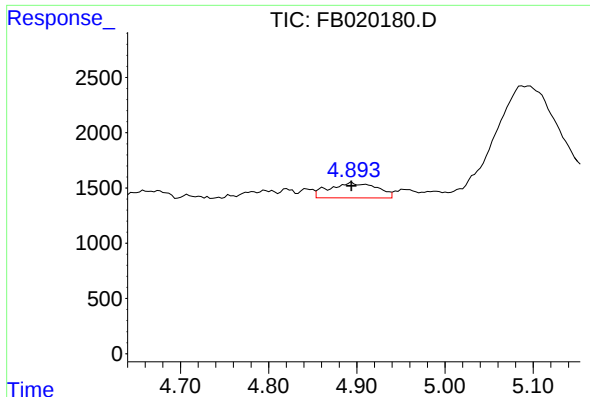

#1 2-Methylpentane


R.T.: 4.894 min
Delta R.T.: 0.000 min
Response: 5095
Conc: 0.15 ng/ml

Instrument :
FID_B
ClientSampleId :
OR-02-031219-A

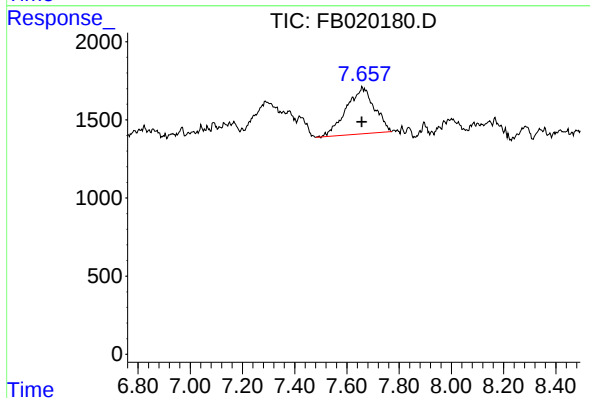


#2 2,2,4-Trimethylpentane

R.T.: 7.659 min
Delta R.T.: 0.002 min
Response: 22233
Conc: 0.68 ng/ml

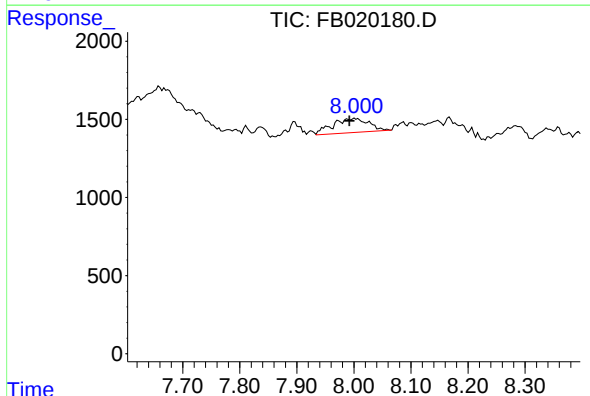


#3 n-Heptane

R.T.: 8.002 min
Delta R.T.: 0.010 min
Response: 3983
Conc: 0.10 ng/ml

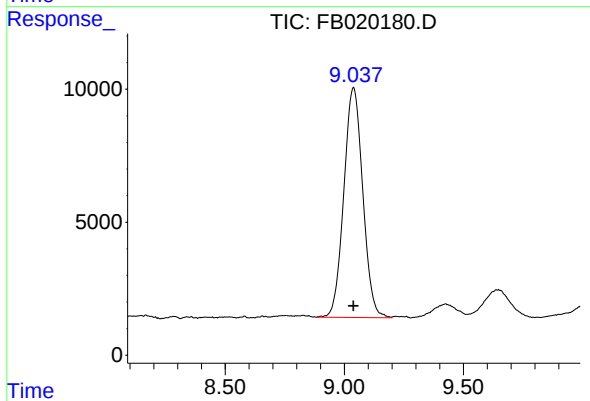

#5 AAA-TFT


R.T.: 9.039 min
Delta R.T.: 0.000 min
Response: 477929
Conc: 18.20 ng/ml

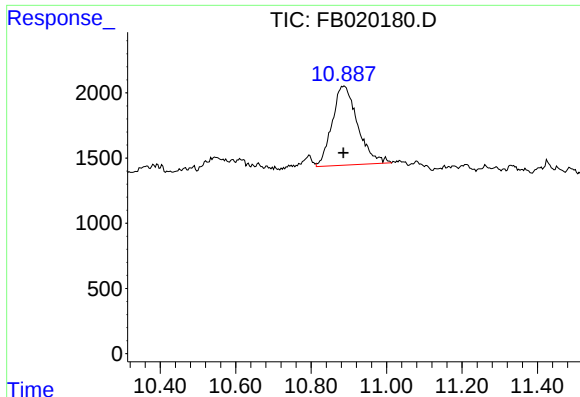

#6 Toluene


R.T.: 10.888 min
Delta R.T.: 0.002 min
Response: 28395
Conc: 0.77 ng/ml

Instrument :
FID_B
ClientSampleId :
OR-02-031219-A

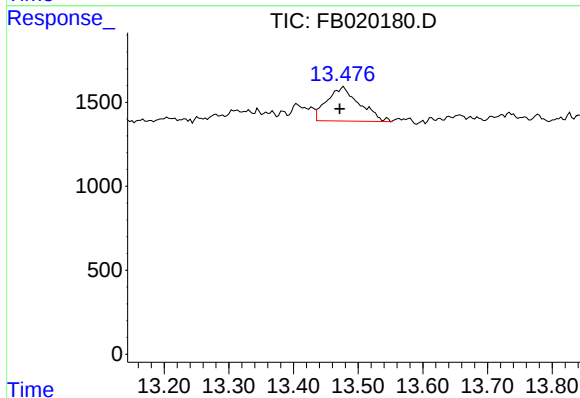


#8 m-Xylene

R.T.: 13.478 min
Delta R.T.: 0.006 min
Response: 7041
Conc: 0.33 ng/ml

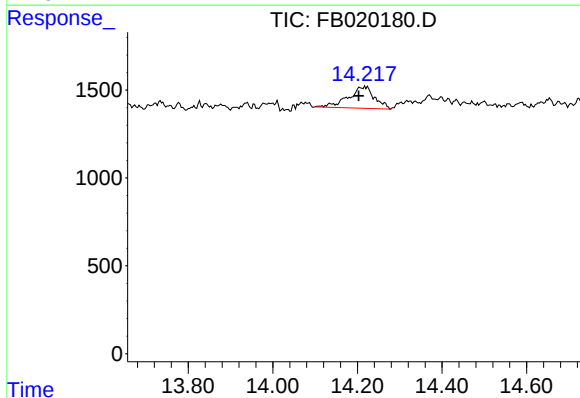

#9 o-Xylene

R.T.: 14.218 min
Delta R.T.: 0.015 min
Response: 5280
Conc: 0.28 ng/ml

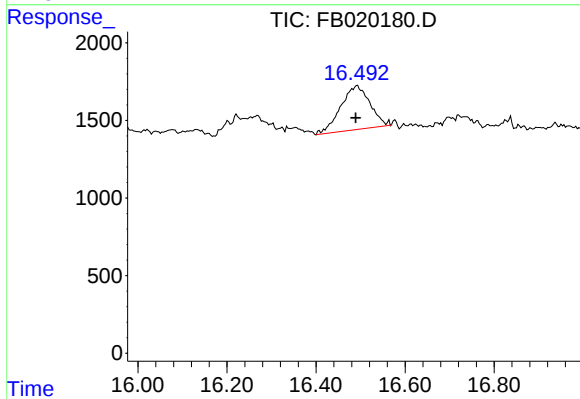

#10 1,2,4-Trimethylbenzene

R.T.: 16.493 min
Delta R.T.: 0.003 min
Response: 12796
Conc: 0.65 ng/ml