

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB031319\
 Data File : FB020186.D
 Signal(s) : FID2B.CH
 Acq On : 13 Mar 2019 13:52
 Operator : MJ/SJ
 Sample : K1693-07MS
 Misc : 5.02g/5.00ml DI WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 OR-02-031219-BMS

Integration File: Calibration.e
 Quant Time: Mar 14 01:53:23 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB031119.M
 Quant Title :
 QLast Update : Mon Mar 11 13:44:46 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.040	473777	18.047 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.898	829363	24.586 ng/ml
2) t 2,2,4-Trimethylpentane	7.665	677748	20.667 ng/ml
3) t n-Heptane	7.995	312302	7.504 ng/ml
4) t Benzene	8.132	407176	8.746 ng/ml
6) t Toluene	10.887	910664	24.644 ng/ml
7) t Ethylbenzene	13.339	194818	8.280 ng/ml
8) t m-Xylene	13.473	378070	17.723 ng/ml
9) t O-Xylene	14.205	364347	19.234 ng/ml
10) t 1,2,4-Trimethylbenzene	16.490	376150	18.967 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB031319\
Data File : FB020186.D
Signal(s) : FID2B.CH
Acq On : 13 Mar 2019 13:52
Operator : MJ/SJ
Sample : K1693-07MS
Misc : 5.02g/5.00ml DI WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
OR-02-031219-BMS

Integration File: Calibration.e
Quant Time: Mar 14 01:53:23 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB031119.M
Quant Title :
QLast Update : Mon Mar 11 13:44:46 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

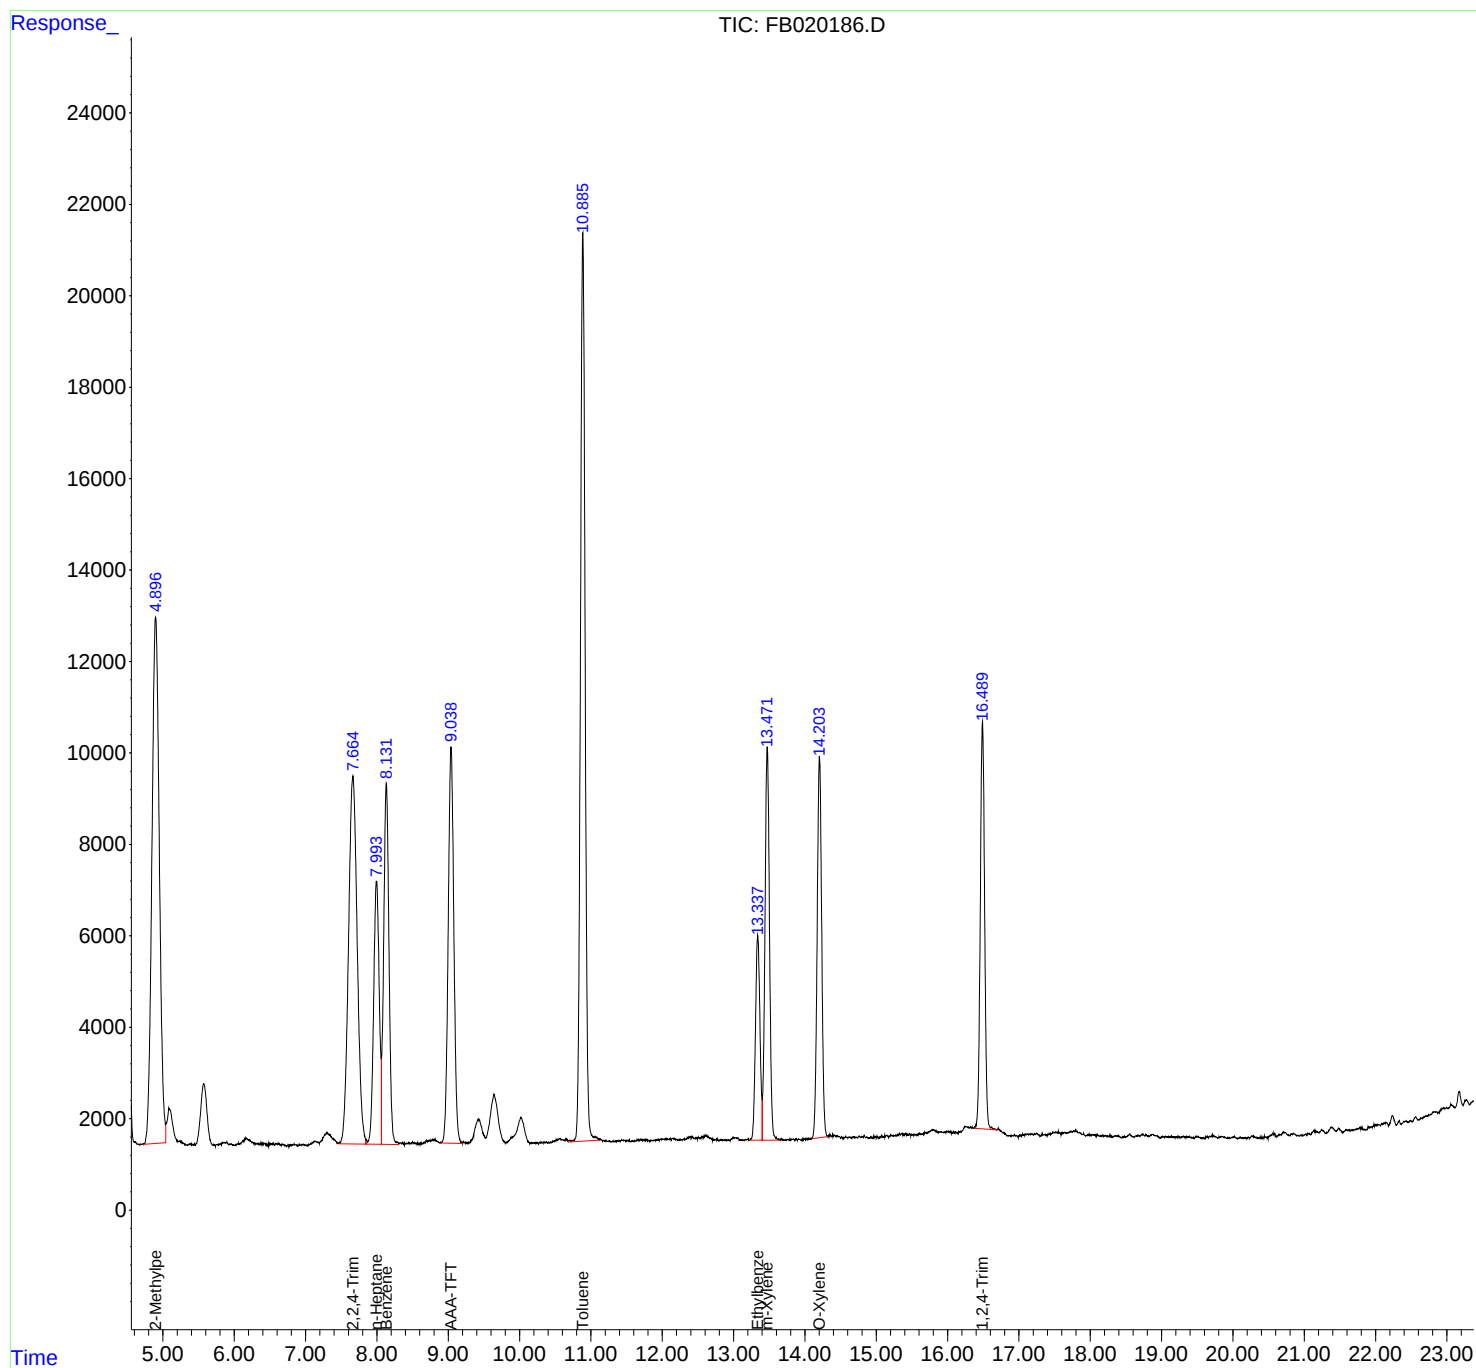


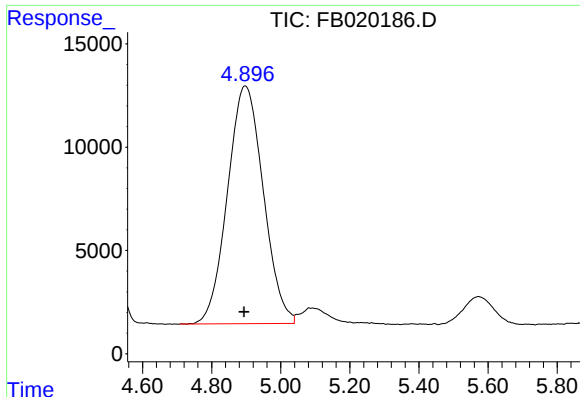

#1 2-Methylpentane


R.T.: 4.898 min
Delta R.T.: 0.004 min
Response: 829363
Conc: 24.59 ng/ml

Instrument :
FID_B
ClientSampleId :
OR-02-031219-BMS

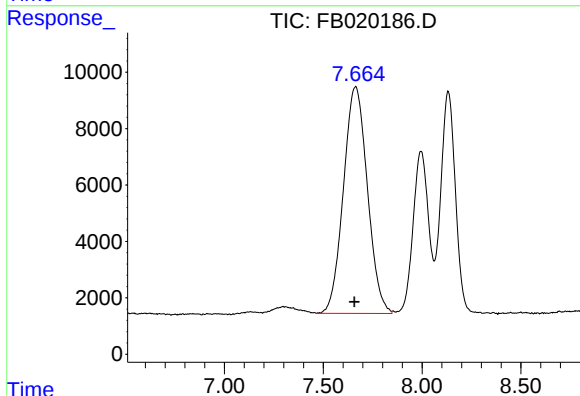


#2 2,2,4-Trimethylpentane

R.T.: 7.665 min
Delta R.T.: 0.008 min
Response: 677748
Conc: 20.67 ng/ml

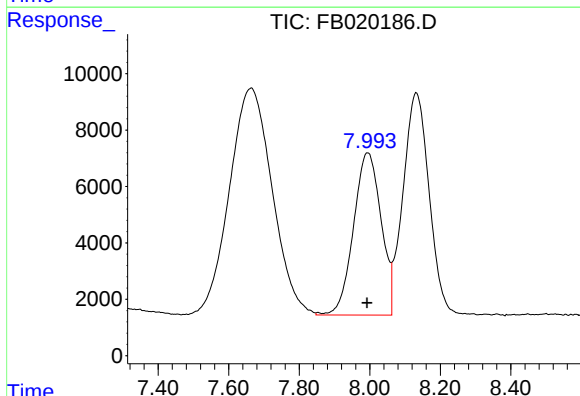


#3 n-Heptane

R.T.: 7.995 min
Delta R.T.: 0.002 min
Response: 312302
Conc: 7.50 ng/ml

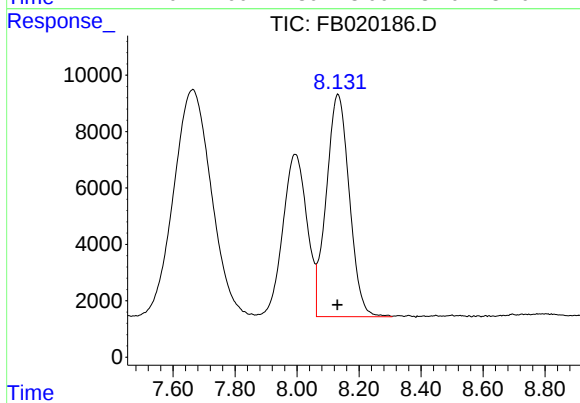

#4 Benzene


R.T.: 8.132 min
Delta R.T.: 0.002 min
Response: 407176
Conc: 8.75 ng/ml

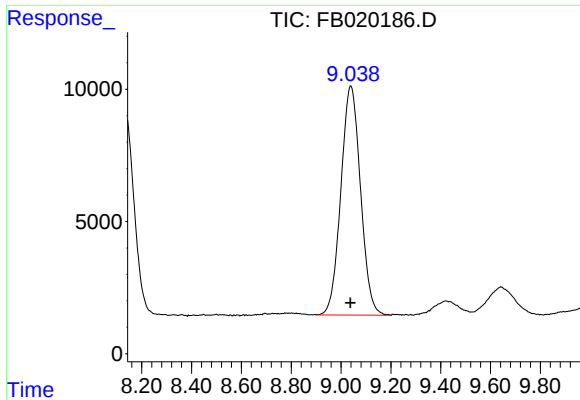

#5 AAA-TFT


R.T.: 9.040 min
 Delta R.T.: 0.002 min
 Response: 473777
 Conc: 18.05 ng/ml

Instrument :
 FID_B
 ClientSampleId :
 OR-02-031219-BMS

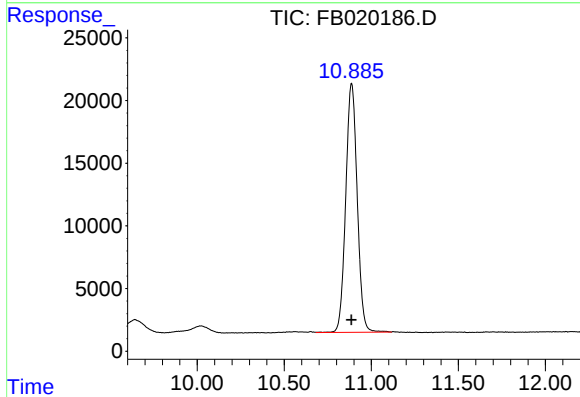


#6 Toluene

R.T.: 10.887 min
 Delta R.T.: 0.002 min
 Response: 910664
 Conc: 24.64 ng/ml

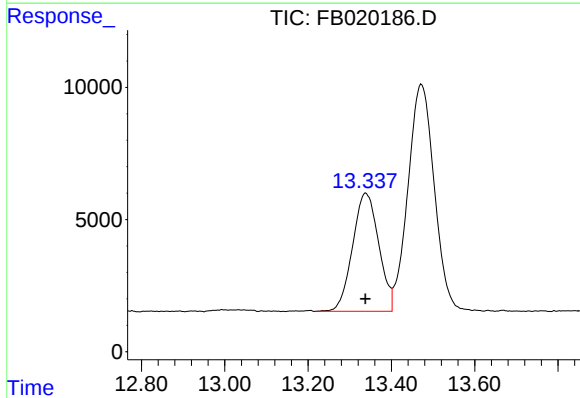


#7 Ethylbenzene

R.T.: 13.339 min
 Delta R.T.: 0.001 min
 Response: 194818
 Conc: 8.28 ng/ml

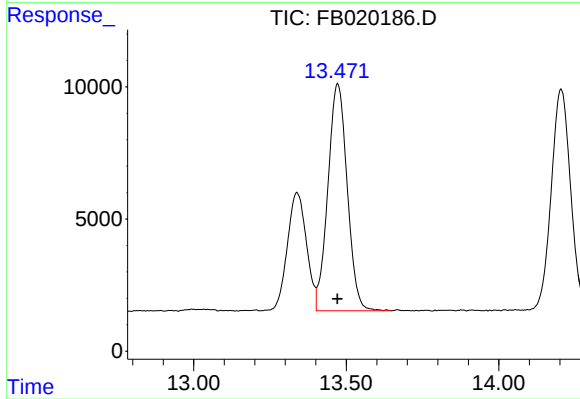

#8 m-Xylene


R.T.: 13.473 min
 Delta R.T.: 0.001 min
 Response: 378070
 Conc: 17.72 ng/ml

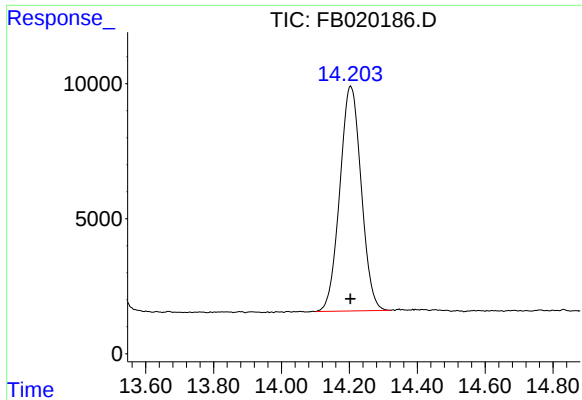

#9 O-Xylene

R.T.: 14.205 min
Delta R.T.: 0.001 min
Response: 364347
Conc: 19.23 ng/ml

Instrument :
FID_B
ClientSampleId :
OR-02-031219-BMS

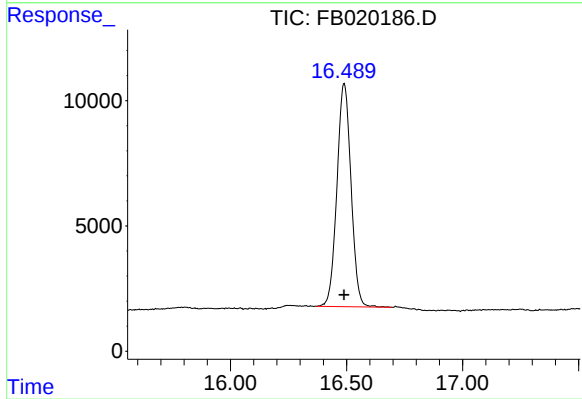

#10 1,2,4-Trimethylbenzene

R.T.: 16.490 min
Delta R.T.: 0.000 min
Response: 376150
Conc: 18.97 ng/ml