

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB031319\
 Data File : FB020187.D
 Signal(s) : FID2B.CH
 Acq On : 13 Mar 2019 14:22
 Operator : MJ/SJ
 Sample : K1693-07MSD
 Misc : 5.04g/5.00ml DI WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 OR-02-031219-BMSD

Integration File: Calibration.e
 Quant Time: Mar 14 01:53:39 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB031119.M
 Quant Title :
 QLast Update : Mon Mar 11 13:44:46 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.040	463920	17.671 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.898	789114	23.393 ng/ml
2) t 2,2,4-Trimethylpentane	7.664	632558	19.289 ng/ml
3) t n-Heptane	7.996	291808	7.012 ng/ml
4) t Benzene	8.133	390307	8.383 ng/ml
6) t Toluene	10.887	885843	23.972 ng/ml
7) t Ethylbenzene	13.340	190812	8.110 ng/ml
8) t m-Xylene	13.473	368124	17.257 ng/ml
9) t O-Xylene	14.205	353541	18.663 ng/ml
10) t 1,2,4-Trimethylbenzene	16.491	357821	18.043 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB031319\
Data File : FB020187.D
Signal(s) : FID2B.CH
Acq On : 13 Mar 2019 14:22
Operator : MJ/SJ
Sample : K1693-07MSD
Misc : 5.04g/5.00ml DI WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
OR-02-031219-BMSD

Integration File: Calibration.e
Quant Time: Mar 14 01:53:39 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB031119.M
Quant Title :
QLast Update : Mon Mar 11 13:44:46 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

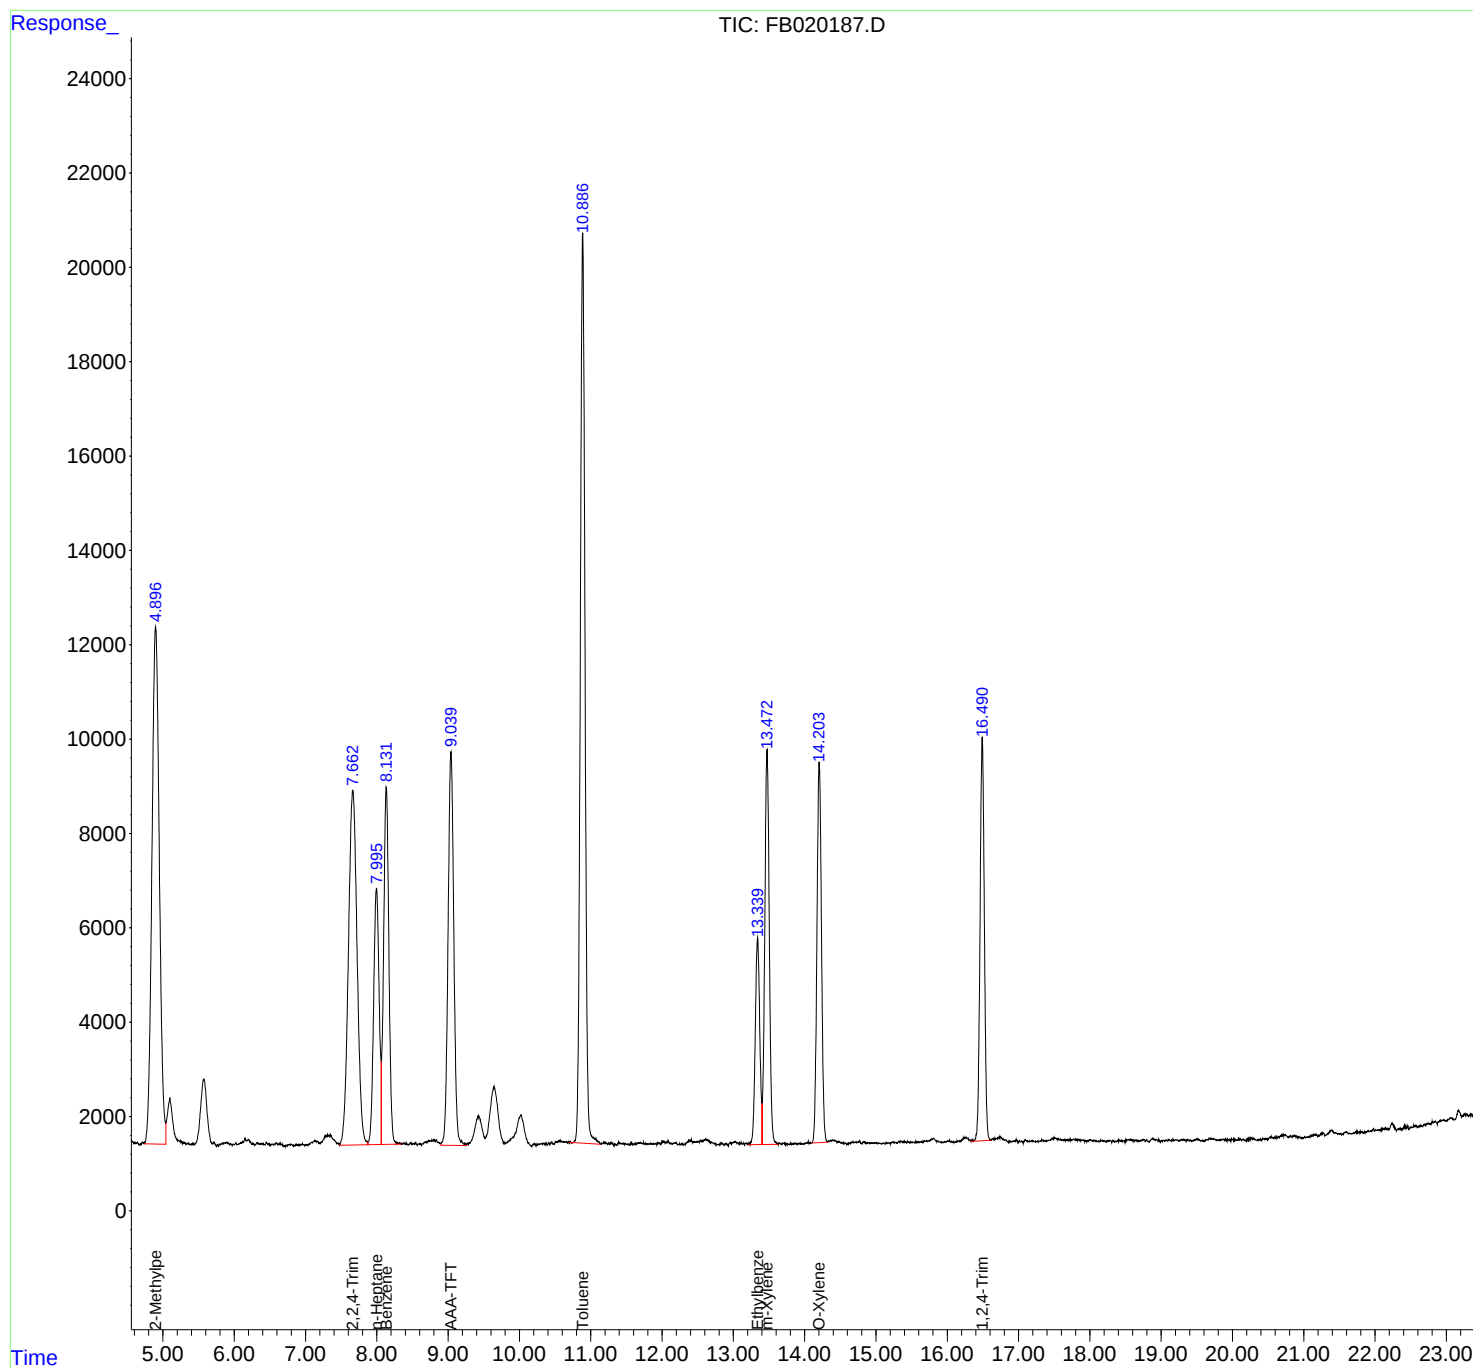


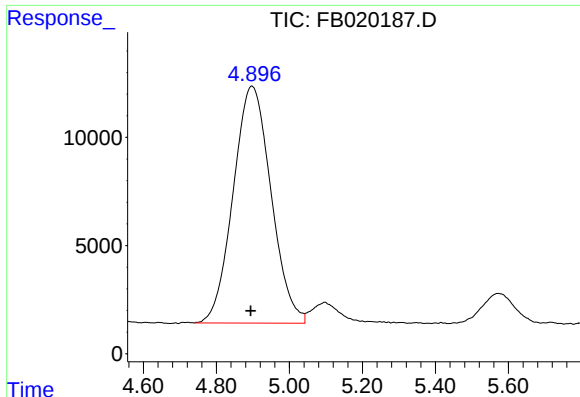

#1 2-Methylpentane


R.T.: 4.898 min
Delta R.T.: 0.004 min
Response: 789114
Conc: 23.39 ng/ml

Instrument :
FID_B
ClientSampleId :
OR-02-031219-BMSD

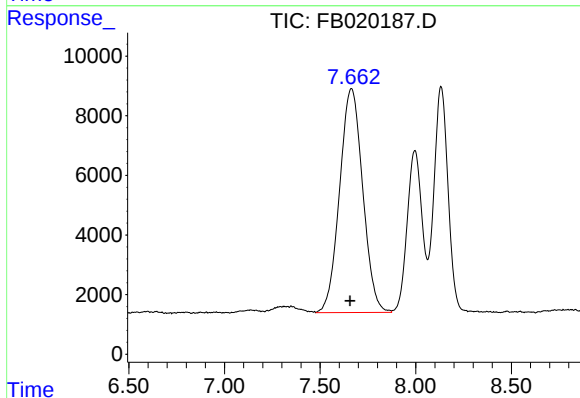


#2 2,2,4-Trimethylpentane

R.T.: 7.664 min
Delta R.T.: 0.006 min
Response: 632558
Conc: 19.29 ng/ml

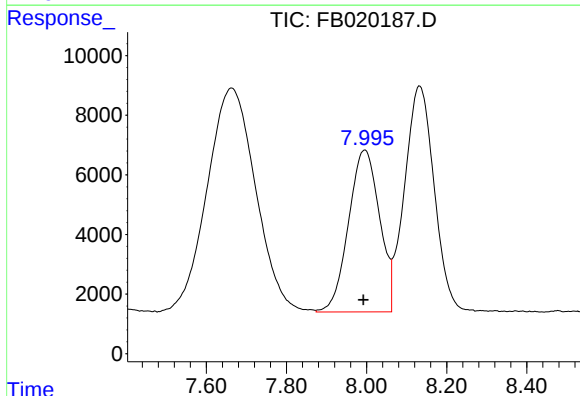


#3 n-Heptane

R.T.: 7.996 min
Delta R.T.: 0.003 min
Response: 291808
Conc: 7.01 ng/ml

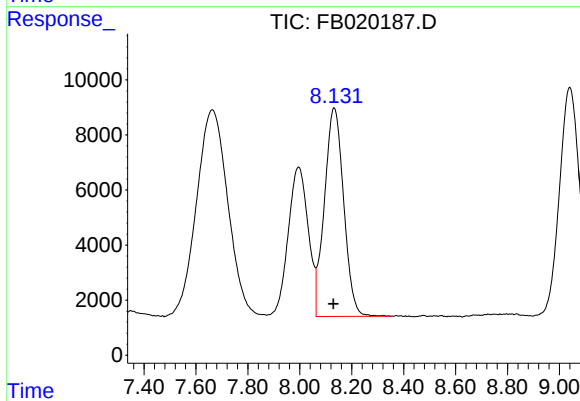


#4 Benzene

R.T.: 8.133 min
Delta R.T.: 0.003 min
Response: 390307
Conc: 8.38 ng/ml

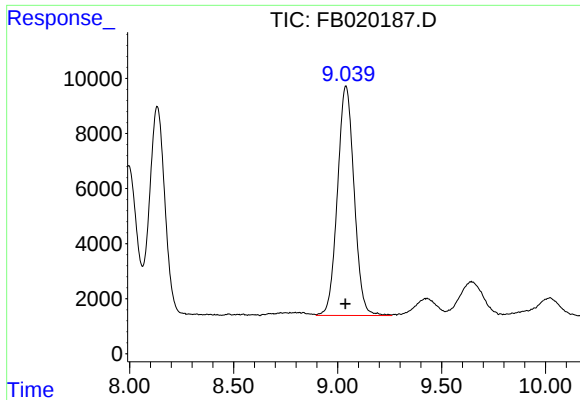


#5 AAA-TFT
 R.T.: 9.040 min
 Delta R.T.: 0.002 min
 Response: 463920
 Conc: 17.67 ng/ml


Instrument :
 FID_B
 ClientSampleId :
 OR-02-031219-BMSD

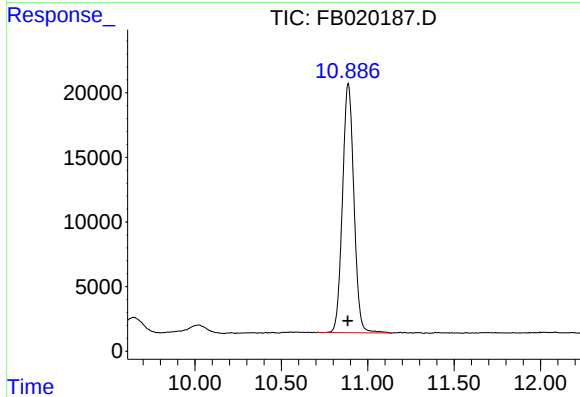


#6 Toluene
 R.T.: 10.887 min
 Delta R.T.: 0.002 min
 Response: 885843
 Conc: 23.97 ng/ml

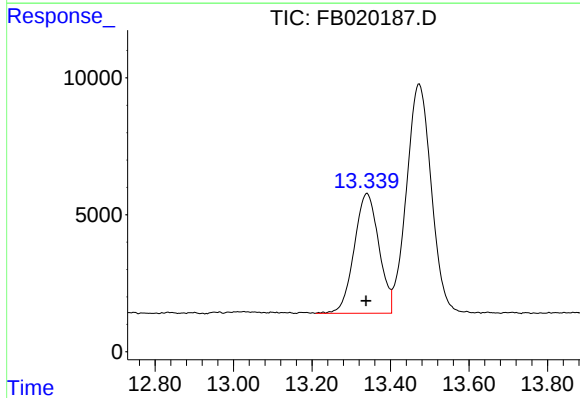

#7 Ethylbenzene
 R.T.: 13.340 min
 Delta R.T.: 0.003 min
 Response: 190812
 Conc: 8.11 ng/ml

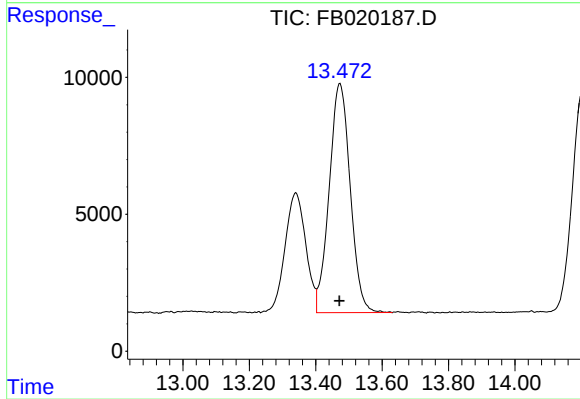


#8 m-Xylene
 R.T.: 13.473 min
 Delta R.T.: 0.002 min
 Response: 368124
 Conc: 17.26 ng/ml

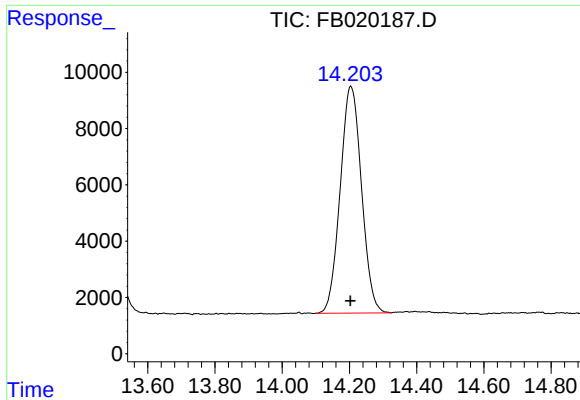

#9 O-Xylene

R.T.: 14.205 min
Delta R.T.: 0.002 min
Response: 353541
Conc: 18.66 ng/ml

Instrument :
FID_B
ClientSampleId :
OR-02-031219-BMSD

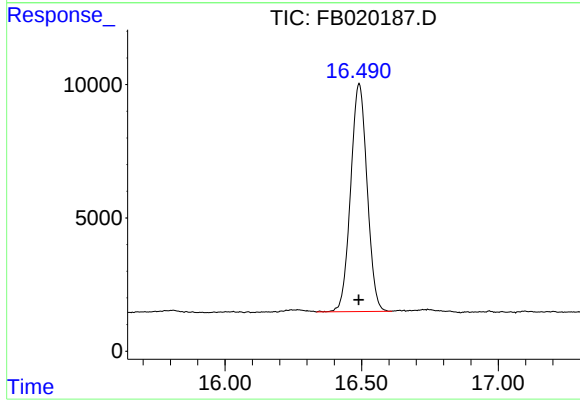

#10 1,2,4-Trimethylbenzene

R.T.: 16.491 min
Delta R.T.: 0.002 min
Response: 357821
Conc: 18.04 ng/ml