

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB031319\
Data File : FB020178.D
Signal(s) : FID2B.CH
Acq On : 13 Mar 2019 9:07
Operator : MJ/SJ
Sample : VBF0313S1
Misc : 5.02g/5.00ml DI WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
VBF0313S1

Integration File: Calibration.e
Quant Time: Mar 14 01:51:49 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB031119.M
Quant Title :
QLast Update : Mon Mar 11 13:44:46 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.037	476879	18.165 ng/ml
Target Compounds			

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB031319\
Data File : FB020178.D
Signal(s) : FID2B.CH
Acq On : 13 Mar 2019 9:07
Operator : MJ/SJ
Sample : VBF0313S1
Misc : 5.02g/5.00ml DI WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
VBF0313S1

Integration File: Calibration.e
Quant Time: Mar 14 01:51:49 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB031119.M
Quant Title :
QLast Update : Mon Mar 11 13:44:46 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

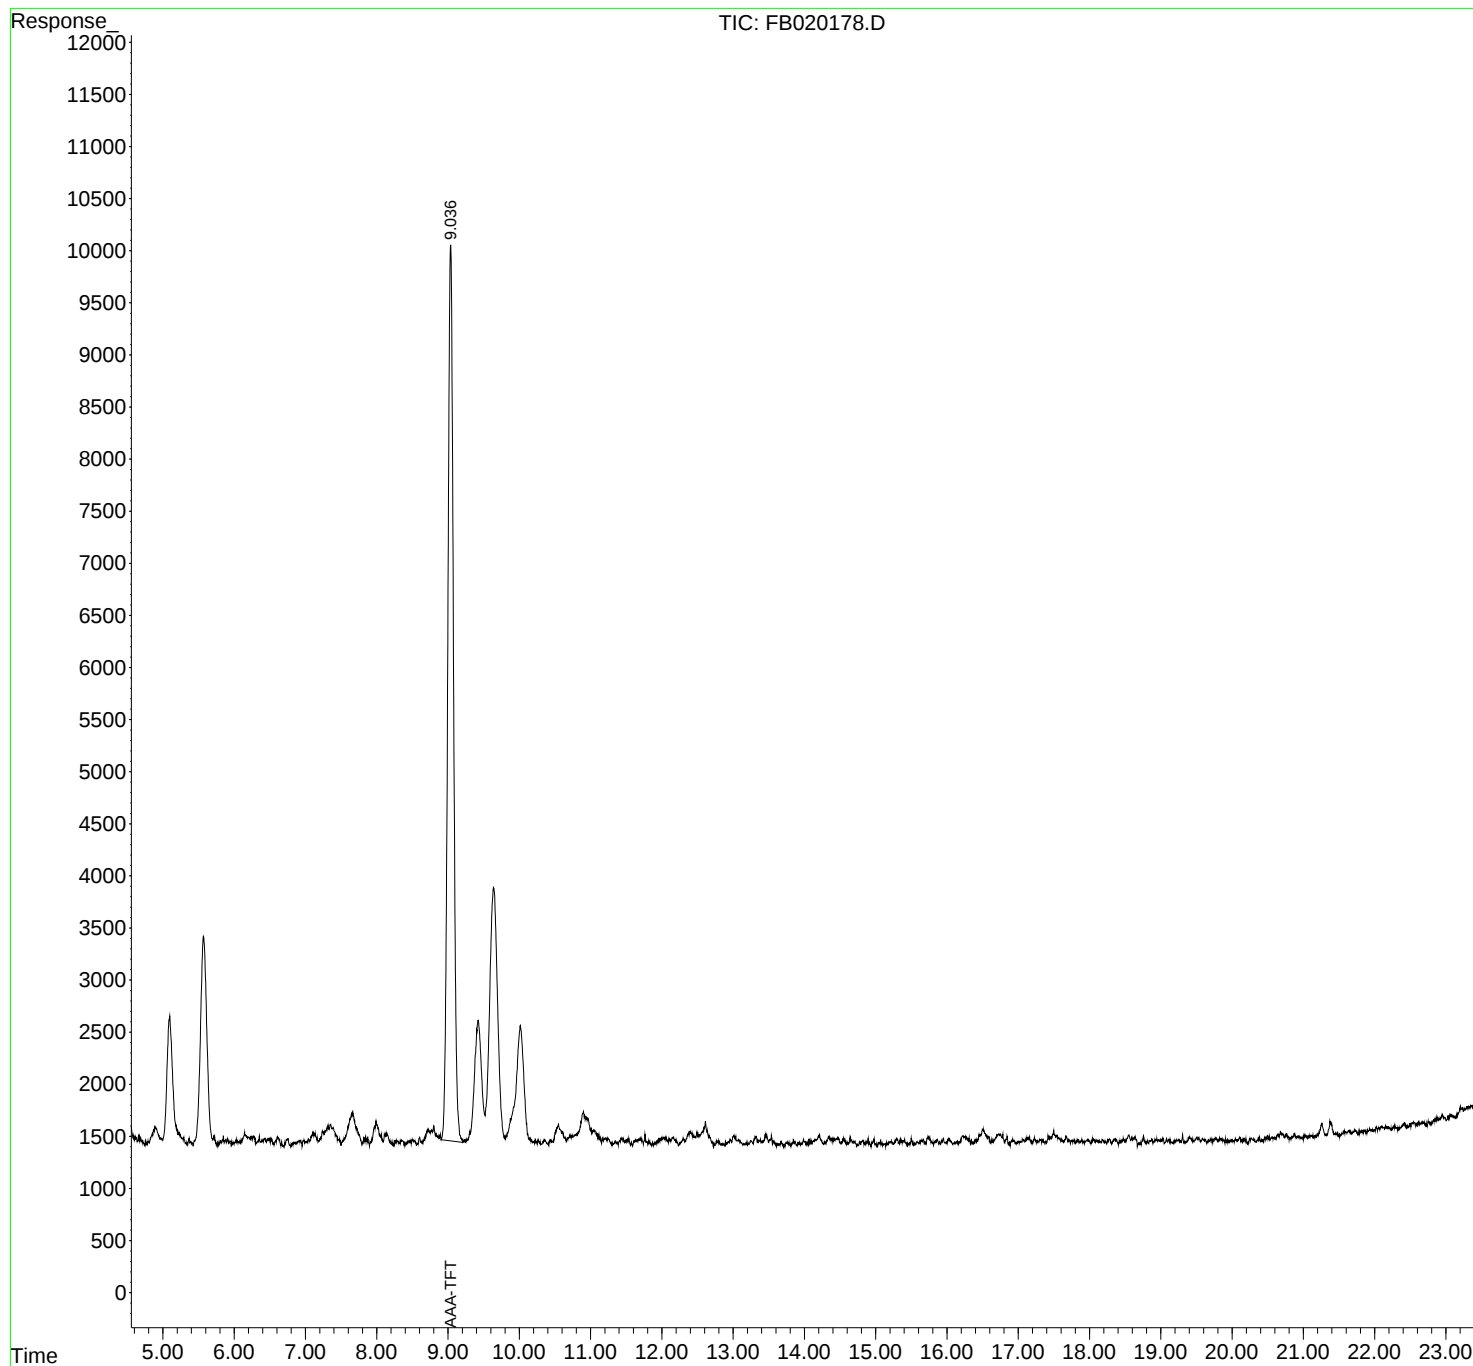

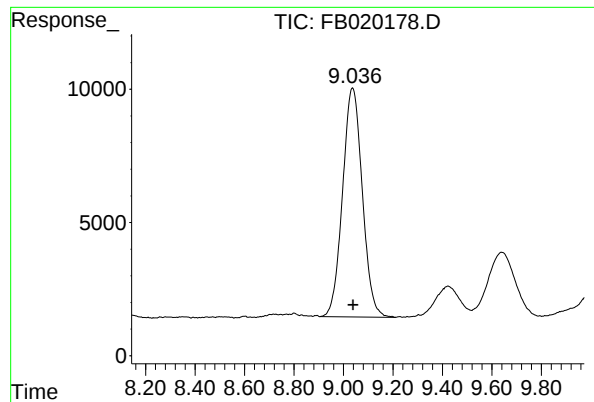

#5 AAA-TFT

R.T.: 9.037 min
Delta R.T.: 0.000 min
Response: 476879
Conc: 18.16 ng/ml

Instrument :
FID_B
ClientSampleId :
VBF0313S1

rteres

Area Percent Report

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB031319\
Data File : FB020178.D
Signal(s) : FID2B.CH
Acq On : 13 Mar 2019 9:07
Sample : VBF0313S1
Misc : 5.02g/5.00ml DI WATER
ALS Vial : 2 Sample Multiplier: 1

Integration File: Calibration.e

Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB031119.M
Title :

Signal : FID2B.CH

peak #	R.T. min	Start min	End min	PK TY	peak height	peak area	peak % max.	% of total
1	4.892	4.779	4.963	PV	135	6866	1.44%	0.582%
2	5.096	4.996	5.286	BV	1199	68393	14.34%	5.802%
3	5.570	5.425	5.702	PV	1980	121080	25.39%	10.271%
4	6.147	6.090	6.224	PV	106	4522	0.95%	0.384%
5	7.108	7.054	7.118	PV	85	1749	0.37%	0.148%
6	7.322	7.284	7.332	VV	139	3386	0.71%	0.287%
7	7.353	7.332	7.460	VB	159	6948	1.46%	0.589%
8	7.654	7.468	7.792	BV	279	20049	4.20%	1.701%
9	7.991	7.872	8.060	BV	169	5248	1.10%	0.445%
10	8.718	8.648	8.738	PV	102	3118	0.65%	0.264%
11	8.801	8.738	8.824	VV	105	3413	0.72%	0.290%
12	9.037	8.905	9.210	PV	8597	476879	100.00%	40.452%
13	9.424	9.239	9.519	VV	1178	82067	17.21%	6.961%
14	9.640	9.519	9.804	VV	2453	190414	39.93%	16.152%
15	10.015	9.804	10.254	VV	1135	94483	19.81%	8.015%
16	10.548	10.413	10.666	PV	199	14599	3.06%	1.238%
17	10.899	10.666	11.022	VV	320	34246	7.18%	2.905%
18	11.057	11.022	11.156	VV	142	8082	1.69%	0.686%
19	11.765	11.741	11.855	VB	103	2198	0.46%	0.186%
20	12.396	12.331	12.478	VV	115	7032	1.47%	0.597%
21	12.493	12.478	12.517	VV	118	2160	0.45%	0.183%
22	12.612	12.517	12.723	VV	228	13022	2.73%	1.105%
23	16.501	16.366	16.608	BV	132	8924	1.87%	0.757%
Sum of corrected areas:						1178881		

FB031119.M Thu Mar 14 02:08:09 2019