

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB031319\
Data File : FB020182.D
Signal(s) : FID2B.CH
Acq On : 13 Mar 2019 11:08
Operator : MJ/SJ
Sample : K1871-02
Misc : 5.03g/5.00ml DI WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
TP-1-A

Manual Integrations
APPROVED

Sohil
3/15/2019 9:52:43 AM

Integration File: Calibration.e
Quant Time: Mar 14 01:52:32 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB031119.M
Quant Title :
QLast Update : Mon Mar 11 13:44:46 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.040	421368	16.050 ng/mlm
Target Compounds			

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB031319\
Data File : FB020182.D
Signal(s) : FID2B.CH
Acq On : 13 Mar 2019 11:08
Operator : MJ/SJ
Sample : K1871-02
Misc : 5.03g/5.00ml DI WATER
ALS Vial : 6 Sample Multiplier: 1


Instrument :
FID_B
ClientSampleId :
TP-1-A


Manual Integrations
APPROVED

Sohil
3/15/2019 9:52:43 AM

Integration File: Calibration.e
Quant Time: Mar 14 01:52:32 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB031119.M
Quant Title :
QLast Update : Mon Mar 11 13:44:46 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

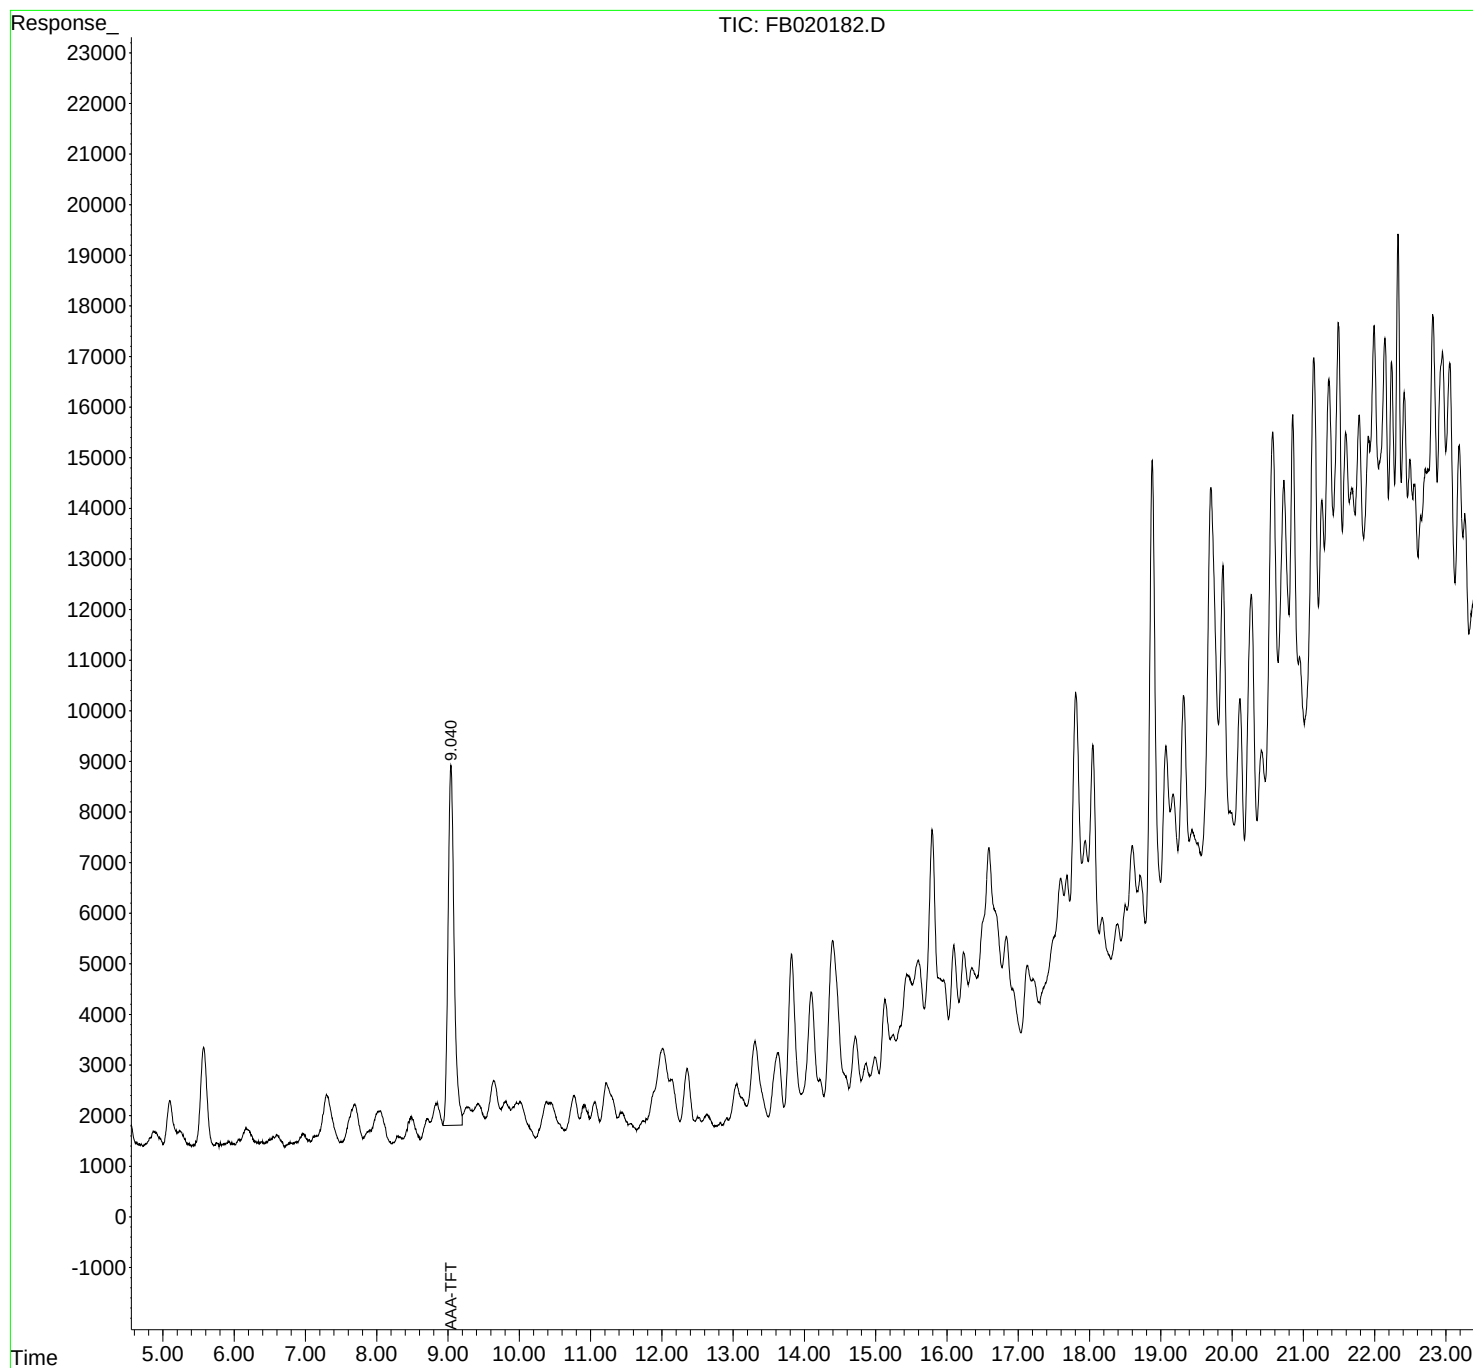

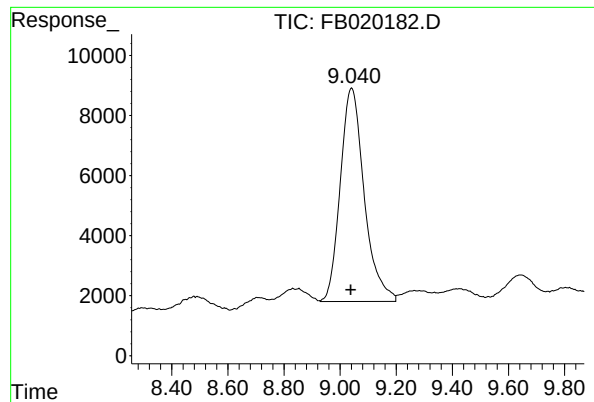

#5 AAA-TFT

R.T.: 9.040 min
Delta R.T.: 0.002 min
Response: 421368
Conc: 16.05 ng/ml m

Instrument :
FID_B
ClientSampleId :
TP-1-A

Manual Integrations
APPROVED

Sohil
3/15/2019 9:52:43 AM

Instrument :
FID_B
ClientSampleId :
TP-1-A

rteres

Area Percent Report

Manual Integrations
APPROVED

Sohil
3/15/2019 9:52:43 AM

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB031319\
Data File : FB020182.D
Signal(s) : FID2B.CH
Acq On : 13 Mar 2019 11:08
Sample : K1871-02
Misc : 5.03g/5.00ml DI WATER
ALS Vial : 6 Sample Multiplier: 1

Integration File: SAMPLE.e

Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB031119.M
Title :

Signal : FID2B.CH

peak #	R.T. min	Start min	End min	PK TY	peak height	peak area	peak % max.	% of total
1	4.867	4.804	4.879	PH	-3402	-155819	-25.20%	-2.857%
2	4.889	4.879	4.900	PV	-1682	-21586	-3.49%	-0.396%
3	4.908	4.900	5.002	PV	39	1571	0.25%	0.029%
4	5.097	5.002	5.200	PV	882	53214	8.60%	0.976%
5	5.209	5.200	5.217	VV	267	2677	0.43%	0.049%
6	5.232	5.217	5.364	VV	295	15371	2.49%	0.282%
7	5.372	5.364	5.406	VV	63	721	0.12%	0.013%
8	5.428	5.406	5.436	PV	41	413	0.07%	0.008%
9	5.573	5.436	5.716	VV	1962	122892	19.87%	2.253%
10	5.756	5.716	5.788	VV	78	2075	0.34%	0.038%
11	5.807	5.788	5.822	PV	83	838	0.14%	0.015%
12	5.833	5.822	5.842	VV	53	487	0.08%	0.009%
13	5.861	5.842	5.867	VV	58	718	0.12%	0.013%
14	5.928	5.867	5.950	VV	108	3778	0.61%	0.069%
15	5.967	5.950	5.984	VV	88	1274	0.21%	0.023%
16	5.992	5.984	6.019	VV	66	1058	0.17%	0.019%
17	6.060	6.019	6.082	VV	149	4038	0.65%	0.074%
18	6.163	6.082	6.277	VV	365	29512	4.77%	0.541%
19	6.282	6.277	6.293	VV	125	993	0.16%	0.018%
20	6.305	6.293	6.319	VV	117	1547	0.25%	0.028%
21	6.327	6.319	6.333	VV	94	705	0.11%	0.013%
22	6.341	6.333	6.355	VV	111	1024	0.17%	0.019%
23	6.383	6.355	6.409	VV	100	2826	0.46%	0.052%
24	6.418	6.409	6.426	VV	79	647	0.10%	0.012%
25	6.498	6.426	6.506	VV	142	4867	0.79%	0.089%
26	6.546	6.506	6.565	VV	199	5989	0.97%	0.110%
27	6.595	6.565	6.713	VV	245	12738	2.06%	0.234%
28	6.730	6.713	6.738	PV	40	326	0.05%	0.006%
29	6.765	6.738	6.780	VV	72	1297	0.21%	0.024%
30	6.789	6.780	6.820	VV	82	1591	0.26%	0.029%
31	6.861	6.820	6.874	VV	93	2446	0.40%	0.045%
32	6.884	6.874	6.895	VV	94	1060	0.17%	0.019%
33	6.929	6.895	6.936	VV	178	3368	0.54%	0.062%
34	6.975	6.936	7.035	VV	249	11727	1.90%	0.215%
35	7.056	7.035	7.073	VV	127	2479	0.40%	0.045%
36	7.161	7.073	7.172	VV	206	9858	1.59%	0.181%

					rters			
37	7.296	7.172	7.493	VV	1006	95737	15.48%	1.755%
38	7.499	7.493	7.507	VV	76	520	0.08%	0.010%
39	7.692	7.507	7.805	VV	805	76712	12.40%	1.406%
40	7.814	7.805	7.819	VV	142	1103	0.18%	0.020%
41	7.918	7.819	7.926	VV	290	14924	2.41%	0.274%
42	8.033	7.926	8.041	VV	654	35247	5.70%	0.646%
43	8.053	8.041	8.204	VV	654	30500	4.93%	0.559%
44	8.231	8.204	8.239	PV	21	263	0.04%	0.005%
45	8.294	8.239	8.314	VV	146	4120	0.67%	0.076%
46	8.326	8.314	8.348	VV	134	2434	0.39%	0.045%
47	8.356	8.348	8.364	VV	112	974	0.16%	0.018%
48	8.479	8.364	8.608	VV	523	41386	6.69%	0.759%
49	8.704	8.608	8.748	VV	470	25290	4.09%	0.464%
50	8.832	8.748	8.842	VV	767	32041	5.18%	0.587%
51	8.854	8.842	8.928	VV	765	29479	4.77%	0.540%
52	9.042	8.928	9.200	VV	7425	472677	76.43%	8.665%
53	9.266	9.200	9.277	VV	670	27783	4.49%	0.509%
54	9.284	9.277	9.328	VV	660	19154	3.10%	0.351%
55	9.337	9.328	9.349	VV	601	7564	1.22%	0.139%
56	9.427	9.349	9.519	VV	718	62264	10.07%	1.141%
57	9.643	9.519	9.733	VV	1161	103665	16.76%	1.900%
58	9.742	9.733	9.748	VV	614	5292	0.86%	0.097%
59	9.804	9.748	9.814	VV	739	27190	4.40%	0.498%
60	9.818	9.814	9.879	VV	738	25223	4.08%	0.462%
61	9.961	9.879	9.987	VV	720	42014	6.79%	0.770%
62	10.008	9.987	10.225	VV	725	52351	8.46%	0.960%
63	10.387	10.225	10.407	PV	703	38987	6.30%	0.715%
64	10.418	10.407	10.426	VV	679	7510	1.21%	0.138%
65	10.436	10.426	10.443	VV	687	6886	1.11%	0.126%
66	10.451	10.443	10.597	VV	675	36906	5.97%	0.677%
67	10.604	10.597	10.629	VV	159	2747	0.44%	0.050%
68	10.637	10.629	10.652	VV	129	1670	0.27%	0.031%
69	10.764	10.652	10.845	VV	787	56288	9.10%	1.032%
70	10.908	10.845	10.917	VV	601	20407	3.30%	0.374%
71	10.923	10.917	10.997	VV	589	20929	3.38%	0.384%
72	11.065	10.997	11.129	VV	635	37268	6.03%	0.683%
73	11.223	11.129	11.371	VV	1002	95506	15.44%	1.751%
74	11.379	11.371	11.386	VV	306	2657	0.43%	0.049%
75	11.432	11.386	11.441	VV	406	11781	1.90%	0.216%
76	11.450	11.441	11.505	VV	400	11739	1.90%	0.215%
77	11.512	11.505	11.526	VV	208	2406	0.39%	0.044%
78	11.538	11.526	11.548	VV	156	1992	0.32%	0.037%
79	11.563	11.548	11.649	VV	167	6388	1.03%	0.117%
80	11.741	11.649	11.763	VV	207	9118	1.47%	0.167%
81	11.782	11.763	11.796	VV	230	4225	0.68%	0.077%
82	12.012	11.796	12.103	VV	1612	186215	30.11%	3.414%
83	12.144	12.103	12.255	VV	987	59148	9.56%	1.084%
84	12.356	12.255	12.469	VV	1183	76047	12.30%	1.394%
85	12.499	12.469	12.558	VV	204	8974	1.45%	0.165%
86	12.630	12.558	12.735	VV	259	16240	2.63%	0.298%
87	12.746	12.735	12.757	PV	23	147	0.02%	0.003%
88	12.820	12.757	12.848	VV	67	1334	0.22%	0.024%
89	12.911	12.848	12.939	PV	136	4039	0.65%	0.074%

Instrument :
FID_B
ClientSampleId :
TP-1-A

Manual Integrations
APPROVED

Sohil
3/15/2019 9:52:43 AM

Instrument :
FID_B
ClientSampleId :
TP-1-A

Manual Integrations
APPROVED

Sohil
3/15/2019 9:52:43 AM

					rters				
90	13.054	12.939	13.183	VV	771	67559	10.92%	1.239%	
91	13.308	13.183	13.497	VV	1547	133233	21.54%	2.442%	
92	13.635	13.497	13.711	PV	1233	87756	14.19%	1.609%	
93	13.821	13.711	13.959	VV	3122	203829	32.96%	3.737%	
94	14.097	13.959	14.204	VV	2288	167236	27.04%	3.066%	
95	14.220	14.204	14.275	VV	524	16508	2.67%	0.303%	
96	14.397	14.275	14.622	VV	3210	309113	49.98%	5.667%	
97	14.716	14.622	14.795	VV	1227	75859	12.27%	1.391%	
98	14.866	14.795	14.922	VV	652	37243	6.02%	0.683%	
99	14.989	14.922	15.049	VV	739	42675	6.90%	0.782%	
100	15.131	15.049	15.208	VV	1827	119594	19.34%	2.192%	
101	15.247	15.208	15.284	VV	1109	47447	7.67%	0.870%	
102	15.436	15.284	15.457	VV	2238	161399	26.10%	2.959%	
103	15.463	15.457	15.518	VV	2205	76885	12.43%	1.409%	
104	15.597	15.518	15.681	VV	2472	209060	33.80%	3.833%	
105	15.792	15.681	15.938	VV	4990	438555	70.91%	8.040%	
106	15.957	15.938	16.022	VV	1968	84829	13.72%	1.555%	
107	16.097	16.022	16.170	VV	2621	170154	27.51%	3.119%	
108	16.233	16.170	16.297	VV	2438	154803	25.03%	2.838%	
109	16.349	16.297	16.416	VV	2090	140504	22.72%	2.576%	
110	16.589	16.416	16.750	VBA	4397	618444	100.00%	11.337%	

Sum of corrected areas: 5454867

FB031119.M Thu Mar 14 02:09:54 2019