

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB031325\
Data File : FB031600.D
Signal(s) : FID2B.CH
Acq On : 13 Mar 2025 10:59
Operator : YP/AJ
Sample : VBF0313W1
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Mar 15 02:12:50 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030625.M
Quant Title :
QLast Update : Thu Mar 06 13:17:04 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.792	430174	18.997 ng/ml
Target Compounds			
6) t Toluene	10.616	5307	0.134 ng/ml
8) t m-Xylene	13.192	7522	0.195 ng/ml
9) t O-Xylene	13.918	10878	0.295 ng/ml
10) t 1,2,4-Trimethylbenzene	16.195	18065	0.639 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB031325\
Data File : FB031600.D
Signal(s) : FID2B.CH
Acq On : 13 Mar 2025 10:59
Operator : YP/AJ
Sample : VBF0313W1
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Mar 15 02:12:50 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030625.M
Quant Title :
QLast Update : Thu Mar 06 13:17:04 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

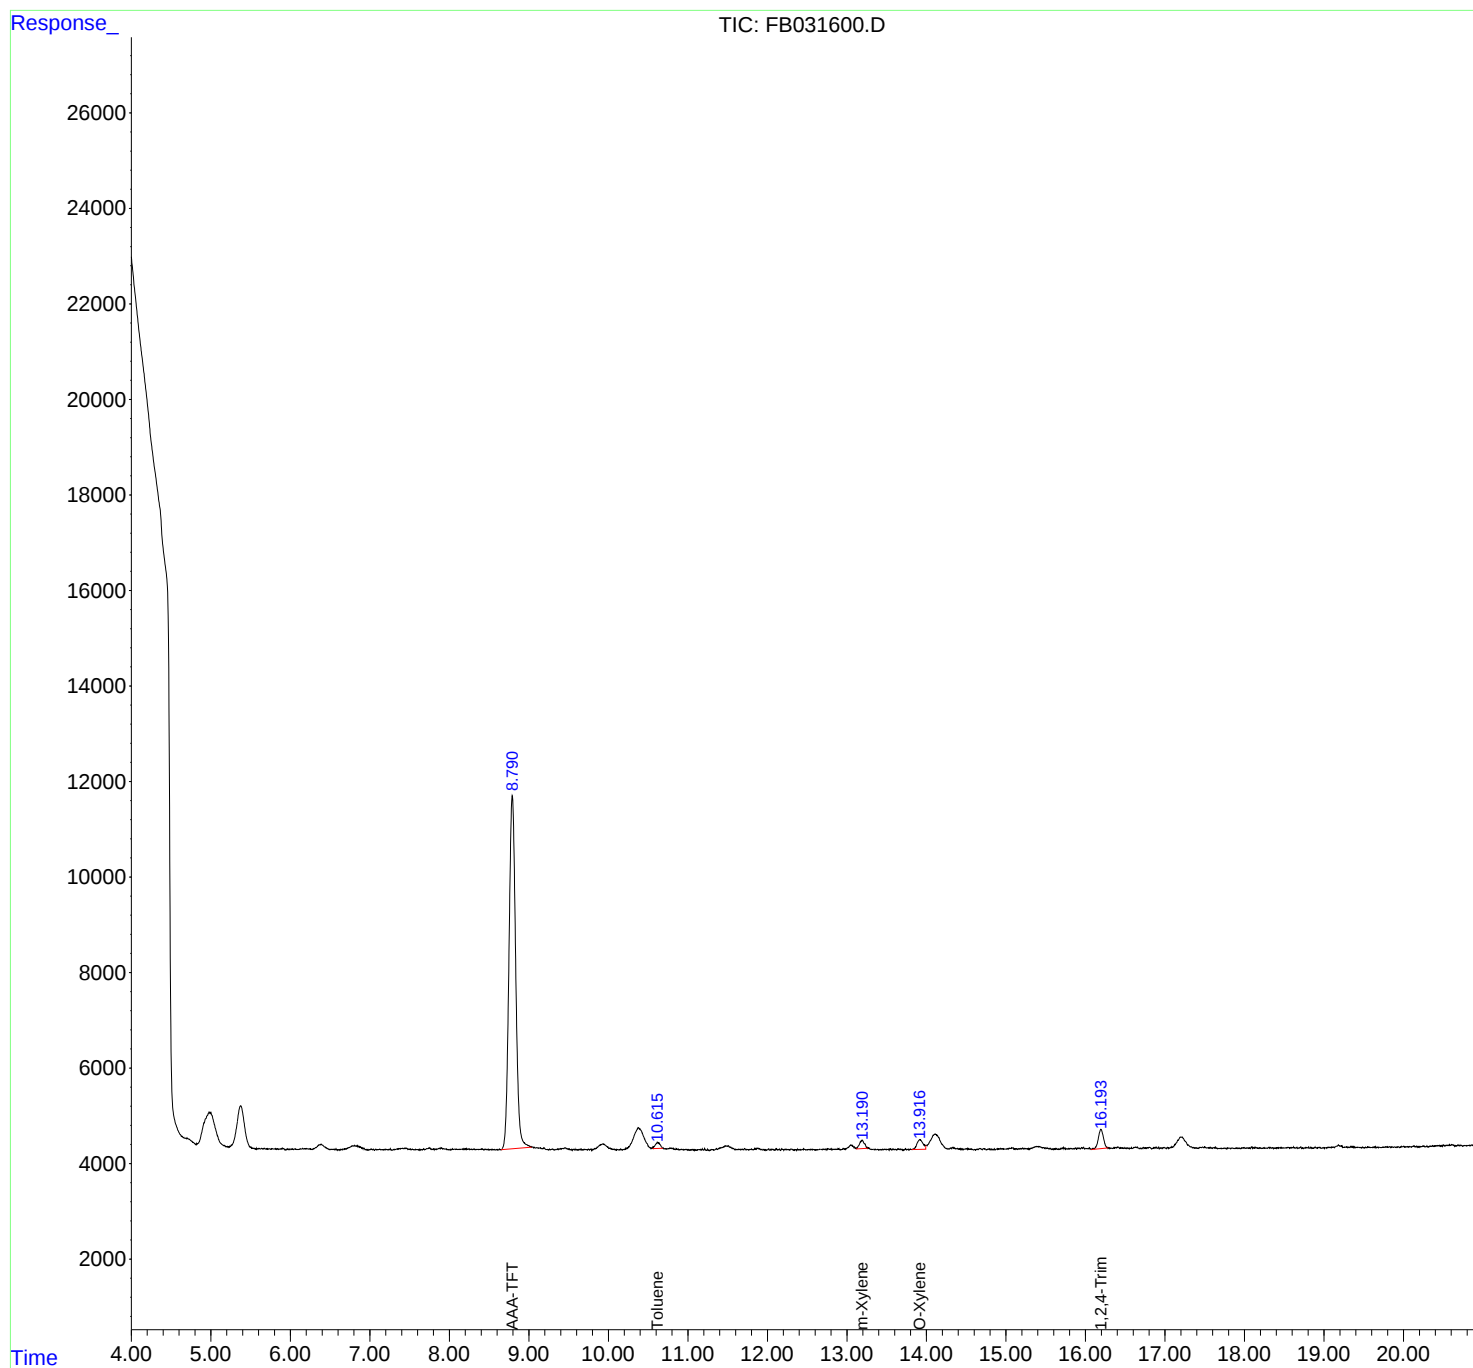


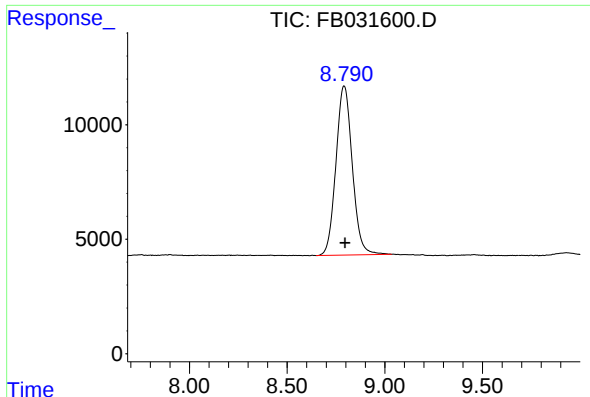

#5 AAA-TFT


R.T.: 8.792 min
Delta R.T.: -0.005 min
Response: 430174
Conc: 19.00 ng/ml

Instrument :
FID_B
ClientSampleId :

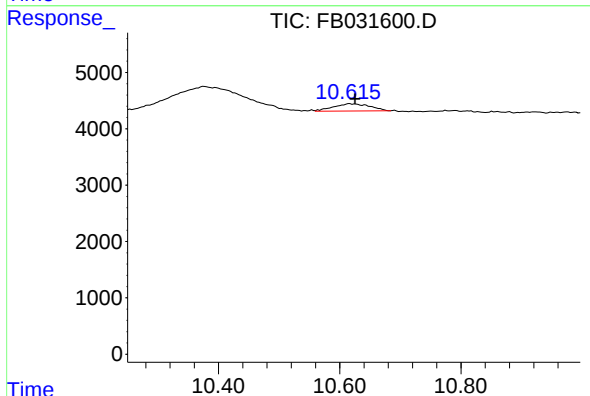


#6 Toluene

R.T.: 10.616 min
Delta R.T.: -0.009 min
Response: 5307
Conc: 0.13 ng/ml

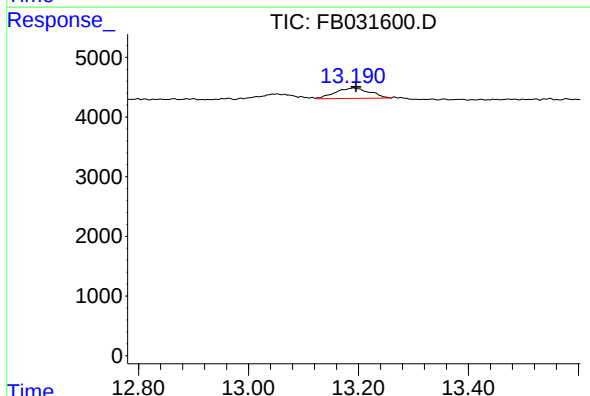


#8 m-Xylene

R.T.: 13.192 min
Delta R.T.: -0.004 min
Response: 7522
Conc: 0.20 ng/ml

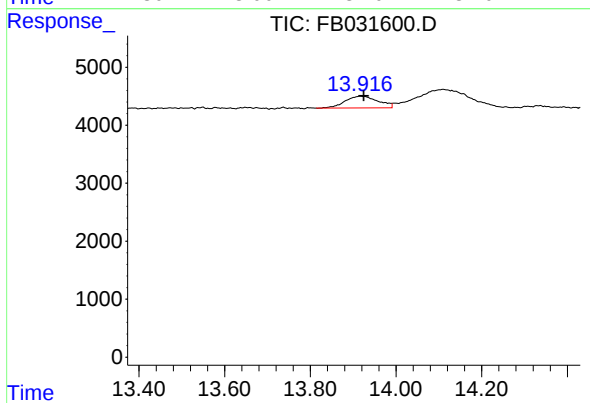

#9 O-Xylene

R.T.: 13.918 min
Delta R.T.: -0.006 min
Response: 10878
Conc: 0.29 ng/ml

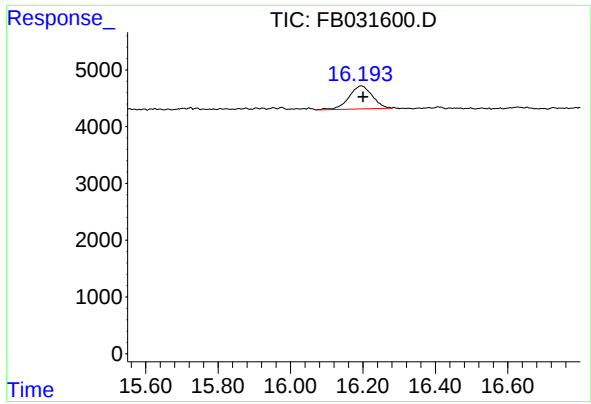

#10 1,2,4-Trimethylbenzene

R.T.: 16.195 min
Delta R.T.: -0.005 min
Response: 18065
Conc: 0.64 ng/ml

Instrument :
FID_B
ClientSampleId :