

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB031325\
 Data File : FB031601.D
 Signal(s) : FID2B.CH
 Acq On : 13 Mar 2025 11:27
 Operator : YP/AJ
 Sample : BSF0313W1
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0313W1

Integration File: Calibration.e
 Quant Time: Mar 15 02:13:02 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030625.M
 Quant Title :
 QLast Update : Thu Mar 06 13:17:04 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.793	368784	16.286 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.721	856187	33.664 ng/ml
2) t 2,2,4-Trimethylpentane	7.423	1056522	30.473 ng/ml
3) t n-Heptane	7.754	319505	10.322 ng/ml
4) t Benzene	7.894	397563	9.406 ng/ml
6) t Toluene	10.621	1112679	28.129 ng/ml
7) t Ethylbenzene	13.057	321816	9.124 ng/ml
8) t m-Xylene	13.191	702404	18.222 ng/ml
9) t O-Xylene	13.919	656933	17.801 ng/ml
10) t 1,2,4-Trimethylbenzene	16.195	496337	17.567 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB031325\
Data File : FB031601.D
Signal(s) : FID2B.CH
Acq On : 13 Mar 2025 11:27
Operator : YP/AJ
Sample : BSF0313W1
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0313W1

Integration File: Calibration.e
Quant Time: Mar 15 02:13:02 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030625.M
Quant Title :
QLast Update : Thu Mar 06 13:17:04 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

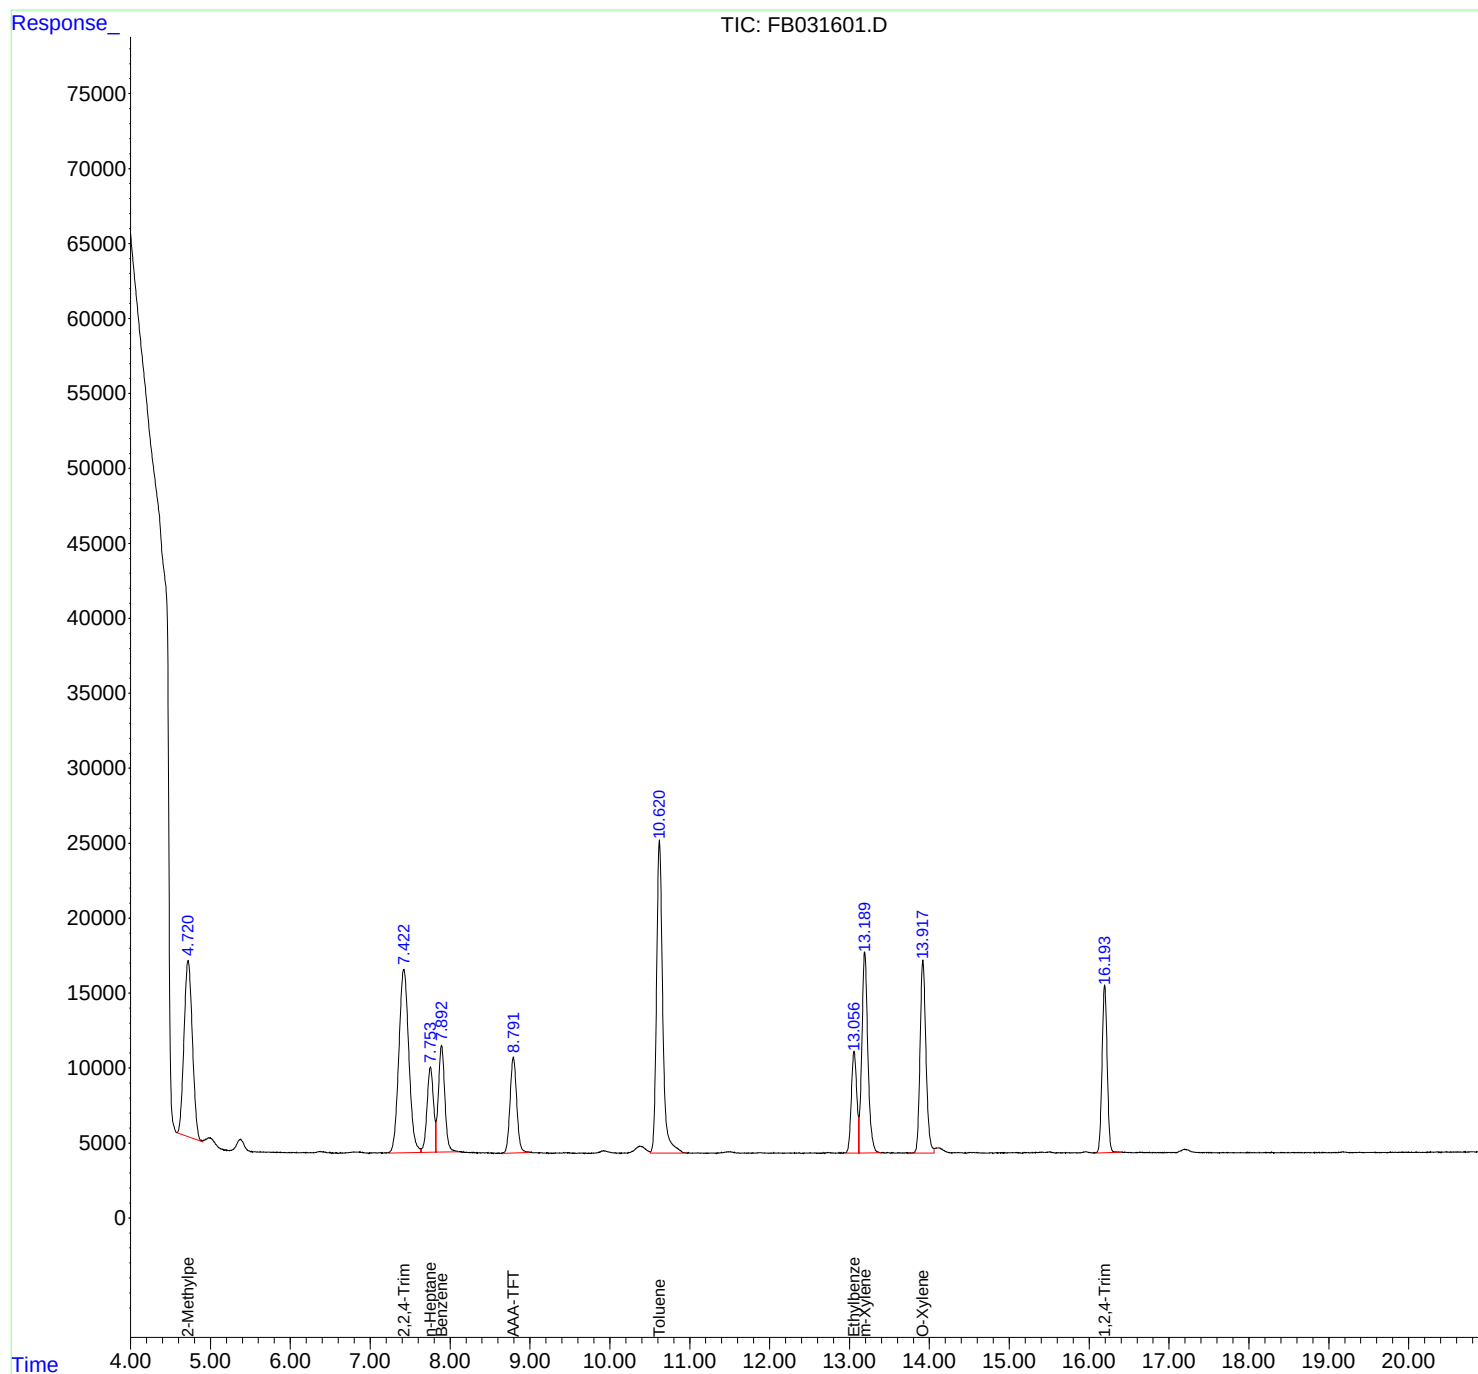


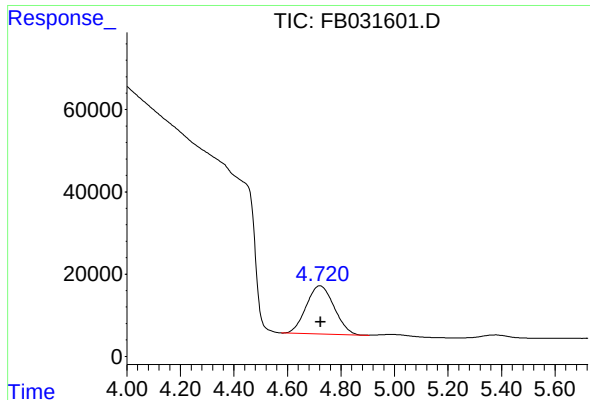

#1 2-Methylpentane


R.T.: 4.721 min
Delta R.T.: -0.003 min
Response: 856187
Conc: 33.66 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0313W1

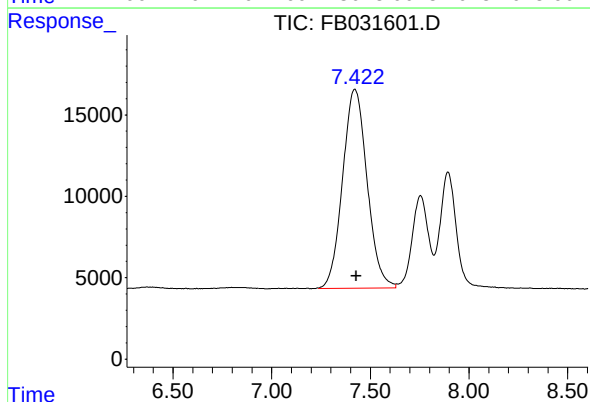


#2 2,2,4-Trimethylpentane

R.T.: 7.423 min
Delta R.T.: -0.006 min
Response: 1056522
Conc: 30.47 ng/ml

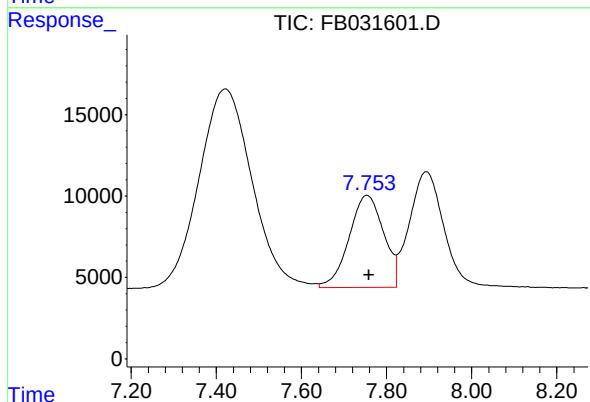


#3 n-Heptane

R.T.: 7.754 min
Delta R.T.: -0.004 min
Response: 319505
Conc: 10.32 ng/ml

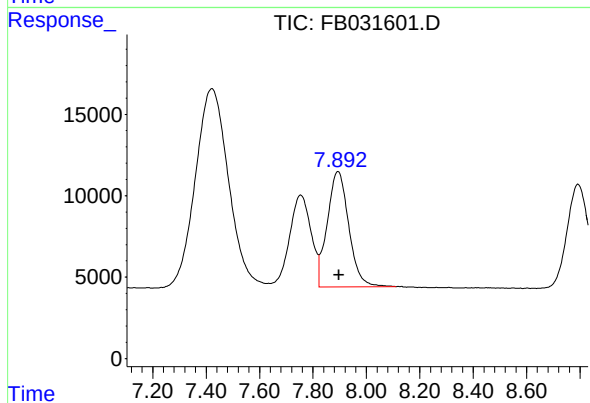

#4 Benzene


R.T.: 7.894 min
Delta R.T.: -0.003 min
Response: 397563
Conc: 9.41 ng/ml

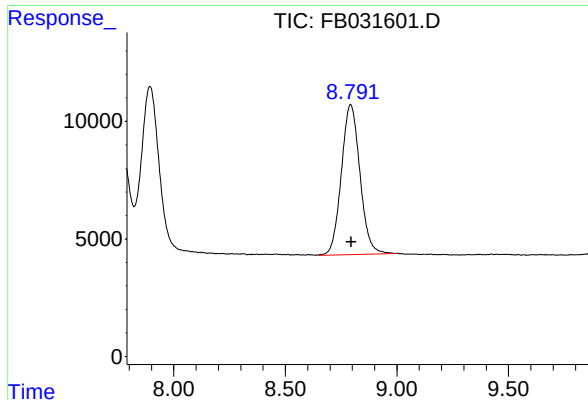

#5 AAA-TFT


R.T.: 8.793 min
Delta R.T.: -0.004 min
Response: 368784
Conc: 16.29 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0313W1

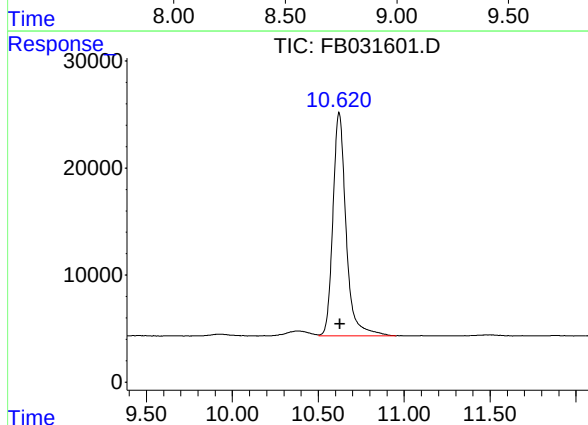


#6 Toluene

R.T.: 10.621 min
Delta R.T.: -0.004 min
Response: 1112679
Conc: 28.13 ng/ml

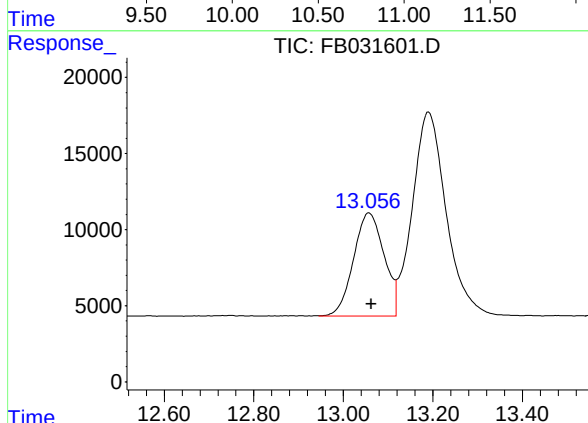


#7 Ethylbenzene

R.T.: 13.057 min
Delta R.T.: -0.005 min
Response: 321816
Conc: 9.12 ng/ml

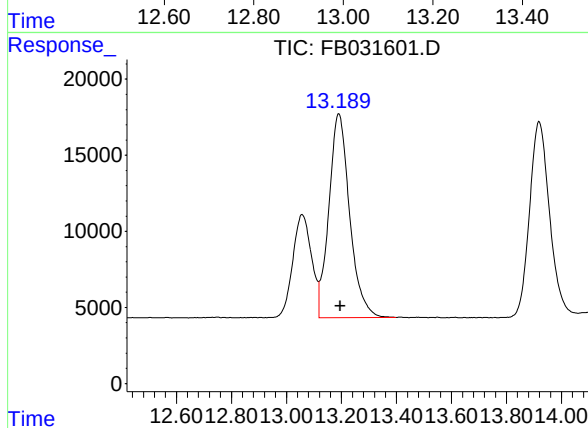

#8 m-Xylene


R.T.: 13.191 min
Delta R.T.: -0.005 min
Response: 702404
Conc: 18.22 ng/ml

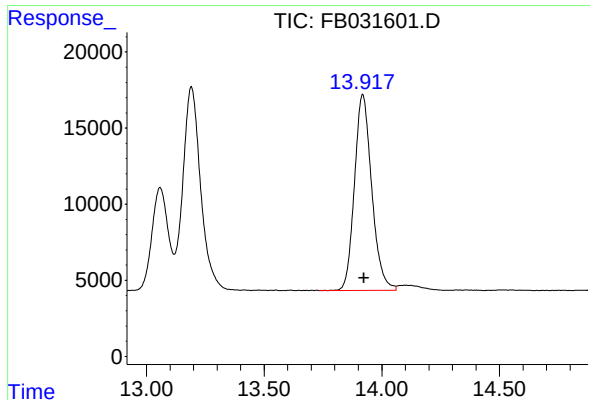

#9 O-Xylene

R.T.: 13.919 min
Delta R.T.: -0.005 min
Response: 656933
Conc: 17.80 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0313W1

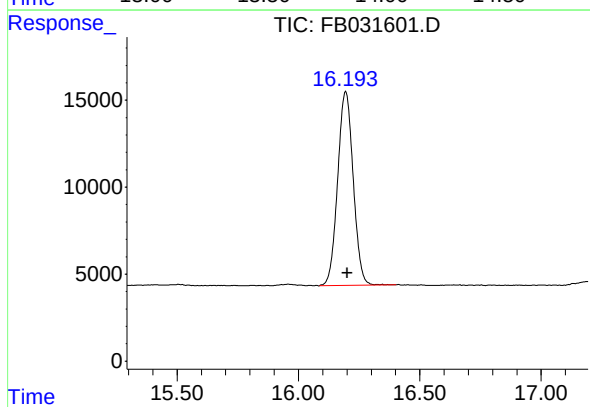

#10 1,2,4-Trimethylbenzene

R.T.: 16.195 min
Delta R.T.: -0.006 min
Response: 496337
Conc: 17.57 ng/ml