

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB031419\
 Data File : FB020200.D
 Signal(s) : FID2B.CH
 Acq On : 14 Mar 2019 11:44
 Operator : MJ/SJ
 Sample : K1895-01
 Misc : 5.03g/5.00ml DI WATER
 ALS Vial : 5 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Mar 15 01:45:41 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB031119.M
 Quant Title :
 QLast Update : Mon Mar 11 13:44:46 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.094	950653	36.212 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.893	94521	2.802 ng/ml
2) t 2,2,4-Trimethylpentane	7.632	187129	5.706 ng/ml
3) t n-Heptane	7.995	431979	10.380 ng/ml
6) t Toluene	10.888	351467	9.511 ng/ml
7) t Ethylbenzene	13.323	375699	15.968 ng/ml
8) t m-Xylene	13.464	279433	13.099 ng/ml
9) t O-Xylene	14.203	160928	8.495 ng/ml
10) t 1,2,4-Trimethylbenzene	16.489	682348	34.407 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB031419\
Data File : FB020200.D
Signal(s) : FID2B.CH
Acq On : 14 Mar 2019 11:44
Operator : MJ/SJ
Sample : K1895-01
Misc : 5.03g/5.00ml DI WATER
ALS Vial : 5 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Mar 15 01:45:41 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB031119.M
Quant Title :
QLast Update : Mon Mar 11 13:44:46 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

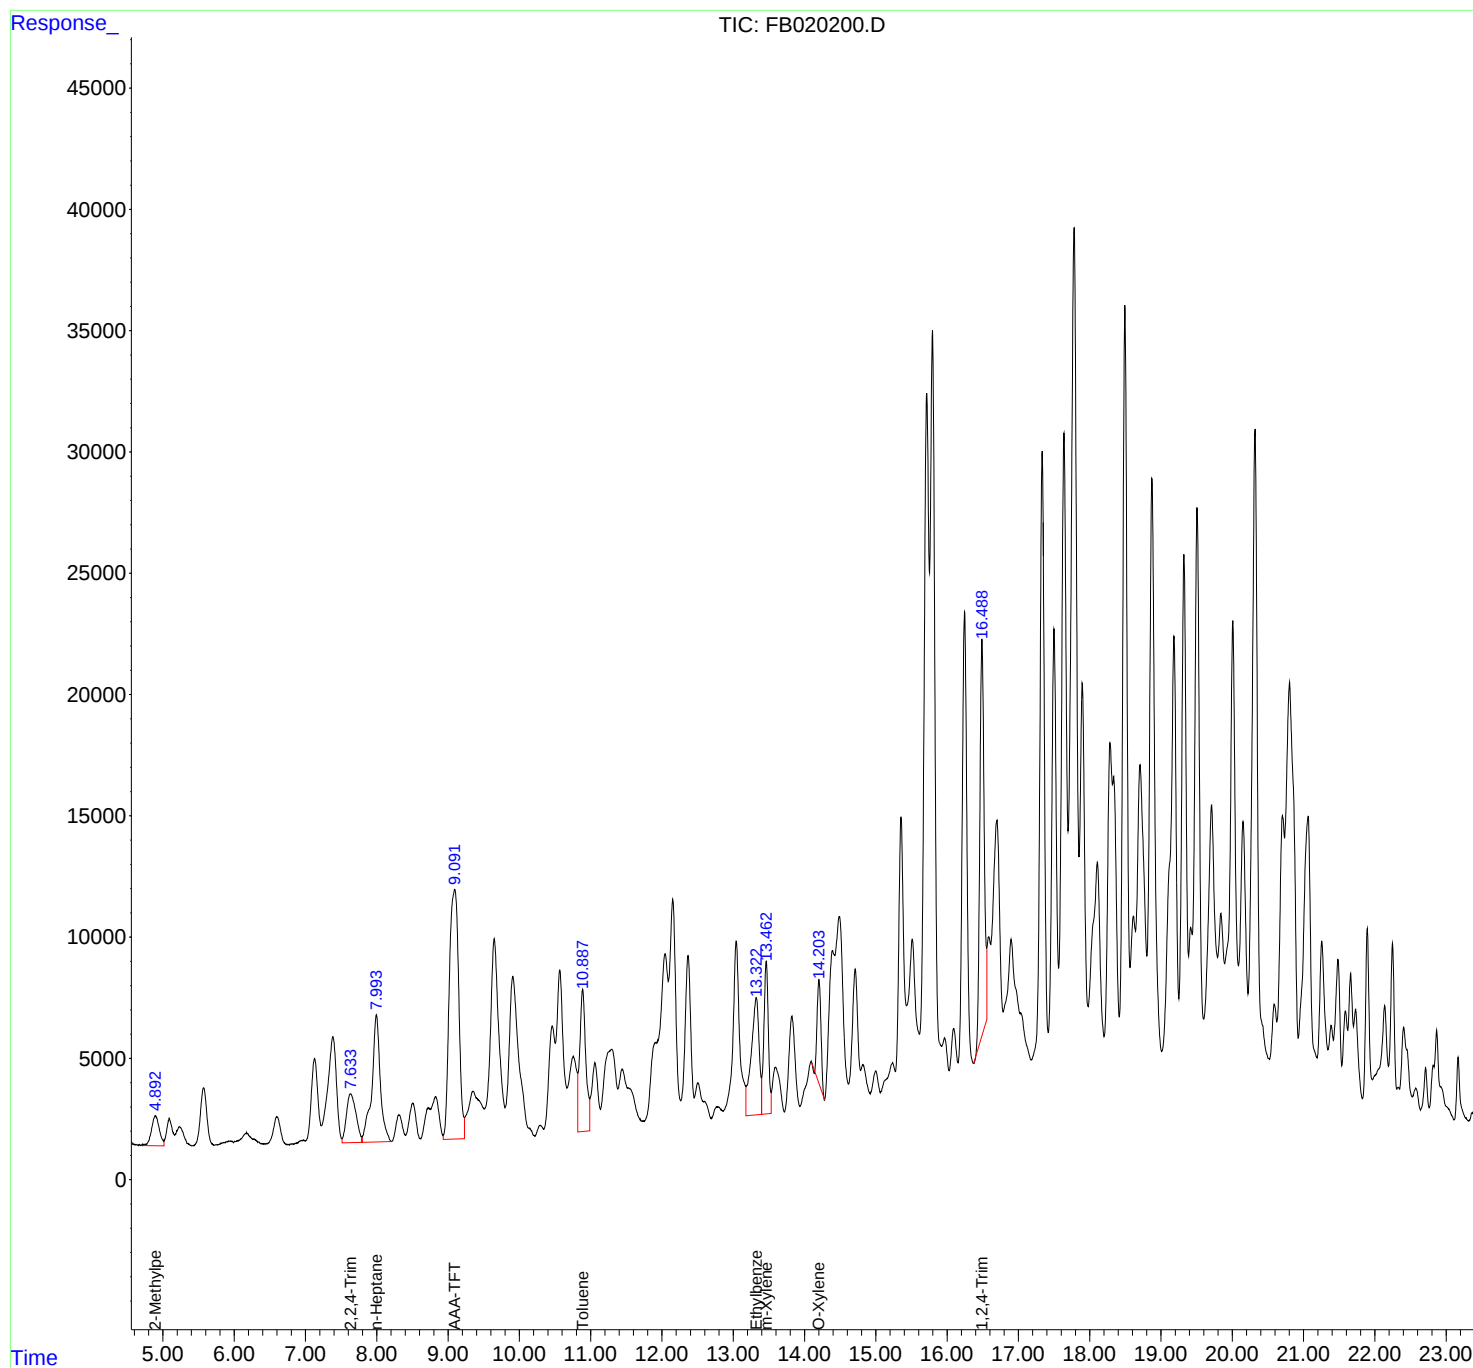

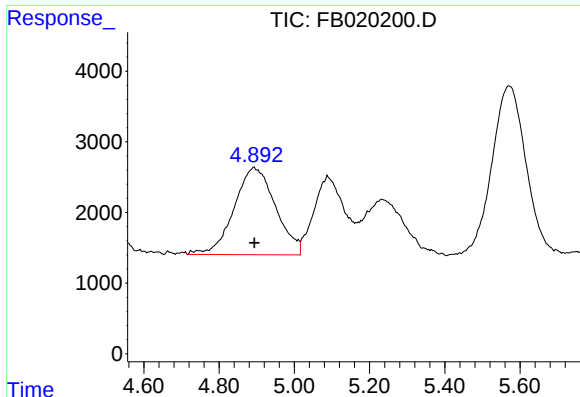


#1 2-Methylpentane

R.T.: 4.893 min
Delta R.T.: -0.001 min
Response: 94521
Conc: 2.80 ng/ml

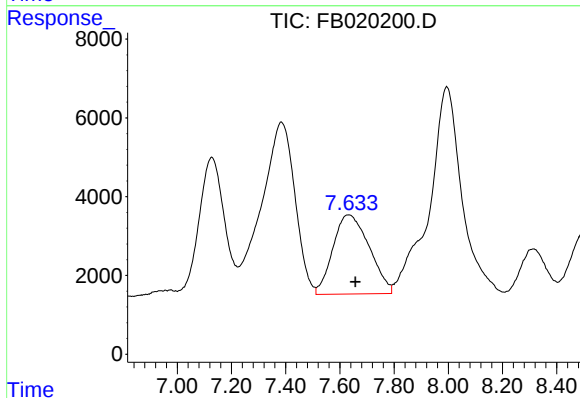


#2 2,2,4-Trimethylpentane

R.T.: 7.632 min
Delta R.T.: -0.025 min
Response: 187129
Conc: 5.71 ng/ml

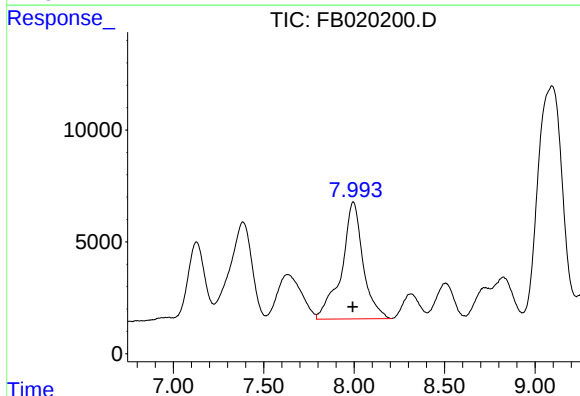


#3 n-Heptane

R.T.: 7.995 min
Delta R.T.: 0.003 min
Response: 431979
Conc: 10.38 ng/ml

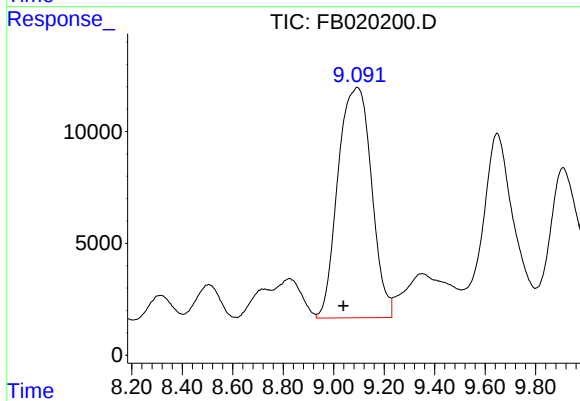


#5 AAA-TFT

R.T.: 9.094 min
Delta R.T.: 0.056 min
Response: 950653
Conc: 36.21 ng/ml

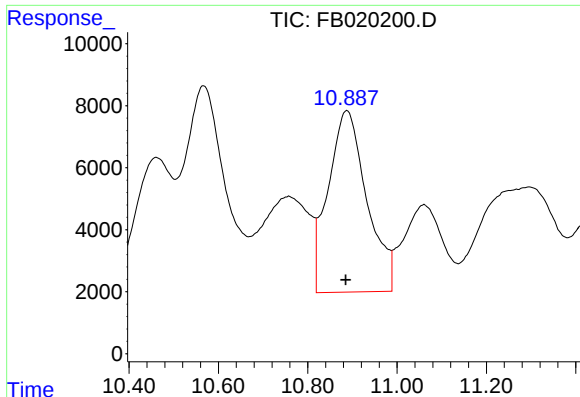


#6 Toluene

R.T.: 10.888 min
Delta R.T.: 0.003 min
Response: 351467
Conc: 9.51 ng/ml

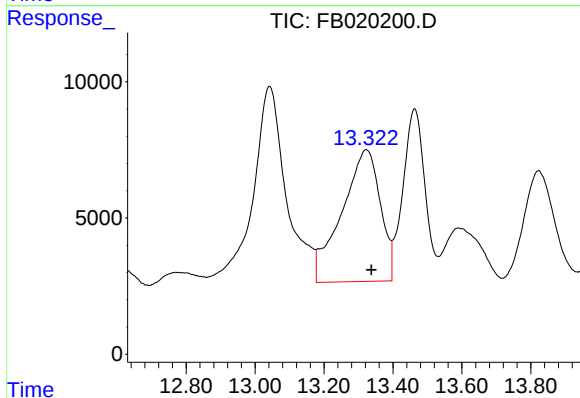


#7 Ethylbenzene

R.T.: 13.323 min
Delta R.T.: -0.015 min
Response: 375699
Conc: 15.97 ng/ml

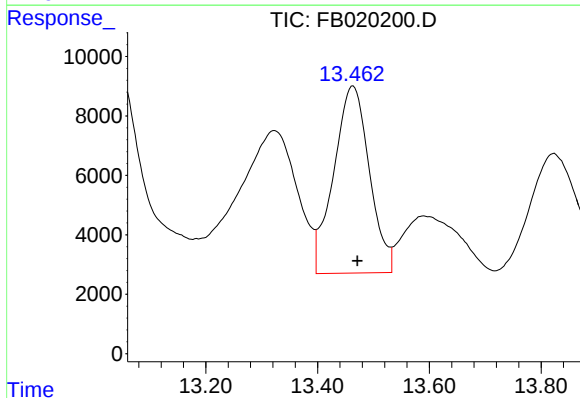


#8 m-Xylene

R.T.: 13.464 min
Delta R.T.: -0.008 min
Response: 279433
Conc: 13.10 ng/ml

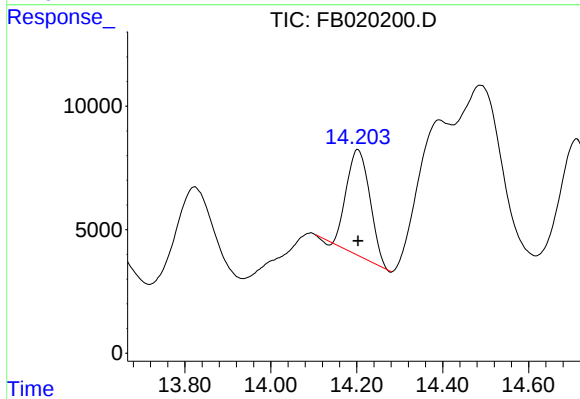

#9 O-Xylene

R.T.: 14.203 min
Delta R.T.: 0.000 min
Response: 160928
Conc: 8.50 ng/ml

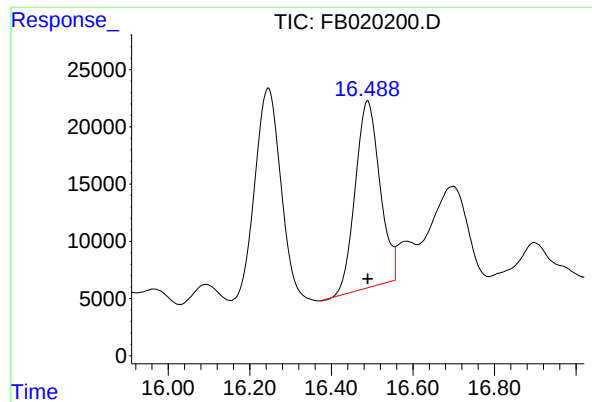

#10 1,2,4-Trimethylbenzene

R.T.: 16.489 min
Delta R.T.: 0.000 min
Response: 682348
Conc: 34.41 ng/ml