

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB031419\
 Data File : FB020215.D
 Signal(s) : FID2B.CH
 Acq On : 14 Mar 2019 19:18
 Operator : MJ/SJ
 Sample : K1927-02
 Misc : 5.05g/5.00ml DI WATER
 ALS Vial : 20 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Mar 15 01:48:35 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB031119.M
 Quant Title :
 QLast Update : Mon Mar 11 13:44:46 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	9.046	468947	17.863 ng/ml
Target Compounds				
1) t	2-Methylpentane	4.907	7964	0.236 ng/ml
2) t	2,2,4-Trimethylpentane	7.655	46375	1.414 ng/ml
3) t	n-Heptane	7.996	25927	0.623 ng/ml
4) t	Benzene	8.124	649	0.014 ng/ml
6) t	Toluene	10.891	192218	5.202 ng/ml
7) t	Ethylbenzene	13.338	230617	9.802 ng/ml
8) t	m-Xylene	13.473	429815	20.149 ng/ml
9) t	O-Xylene	14.207	215152	11.358 ng/ml
10) t	1,2,4-Trimethylbenzene	16.493	700972	35.346 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB031419\
Data File : FB020215.D
Signal(s) : FID2B.CH
Acq On : 14 Mar 2019 19:18
Operator : MJ/SJ
Sample : K1927-02
Misc : 5.05g/5.00ml DI WATER
ALS Vial : 20 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Mar 15 01:48:35 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB031119.M
Quant Title :
QLast Update : Mon Mar 11 13:44:46 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

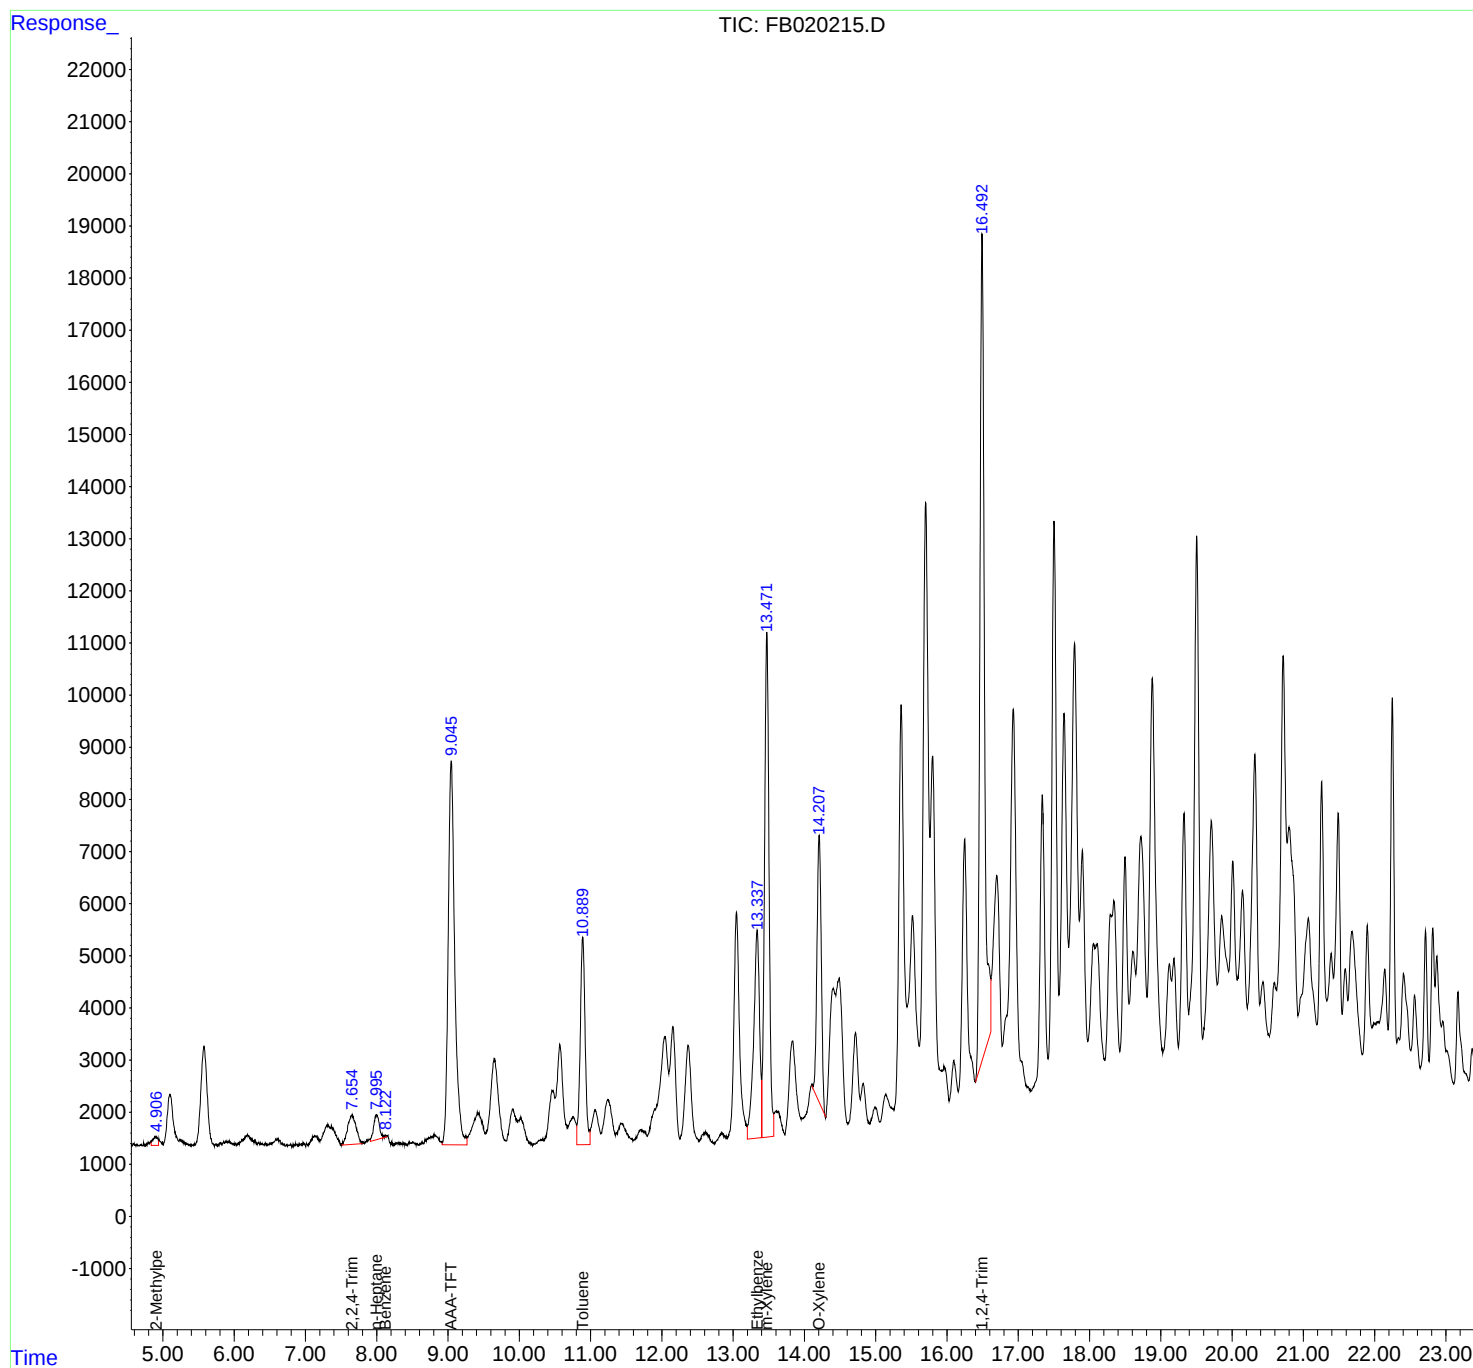

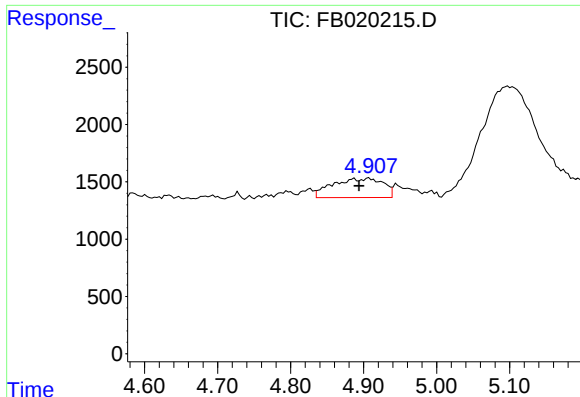


#1 2-Methylpentane

R.T.: 4.907 min
Delta R.T.: 0.013 min
Response: 7964
Conc: 0.24 ng/ml

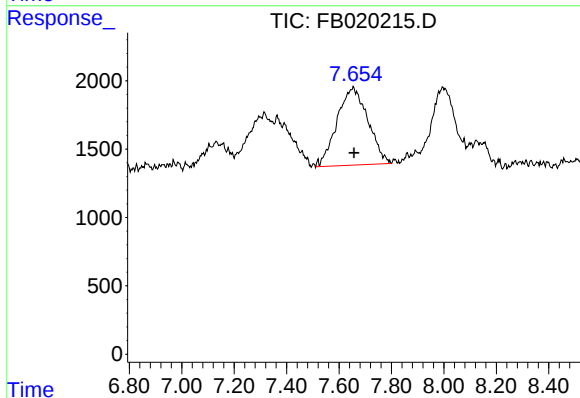


#2 2,2,4-Trimethylpentane

R.T.: 7.655 min
Delta R.T.: -0.002 min
Response: 46375
Conc: 1.41 ng/ml

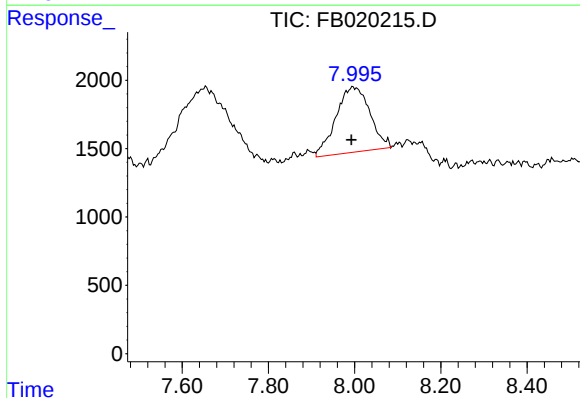


#3 n-Heptane

R.T.: 7.996 min
Delta R.T.: 0.004 min
Response: 25927
Conc: 0.62 ng/ml

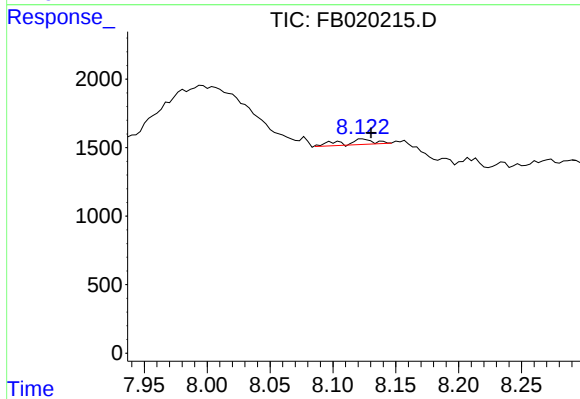


#4 Benzene

R.T.: 8.124 min
Delta R.T.: -0.006 min
Response: 649
Conc: 0.01 ng/ml

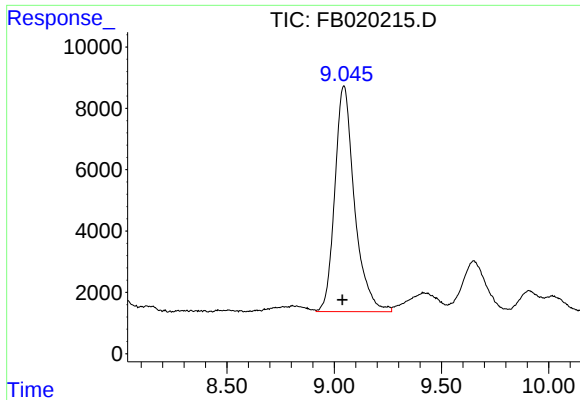


#5 AAA-TFT

R.T.: 9.046 min
 Delta R.T.: 0.008 min
 Response: 468947
 Conc: 17.86 ng/ml

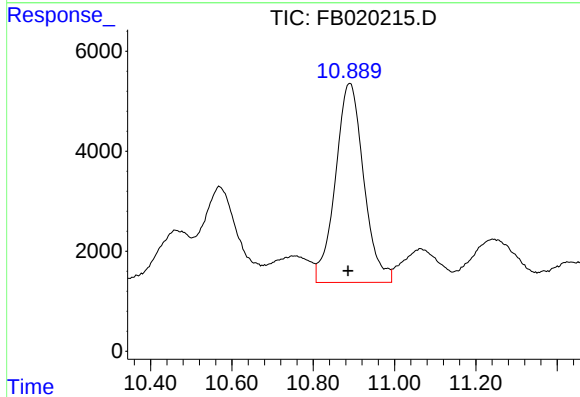


#6 Toluene

R.T.: 10.891 min
 Delta R.T.: 0.005 min
 Response: 192218
 Conc: 5.20 ng/ml

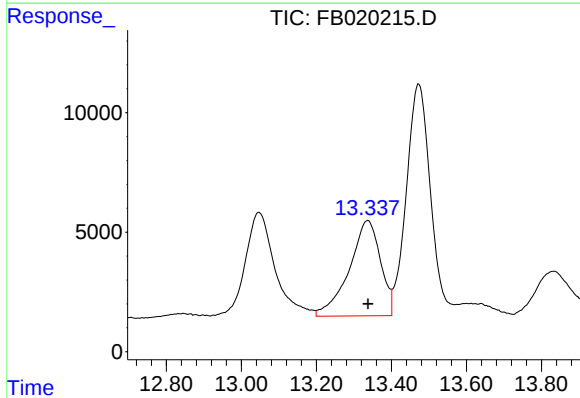


#7 Ethylbenzene

R.T.: 13.338 min
 Delta R.T.: 0.000 min
 Response: 230617
 Conc: 9.80 ng/ml

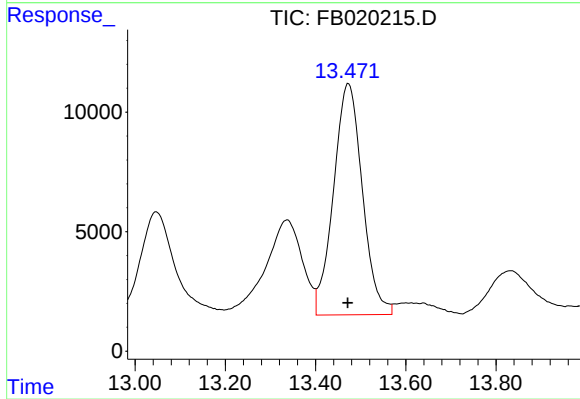


#8 m-Xylene

R.T.: 13.473 min
 Delta R.T.: 0.002 min
 Response: 429815
 Conc: 20.15 ng/ml

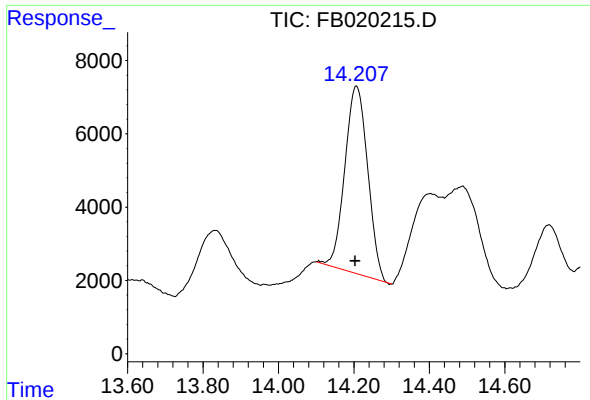

#9 O-Xylene

R.T.: 14.207 min
Delta R.T.: 0.004 min
Response: 215152
Conc: 11.36 ng/ml

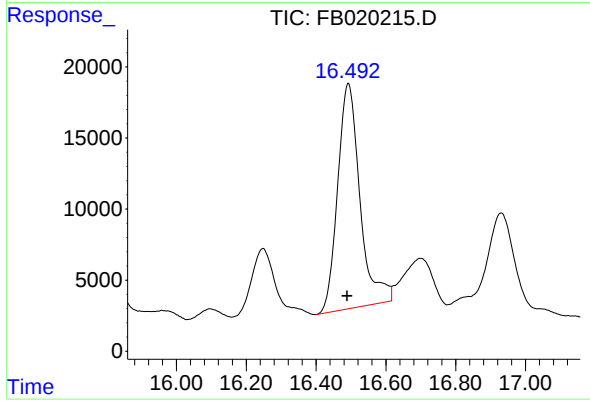

#10 1,2,4-Trimethylbenzene

R.T.: 16.493 min
Delta R.T.: 0.004 min
Response: 700972
Conc: 35.35 ng/ml