

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB031419\
 Data File : FB020217.D
 Signal(s) : FID2B.CH
 Acq On : 14 Mar 2019 20:19
 Operator : MJ/SJ
 Sample : K1698-01
 Misc : 5.02g/5.00ml DI WATER
 ALS Vial : 22 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Mar 15 01:48:55 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB031119.M
 Quant Title :
 QLast Update : Mon Mar 11 13:44:46 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.044	398741	15.189 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.891	10629	0.315 ng/ml
2) t 2,2,4-Trimethylpentane	7.662	40872	1.246 ng/ml
3) t n-Heptane	7.982	6077	0.146 ng/ml
6) t Toluene	10.889	18705	0.506 ng/ml
8) t m-Xylene	13.472	8395	0.394 ng/ml
9) t O-Xylene	14.201	778	0.041 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB031419\
Data File : FB020217.D
Signal(s) : FID2B.CH
Acq On : 14 Mar 2019 20:19
Operator : MJ/SJ
Sample : K1698-01
Misc : 5.02g/5.00ml DI WATER
ALS Vial : 22 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Mar 15 01:48:55 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB031119.M
Quant Title :
QLast Update : Mon Mar 11 13:44:46 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

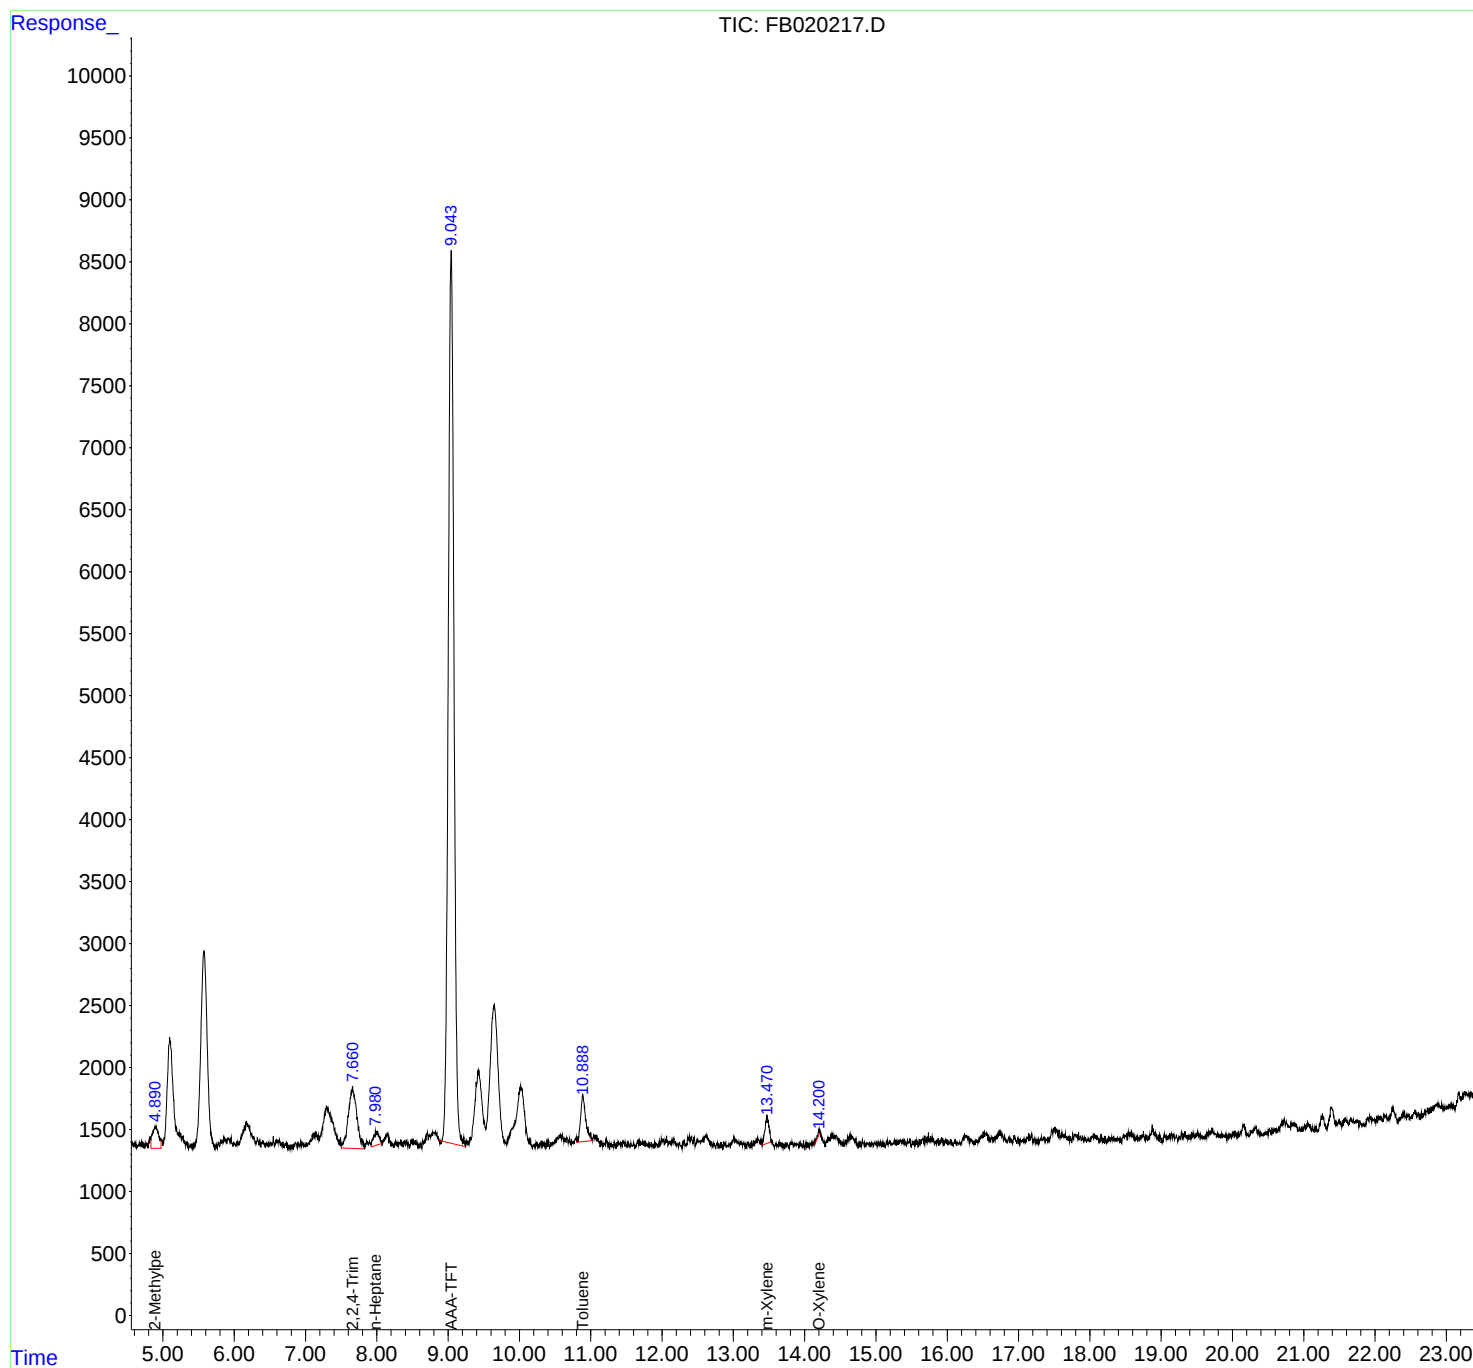

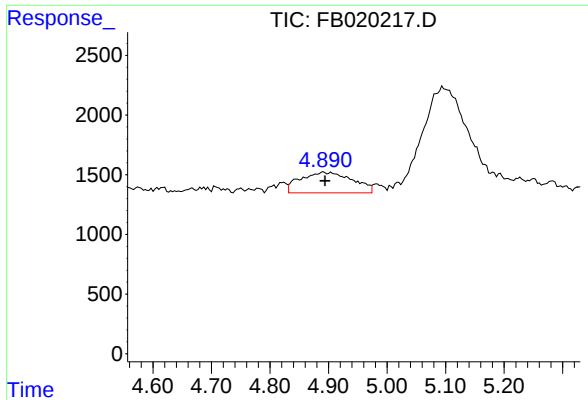


#1 2-Methylpentane

R.T.: 4.891 min
Delta R.T.: -0.003 min
Response: 10629
Conc: 0.32 ng/ml

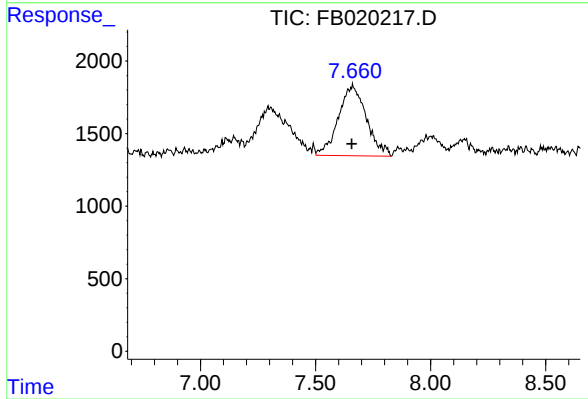


#2 2,2,4-Trimethylpentane

R.T.: 7.662 min
Delta R.T.: 0.005 min
Response: 40872
Conc: 1.25 ng/ml

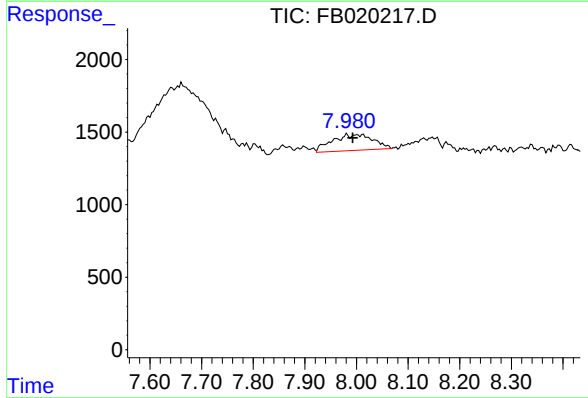


#3 n-Heptane

R.T.: 7.982 min
Delta R.T.: -0.011 min
Response: 6077
Conc: 0.15 ng/ml

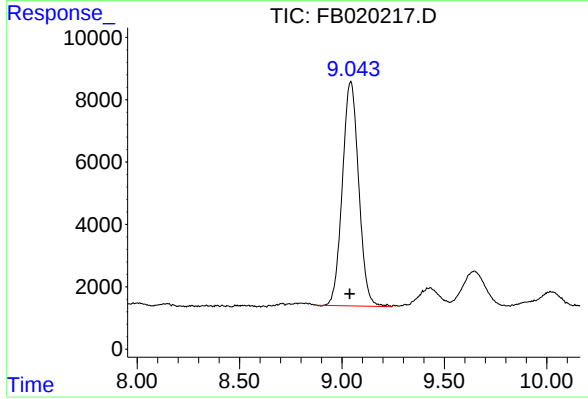


#5 AAA-TFT

R.T.: 9.044 min
Delta R.T.: 0.005 min
Response: 398741
Conc: 15.19 ng/ml

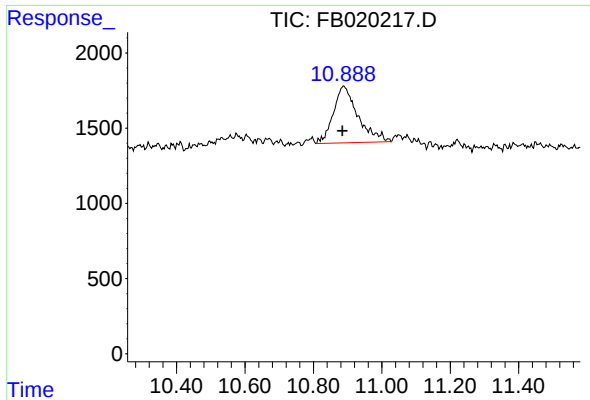


#6 Toluene

R.T.: 10.889 min
Delta R.T.: 0.004 min
Response: 18705
Conc: 0.51 ng/ml

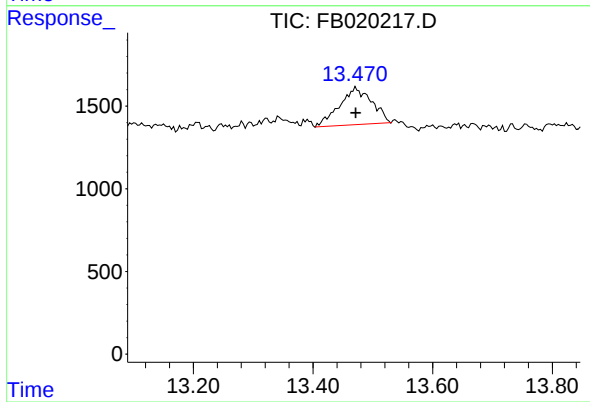

#8 m-Xylene

R.T.: 13.472 min
Delta R.T.: 0.000 min
Response: 8395
Conc: 0.39 ng/ml

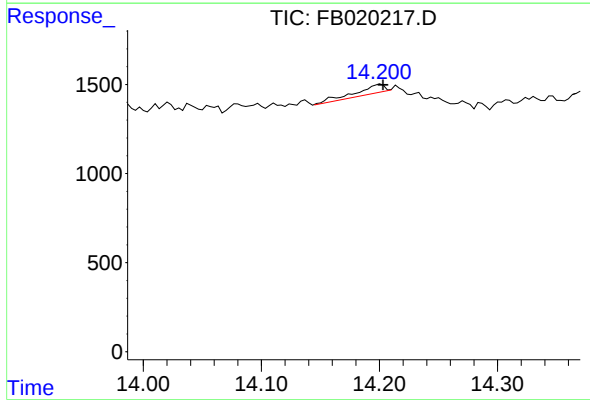

#9 O-Xylene

R.T.: 14.201 min
Delta R.T.: -0.003 min
Response: 778
Conc: 0.04 ng/ml