

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB031419\
 Data File : FB020198.D
 Signal(s) : FID2B.CH
 Acq On : 14 Mar 2019 10:20
 Operator : MJ/SJ
 Sample : BSF0314S1
 Misc : 5.01g/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Mar 15 01:45:05 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB031119.M
 Quant Title :
 QLast Update : Mon Mar 11 13:44:46 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.038	462458	17.616 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.897	978968	29.021 ng/ml
2) t 2,2,4-Trimethylpentane	7.660	921473	28.099 ng/ml
3) t n-Heptane	7.993	395554	9.505 ng/ml
4) t Benzene	8.131	412407	8.858 ng/ml
6) t Toluene	10.885	940862	25.461 ng/ml
7) t Ethylbenzene	13.337	211419	8.986 ng/ml
8) t m-Xylene	13.470	418680	19.627 ng/ml
9) t O-Xylene	14.202	405583	21.411 ng/ml
10) t 1,2,4-Trimethylbenzene	16.488	417643	21.059 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB031419\
Data File : FB020198.D
Signal(s) : FID2B.CH
Acq On : 14 Mar 2019 10:20
Operator : MJ/SJ
Sample : BSF0314S1
Misc : 5.01g/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Mar 15 01:45:05 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB031119.M
Quant Title :
QLast Update : Mon Mar 11 13:44:46 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

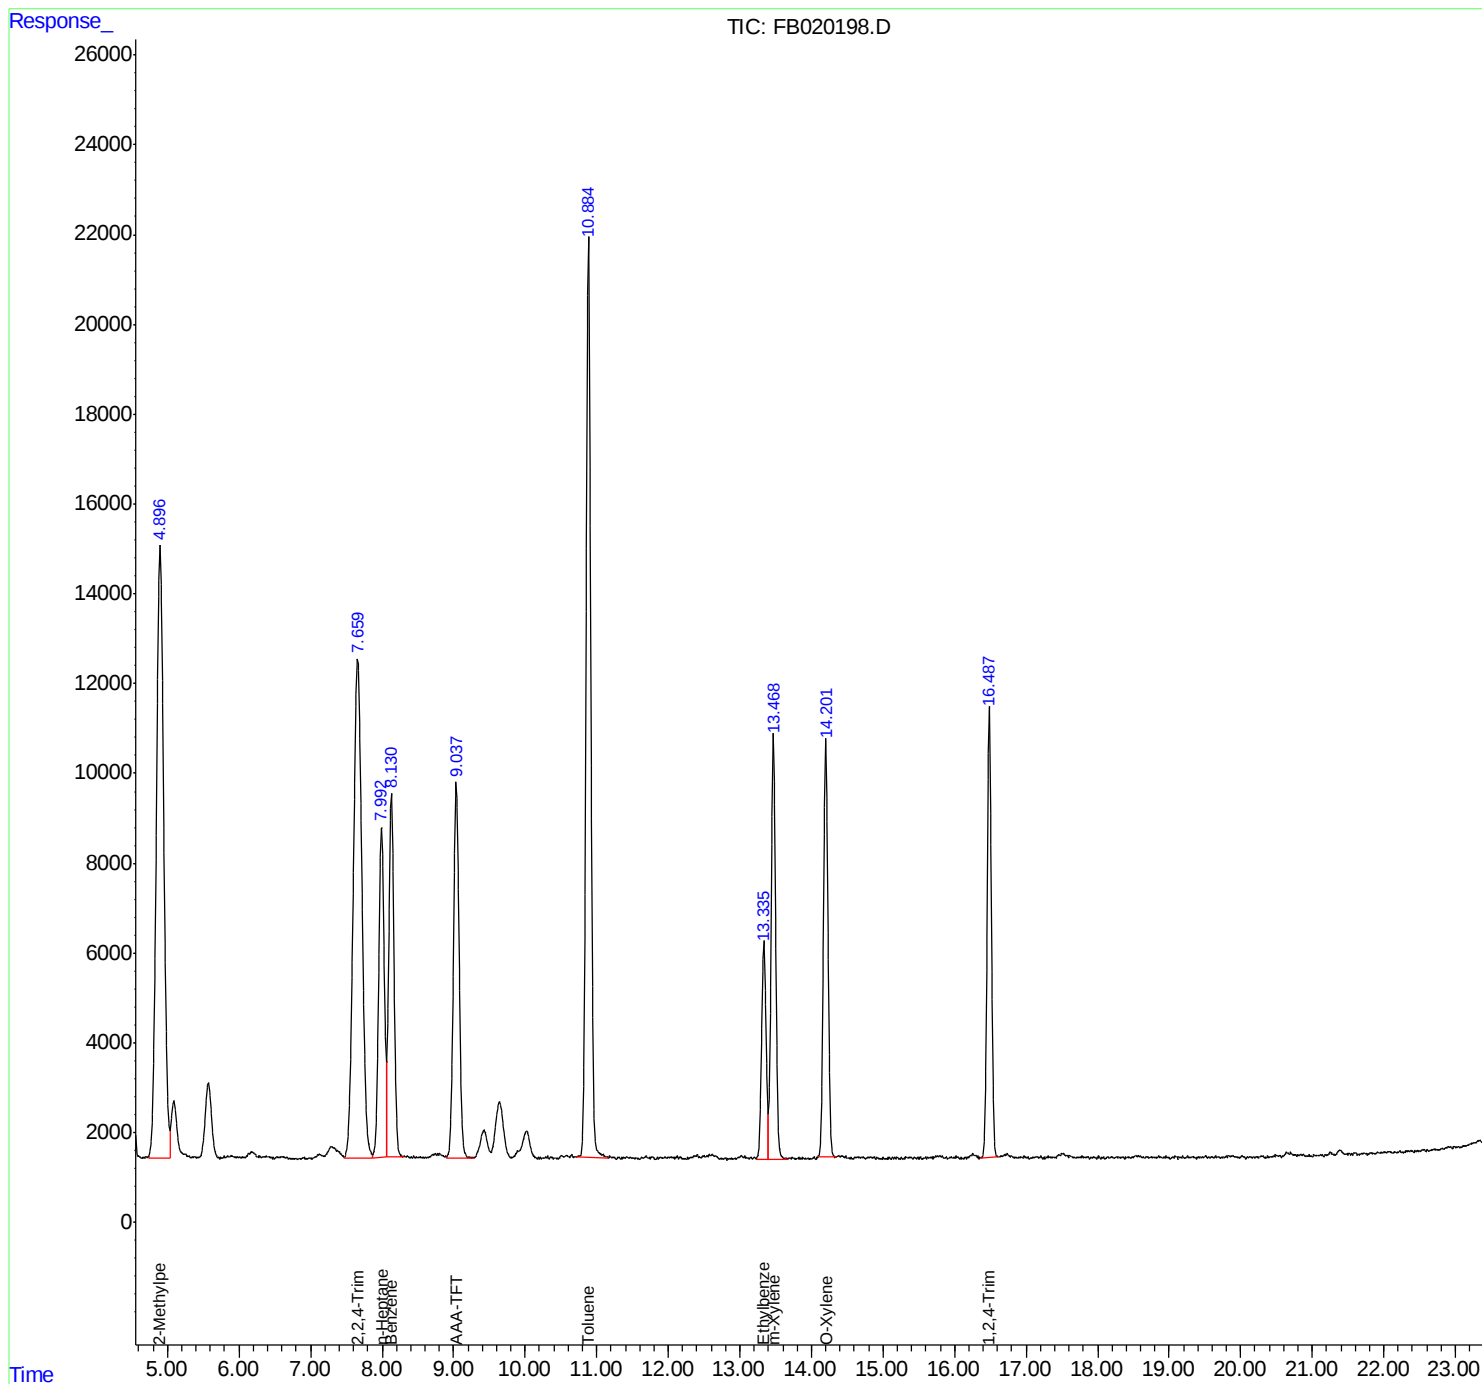

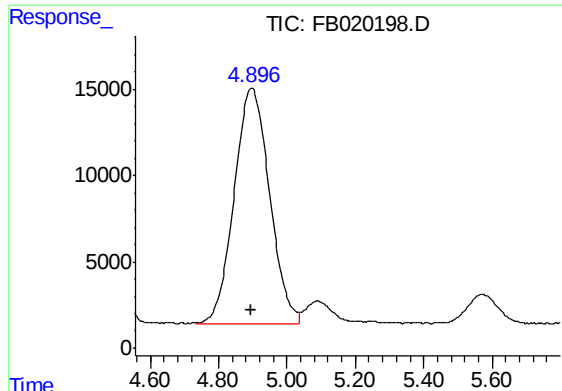


#1 2-Methylpentane

R.T.: 4.897 min
Delta R.T.: 0.003 min
Response: 978968
Conc: 29.02 ng/ml

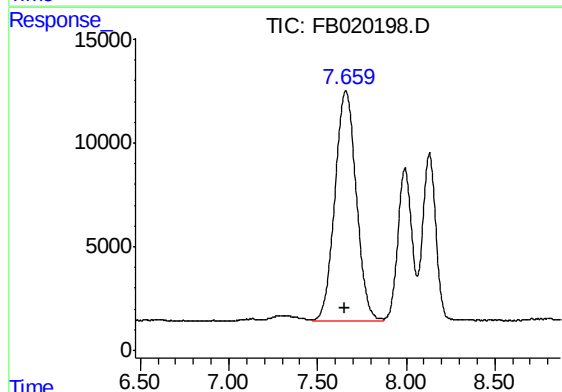


#2 2,2,4-Trimethylpentane

R.T.: 7.660 min
Delta R.T.: 0.002 min
Response: 921473
Conc: 28.10 ng/ml

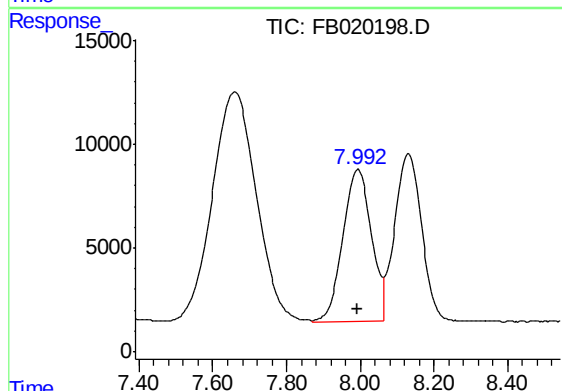


#3 n-Heptane

R.T.: 7.993 min
Delta R.T.: 0.000 min
Response: 395554
Conc: 9.50 ng/ml

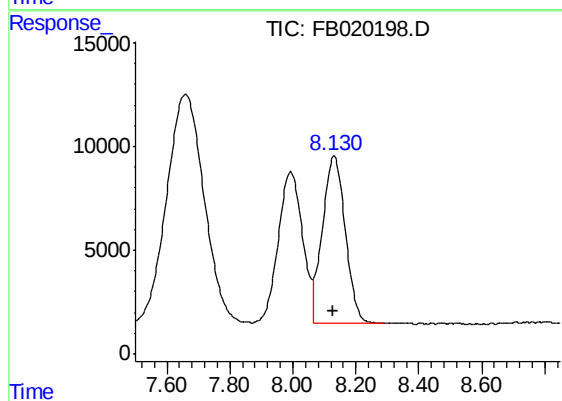


#4 Benzene

R.T.: 8.131 min
Delta R.T.: 0.000 min
Response: 412407
Conc: 8.86 ng/ml

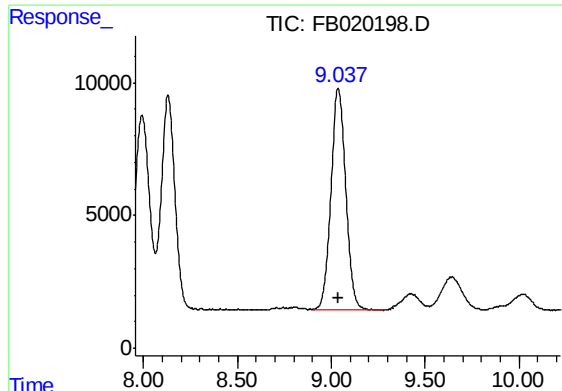


#5 AAA-TFT

R.T.: 9.038 min
Delta R.T.: 0.000 min
Response: 462458
Conc: 17.62 ng/ml

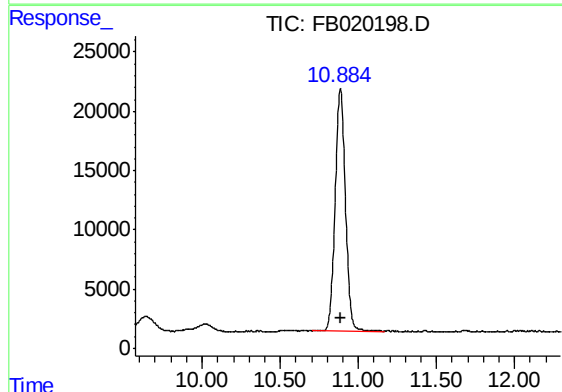


#6 Toluene

R.T.: 10.885 min
Delta R.T.: 0.000 min
Response: 940862
Conc: 25.46 ng/ml

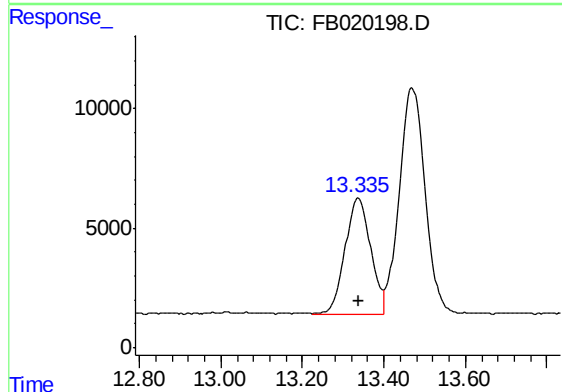


#7 Ethylbenzene

R.T.: 13.337 min
Delta R.T.: 0.000 min
Response: 211419
Conc: 8.99 ng/ml

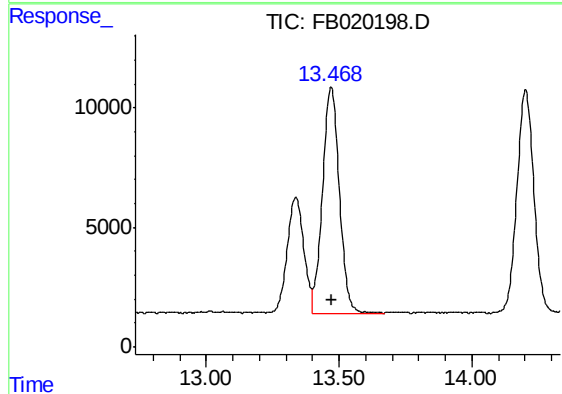


#8 m-Xylene

R.T.: 13.470 min
Delta R.T.: -0.001 min
Response: 418680
Conc: 19.63 ng/ml

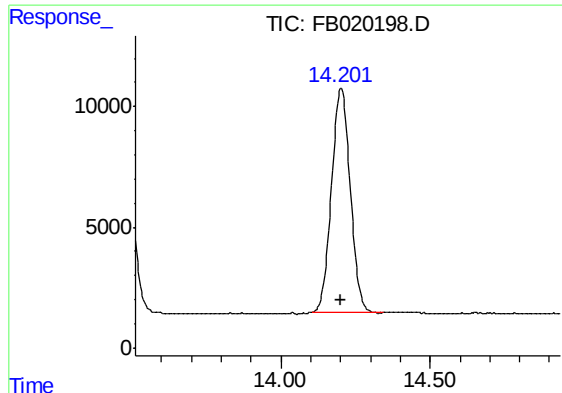

#9 O-Xylene

R.T.: 14.202 min
Delta R.T.: 0.000 min
Response: 405583
Conc: 21.41 ng/ml

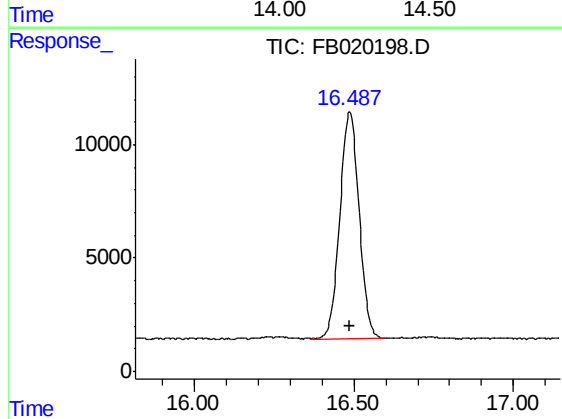

#10 1,2,4-Trimethylbenzene

R.T.: 16.488 min
Delta R.T.: -0.001 min
Response: 417643
Conc: 21.06 ng/ml