

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB031420\
 Data File : FB023935.D
 Signal(s) : FID2B.CH
 Acq On : 14 Mar 2020 10:12
 Operator : DD/AJ
 Sample : BSF0314S1
 Misc : 5.01g/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Mar 16 01:06:42 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030520.M
 Quant Title :
 QLast Update : Thu Mar 05 11:03:12 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.794	443428	21.065 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.686	970669	31.408 ng/ml
2) t 2,2,4-Trimethylpentane	7.414	1100469	32.635 ng/ml
3) t n-Heptane	7.754	353918	10.683 ng/ml
4) t Benzene	7.888	431280	10.300 ng/ml
6) t Toluene	10.626	1289611	31.629 ng/ml
7) t Ethylbenzene	13.066	390498	10.221 ng/ml
8) t m-Xylene	13.199	750636	20.388 ng/ml
9) t O-Xylene	13.927	717497	20.174 ng/ml
10) t 1,2,4-Trimethylbenzene	16.205	611636	20.189 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB031420\
Data File : FB023935.D
Signal(s) : FID2B.CH
Acq On : 14 Mar 2020 10:12
Operator : DD/AJ
Sample : BSF0314S1
Misc : 5.01g/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Mar 16 01:06:42 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030520.M
Quant Title :
QLast Update : Thu Mar 05 11:03:12 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

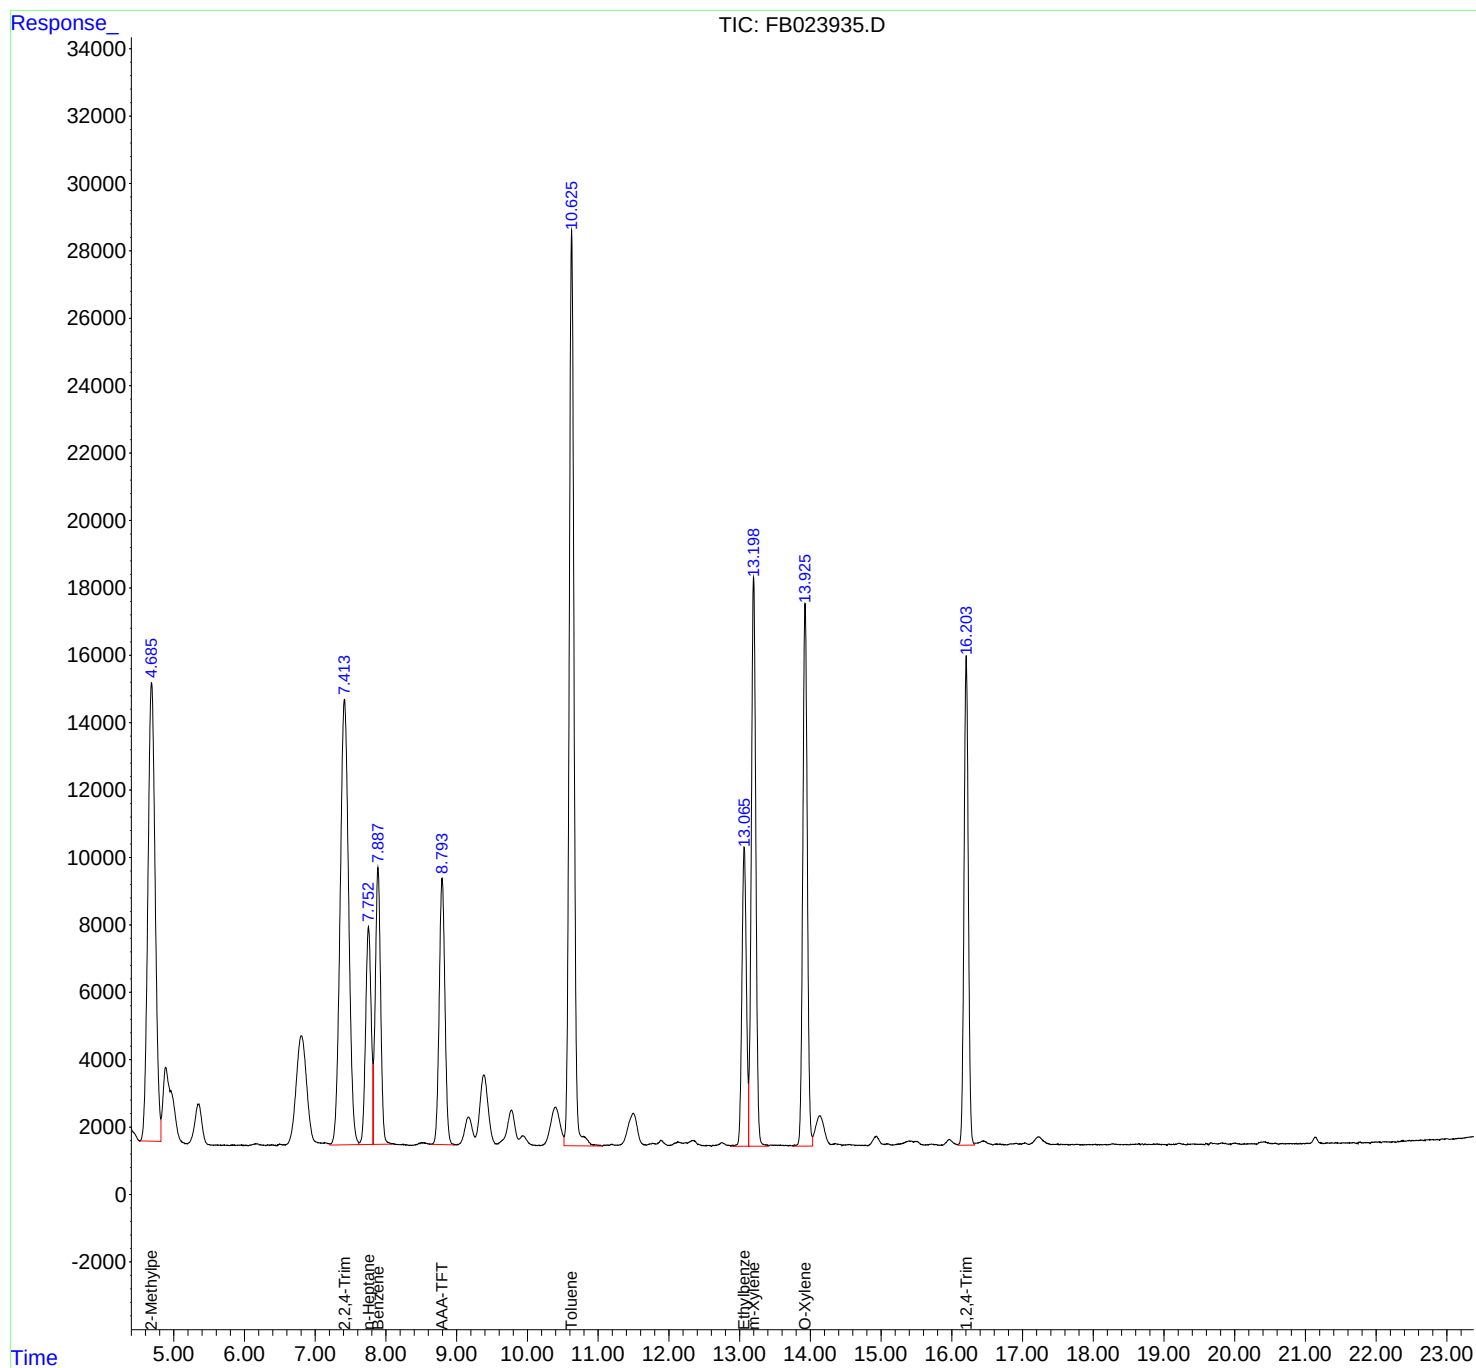

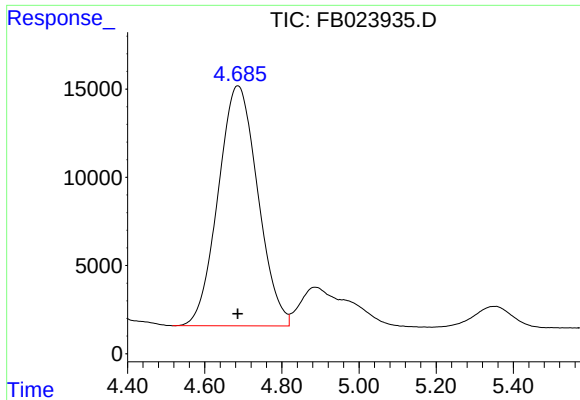


#1 2-Methylpentane

R.T.: 4.686 min
Delta R.T.: 0.000 min
Response: 970669
Conc: 31.41 ng/ml

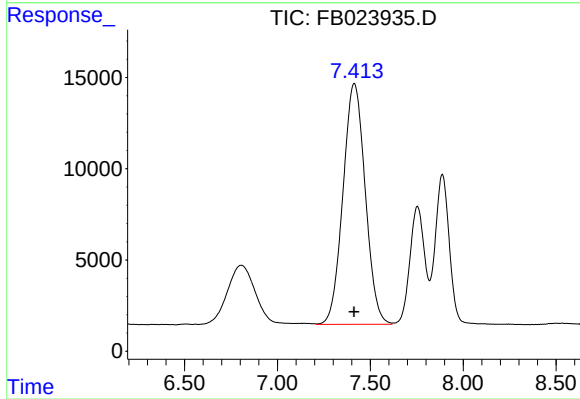


#2 2,2,4-Trimethylpentane

R.T.: 7.414 min
Delta R.T.: 0.001 min
Response: 1100469
Conc: 32.63 ng/ml

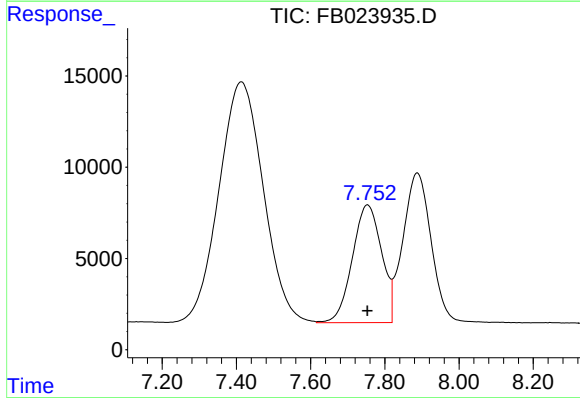


#3 n-Heptane

R.T.: 7.754 min
Delta R.T.: 0.000 min
Response: 353918
Conc: 10.68 ng/ml

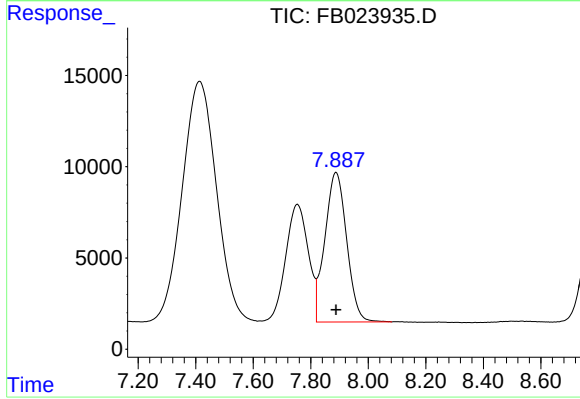


#4 Benzene

R.T.: 7.888 min
Delta R.T.: 0.000 min
Response: 431280
Conc: 10.30 ng/ml

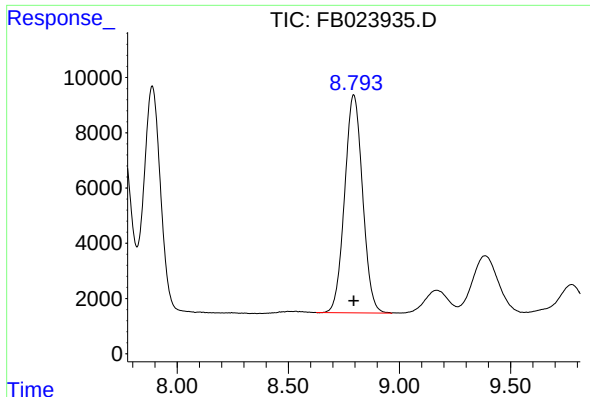


#5 AAA-TFT

R.T.: 8.794 min
Delta R.T.: 0.000 min
Response: 443428
Conc: 21.06 ng/ml

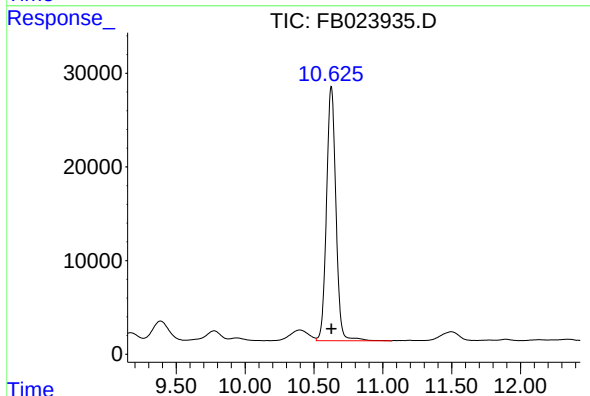


#6 Toluene

R.T.: 10.626 min
Delta R.T.: 0.000 min
Response: 1289611
Conc: 31.63 ng/ml

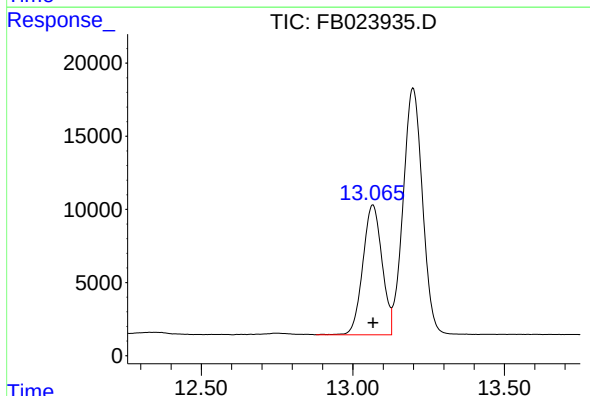


#7 Ethylbenzene

R.T.: 13.066 min
Delta R.T.: 0.000 min
Response: 390498
Conc: 10.22 ng/ml

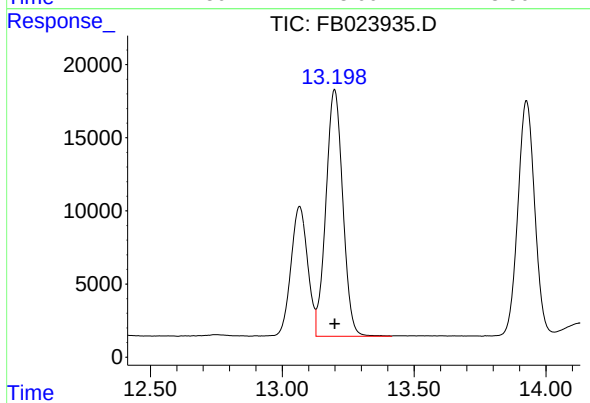


#8 m-Xylene

R.T.: 13.199 min
Delta R.T.: 0.000 min
Response: 750636
Conc: 20.39 ng/ml

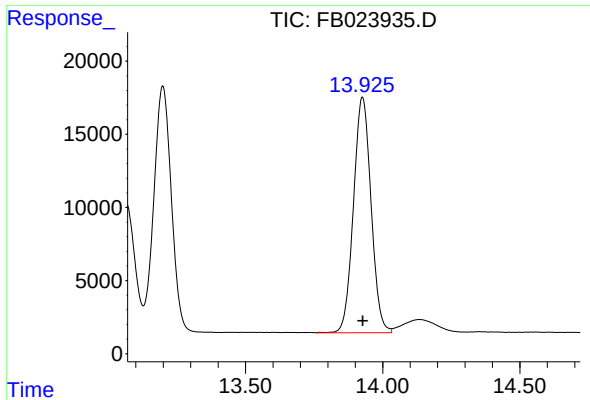

#9 O-Xylene

R.T.: 13.927 min
Delta R.T.: 0.000 min
Response: 717497
Conc: 20.17 ng/ml

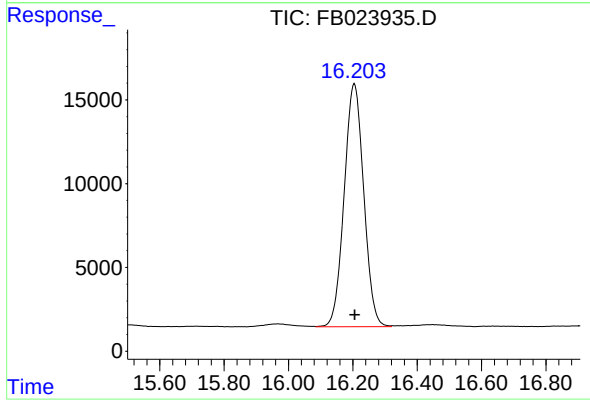

#10 1,2,4-Trimethylbenzene

R.T.: 16.205 min
Delta R.T.: 0.000 min
Response: 611636
Conc: 20.19 ng/ml