

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB031420\
Data File : FB023936.D
Signal(s) : FID2B.CH
Acq On : 14 Mar 2020 11:19
Operator : DD/AJ
Sample : L1942-02
Misc : 5.02g/5.00ml DI WATER
ALS Vial : 4 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Mar 16 01:06:48 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030520.M
Quant Title :
QLast Update : Thu Mar 05 11:03:12 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.794	454784	21.604 ng/ml
Target Compounds			
6) t Toluene	10.629	766	0.019 ng/ml
9) t O-Xylene	13.925	2321	0.065 ng/ml
10) t 1,2,4-Trimethylbenzene	16.215	4603	0.152 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB031420\
Data File : FB023936.D
Signal(s) : FID2B.CH
Acq On : 14 Mar 2020 11:19
Operator : DD/AJ
Sample : L1942-02
Misc : 5.02g/5.00ml DI WATER
ALS Vial : 4 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Mar 16 01:06:48 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030520.M
Quant Title :
QLast Update : Thu Mar 05 11:03:12 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

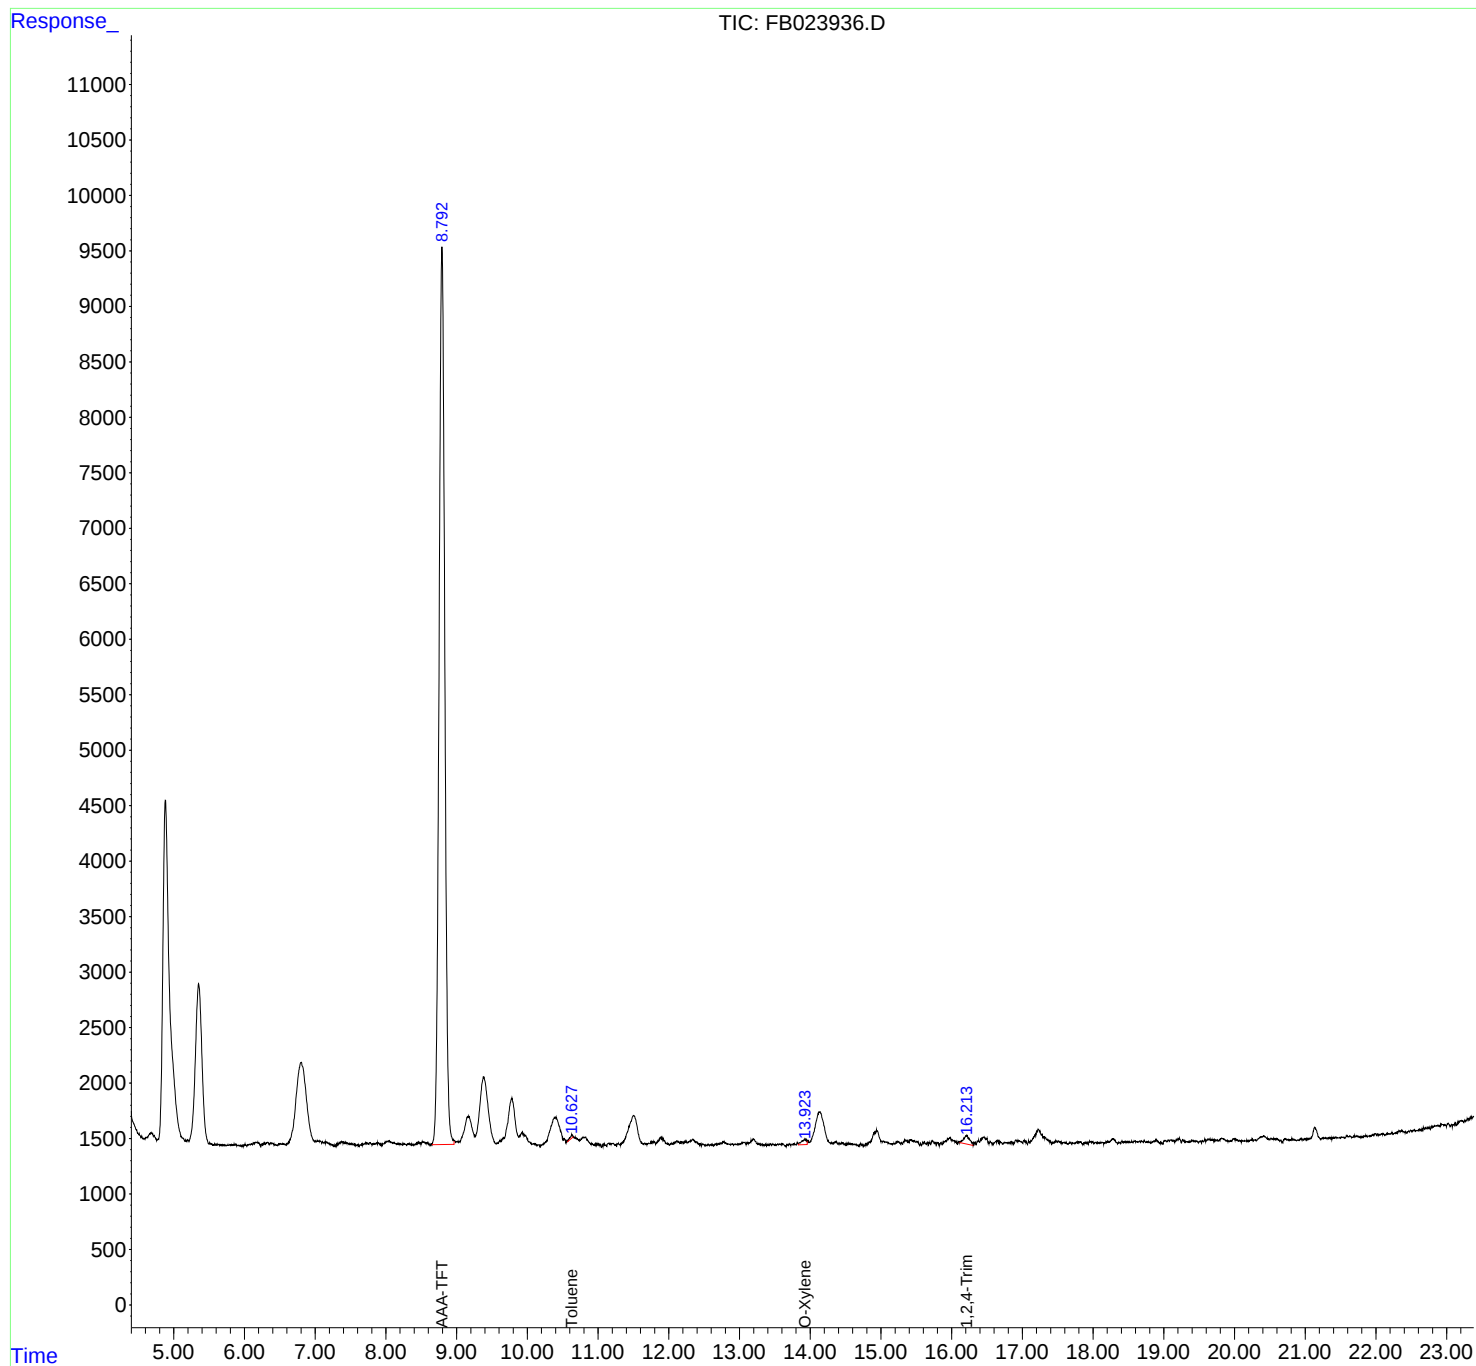

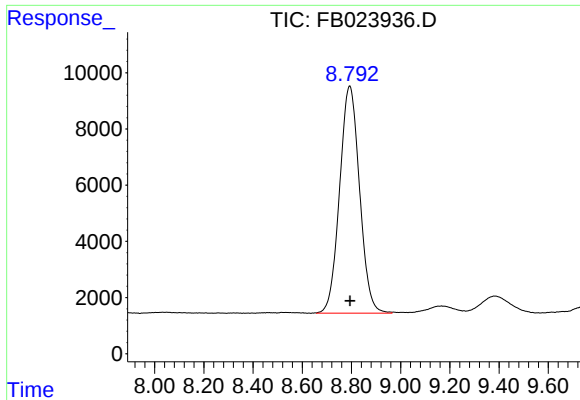


#5 AAA-TFT

R.T.: 8.794 min
Delta R.T.: 0.000 min
Response: 454784
Conc: 21.60 ng/ml

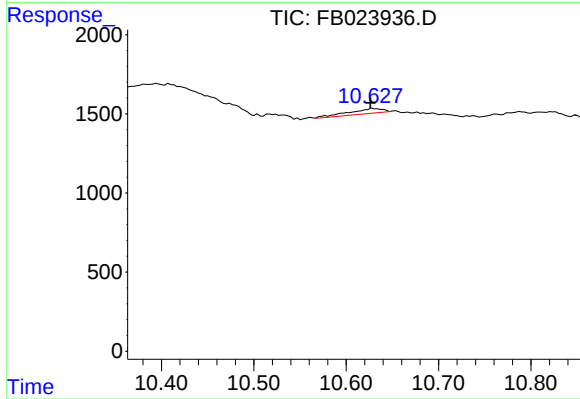


#6 Toluene

R.T.: 10.629 min
Delta R.T.: 0.003 min
Response: 766
Conc: 0.02 ng/ml

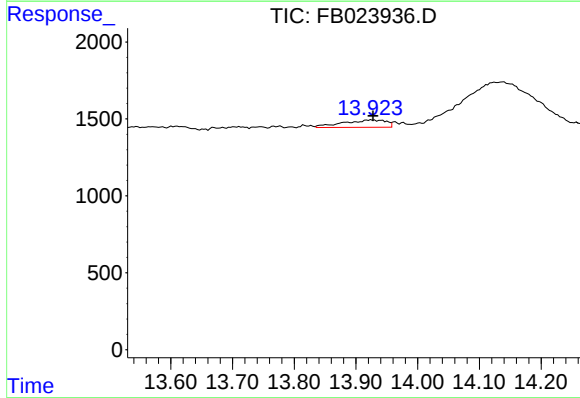

#9 O-Xylene

R.T.: 13.925 min
Delta R.T.: -0.003 min
Response: 2321
Conc: 0.07 ng/ml

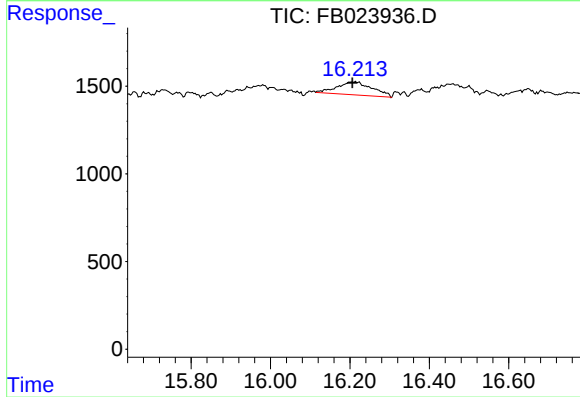

#10 1,2,4-Trimethylbenzene

R.T.: 16.215 min
Delta R.T.: 0.009 min
Response: 4603
Conc: 0.15 ng/ml