

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB031420\
 Data File : FB023941.D
 Signal(s) : FID2B.CH
 Acq On : 14 Mar 2020 13:51
 Operator : DD/AJ
 Sample : L1942-14
 Misc : 5.04g/5.00ml DI WATER
 ALS Vial : 9 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Mar 16 01:07:04 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030520.M
 Quant Title :
 QLast Update : Thu Mar 05 11:03:12 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.796	414362	19.684 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.679	1652	0.053 ng/ml
2) t 2,2,4-Trimethylpentane	7.417	280	0.008 ng/ml
6) t Toluene	10.626	172	0.004 ng/ml
8) t m-Xylene	13.198	3631	0.099 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB031420\
Data File : FB023941.D
Signal(s) : FID2B.CH
Acq On : 14 Mar 2020 13:51
Operator : DD/AJ
Sample : L1942-14
Misc : 5.04g/5.00ml DI WATER
ALS Vial : 9 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Mar 16 01:07:04 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030520.M
Quant Title :
QLast Update : Thu Mar 05 11:03:12 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

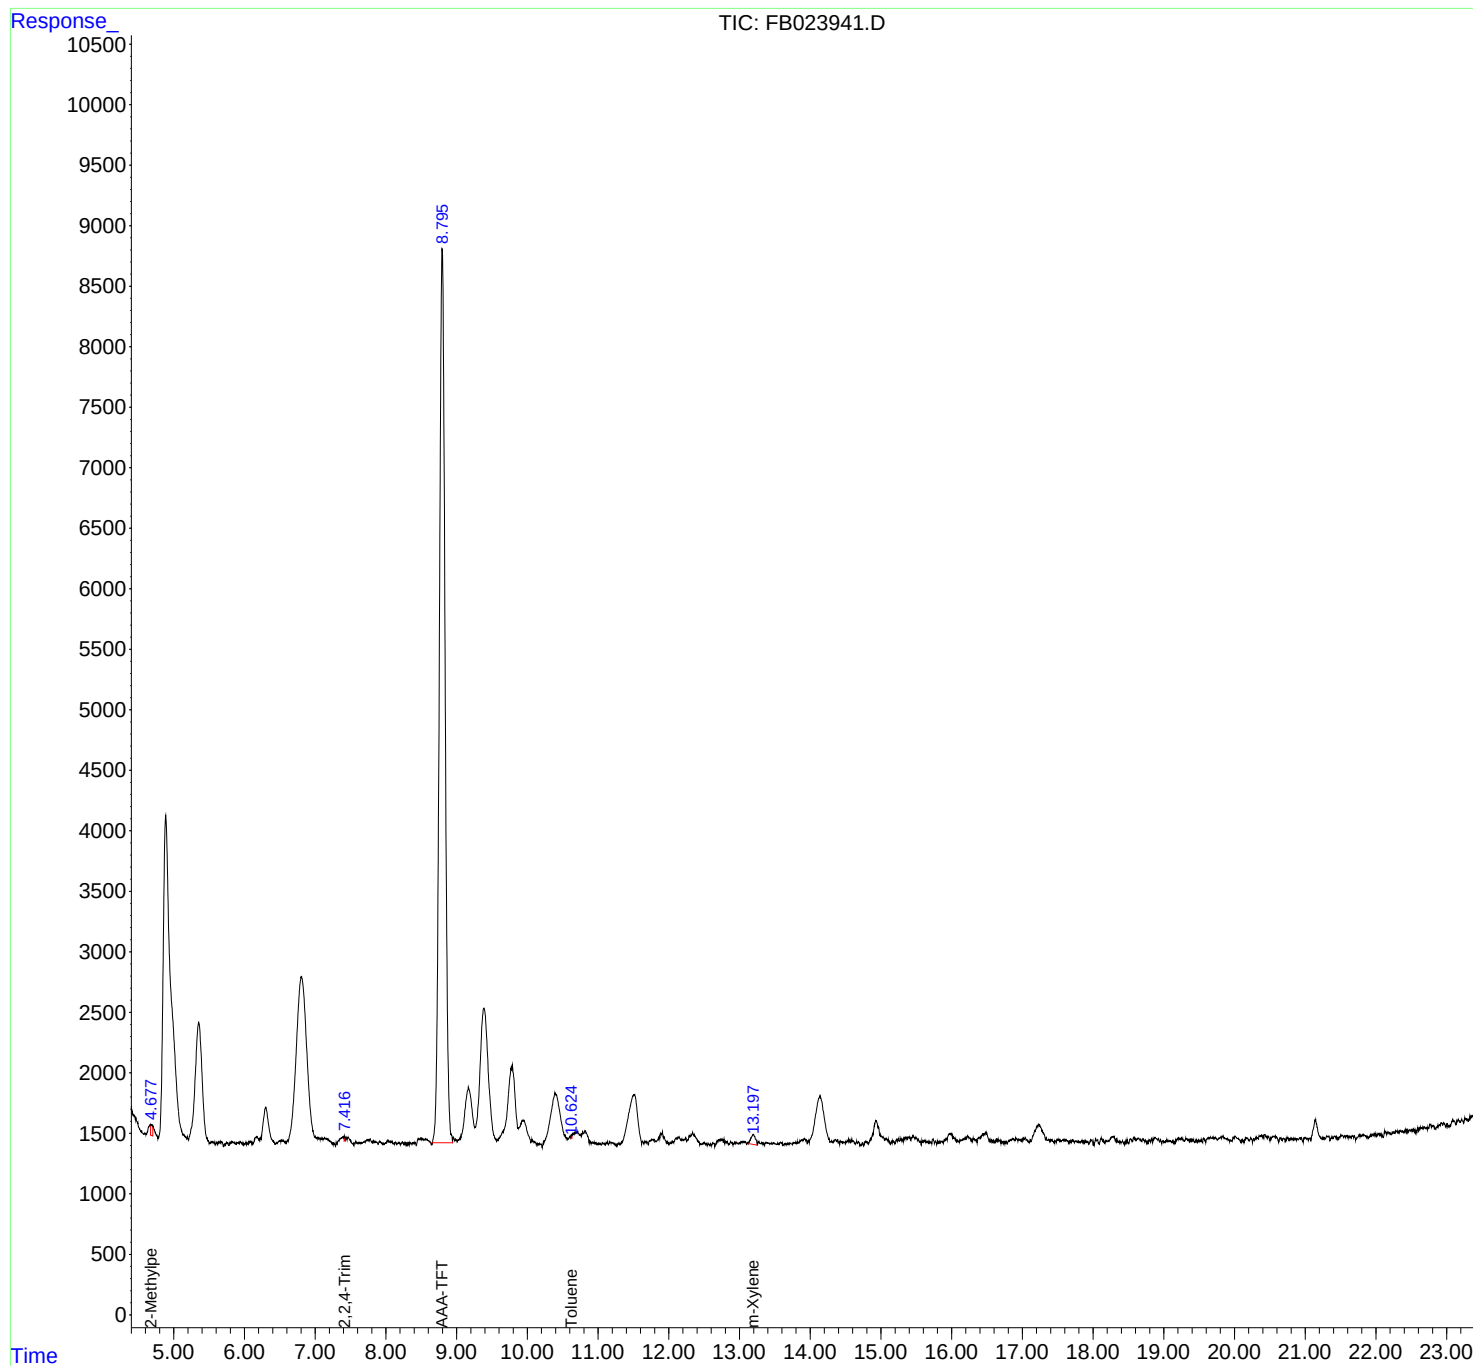

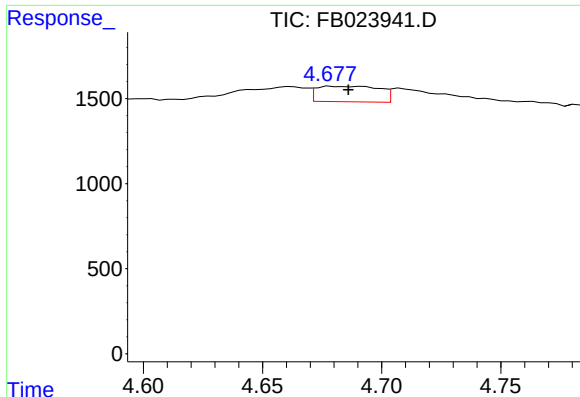


#1 2-Methylpentane

R.T.: 4.679 min
Delta R.T.: -0.007 min
Response: 1652
Conc: 0.05 ng/ml

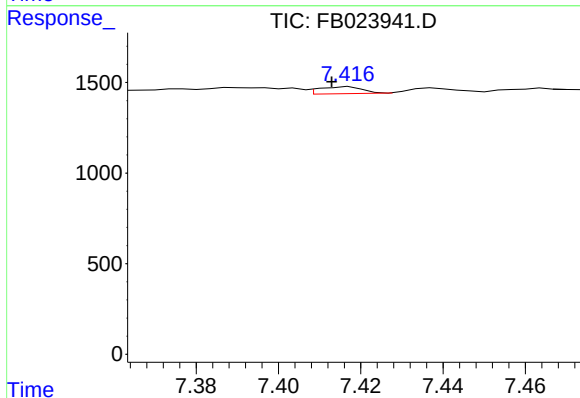


#2 2,2,4-Trimethylpentane

R.T.: 7.417 min
Delta R.T.: 0.004 min
Response: 280
Conc: 0.01 ng/ml

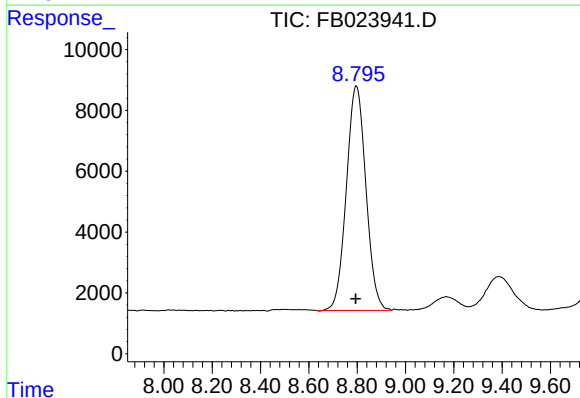


#5 AAA-TFT

R.T.: 8.796 min
Delta R.T.: 0.002 min
Response: 414362
Conc: 19.68 ng/ml

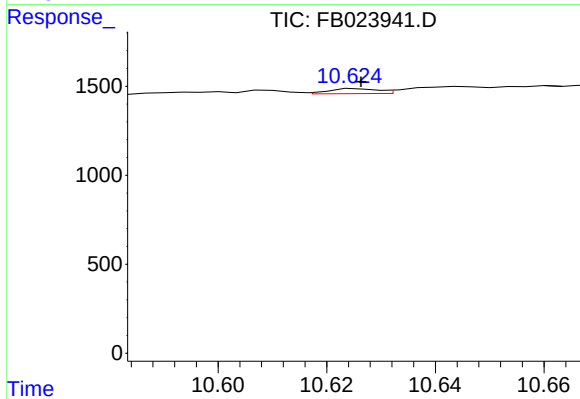

#6 Toluene

R.T.: 10.626 min
Delta R.T.: 0.000 min
Response: 172
Conc: 0.00 ng/ml

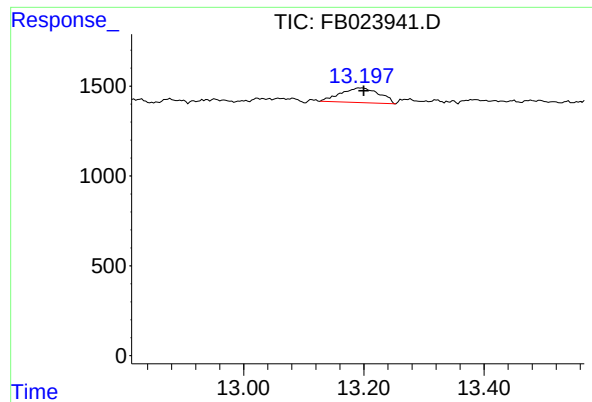

#8 m-Xylene

R.T.: 13.198 min
Delta R.T.: -0.002 min
Response: 3631
Conc: 0.10 ng/ml