

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB031420\
 Data File : FB023947.D
 Signal(s) : FID2B.CH
 Acq On : 14 Mar 2020 16:53
 Operator : DD/AJ
 Sample : L1942-02MSD
 Misc : 5.04g/5.00ml DI WATER
 ALS Vial : 15 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Mar 16 01:07:29 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030520.M
 Quant Title :
 QLast Update : Thu Mar 05 11:03:12 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.796	418660	19.888 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.688	845962	27.373 ng/ml
2) t 2,2,4-Trimethylpentane	7.415	907328	26.907 ng/ml
3) t n-Heptane	7.756	293337	8.854 ng/ml
4) t Benzene	7.890	401177	9.581 ng/ml
6) t Toluene	10.627	1150727	28.222 ng/ml
7) t Ethylbenzene	13.067	345044	9.031 ng/ml
8) t m-Xylene	13.201	674396	18.318 ng/ml
9) t O-Xylene	13.928	650882	18.301 ng/ml
10) t 1,2,4-Trimethylbenzene	16.207	543644	17.945 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB031420\
Data File : FB023947.D
Signal(s) : FID2B.CH
Acq On : 14 Mar 2020 16:53
Operator : DD/AJ
Sample : L1942-02MSD
Misc : 5.04g/5.00ml DI WATER
ALS Vial : 15 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Mar 16 01:07:29 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030520.M
Quant Title :
QLast Update : Thu Mar 05 11:03:12 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

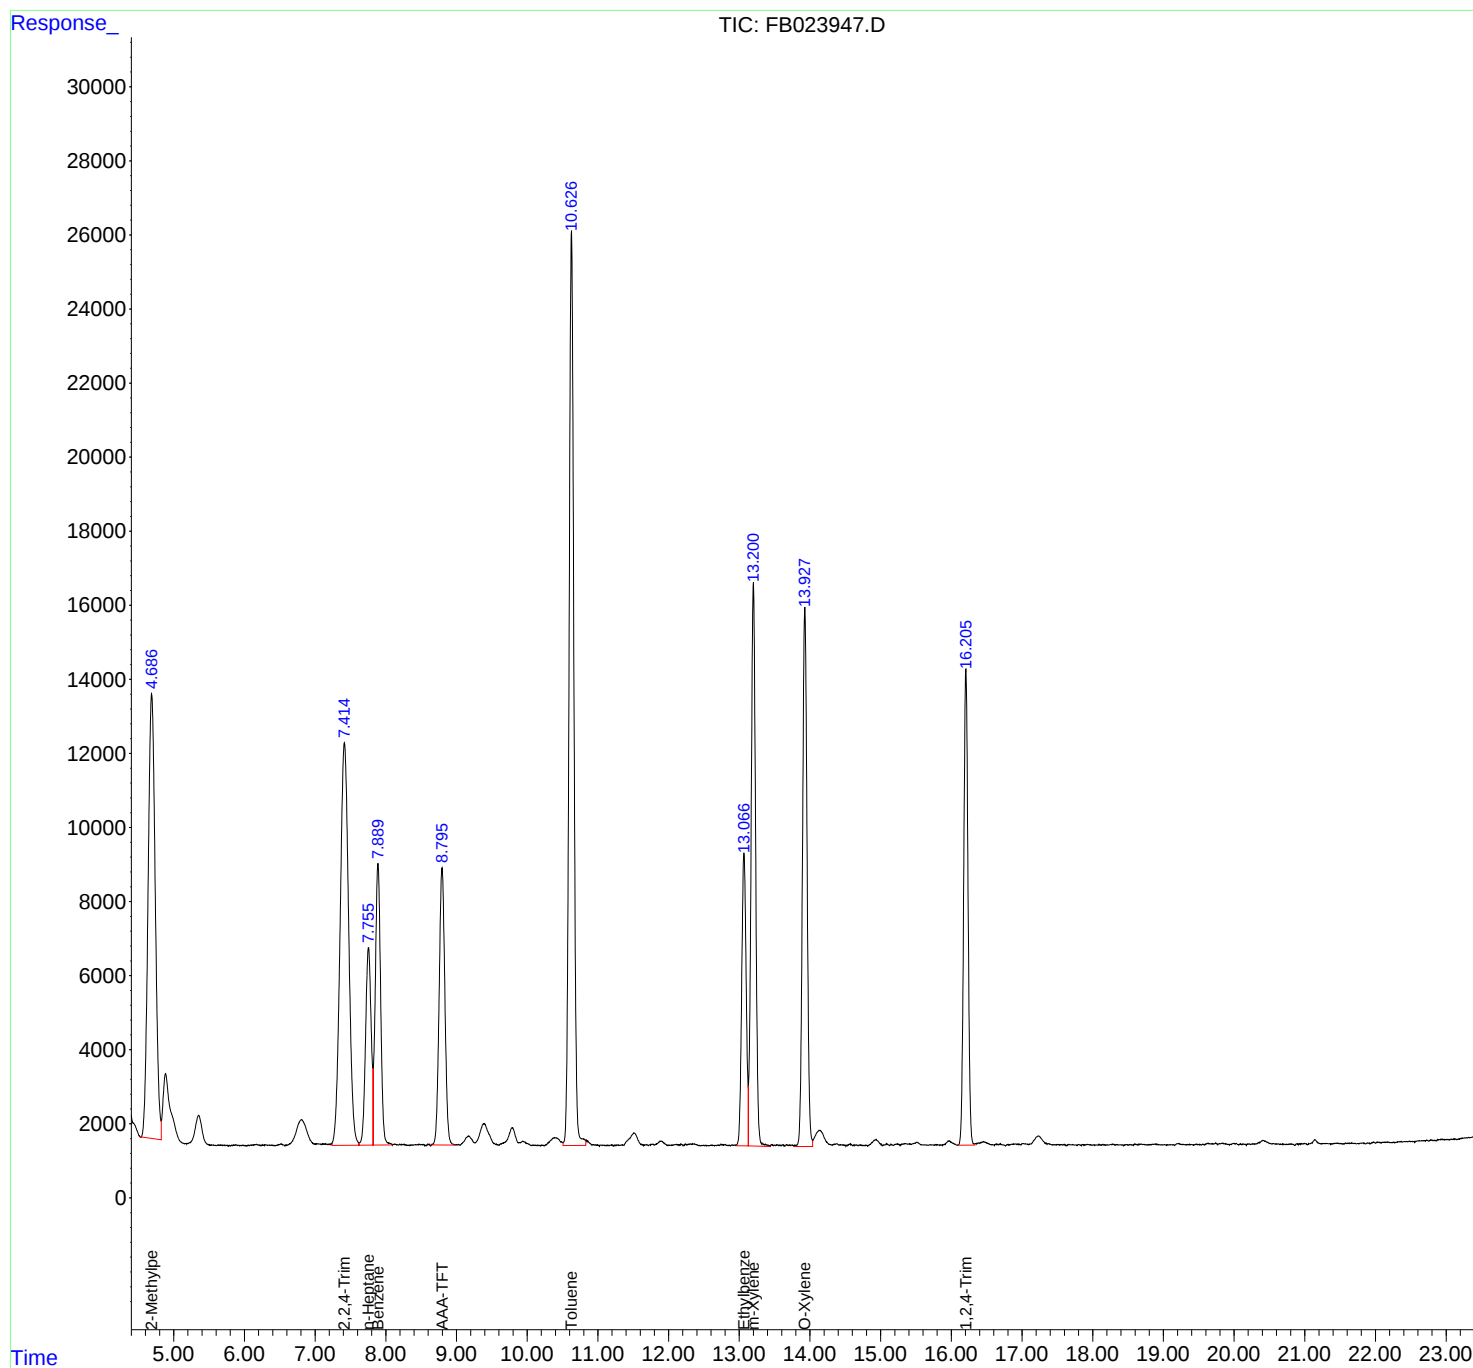

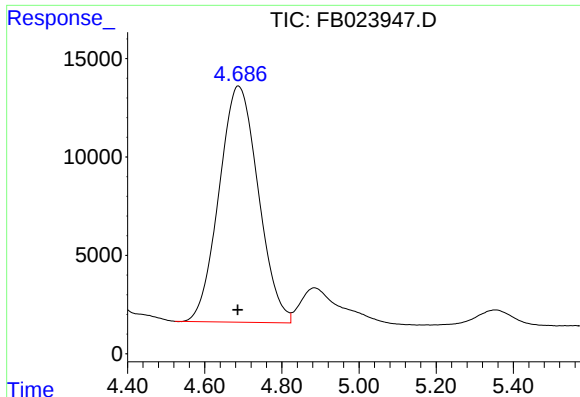


#1 2-Methylpentane

R.T.: 4.688 min
Delta R.T.: 0.002 min
Response: 845962
Conc: 27.37 ng/ml

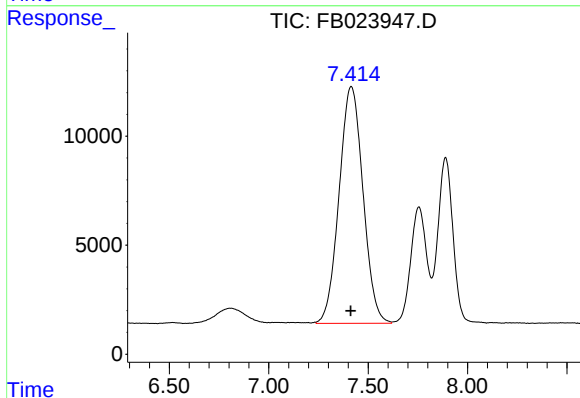


#2 2,2,4-Trimethylpentane

R.T.: 7.415 min
Delta R.T.: 0.002 min
Response: 907328
Conc: 26.91 ng/ml

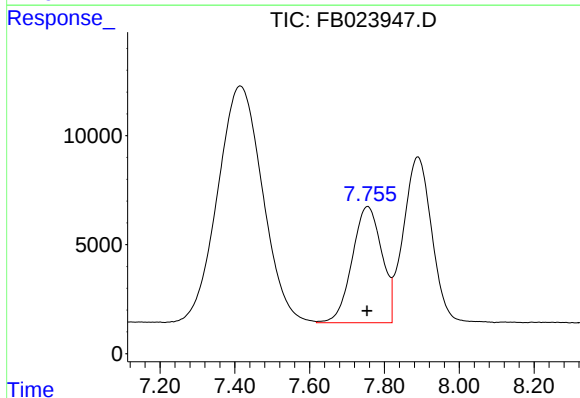


#3 n-Heptane

R.T.: 7.756 min
Delta R.T.: 0.002 min
Response: 293337
Conc: 8.85 ng/ml

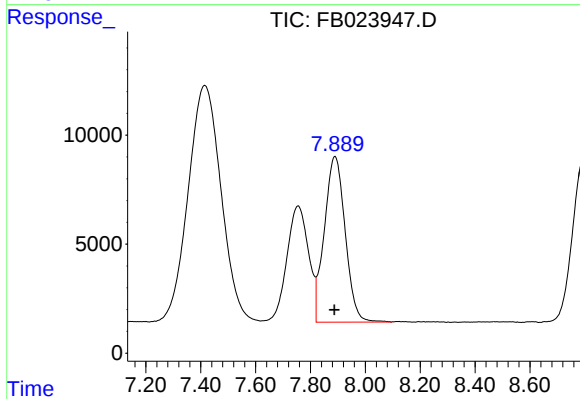


#4 Benzene

R.T.: 7.890 min
Delta R.T.: 0.002 min
Response: 401177
Conc: 9.58 ng/ml

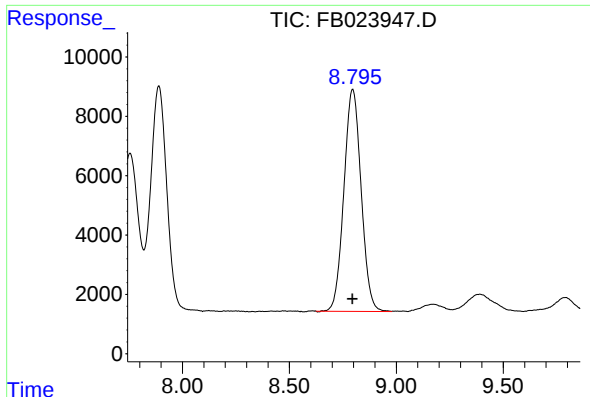


#5 AAA-TFT

R.T.: 8.796 min
Delta R.T.: 0.002 min
Response: 418660
Conc: 19.89 ng/ml

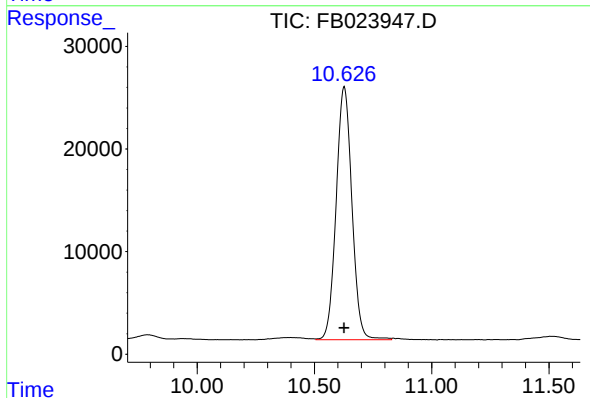


#6 Toluene

R.T.: 10.627 min
Delta R.T.: 0.001 min
Response: 1150727
Conc: 28.22 ng/ml

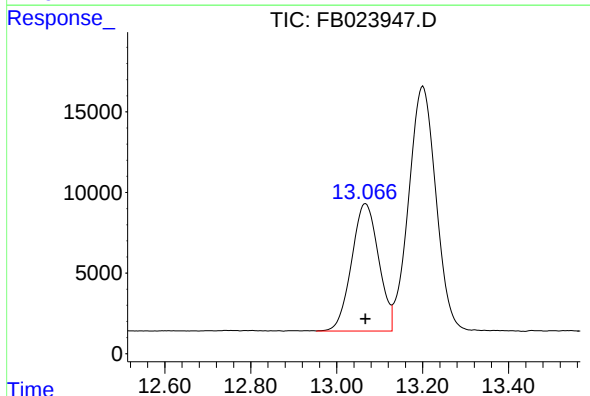


#7 Ethylbenzene

R.T.: 13.067 min
Delta R.T.: 0.000 min
Response: 345044
Conc: 9.03 ng/ml

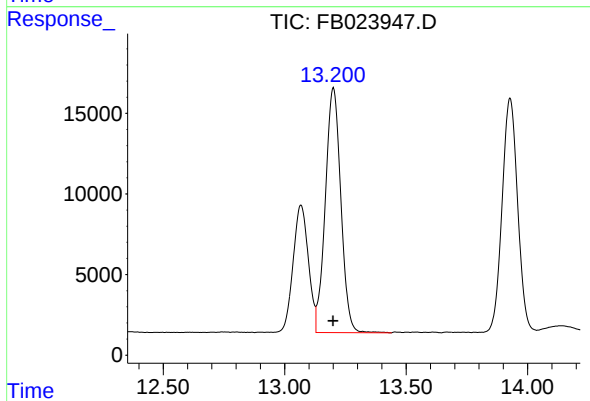


#8 m-Xylene

R.T.: 13.201 min
Delta R.T.: 0.000 min
Response: 674396
Conc: 18.32 ng/ml

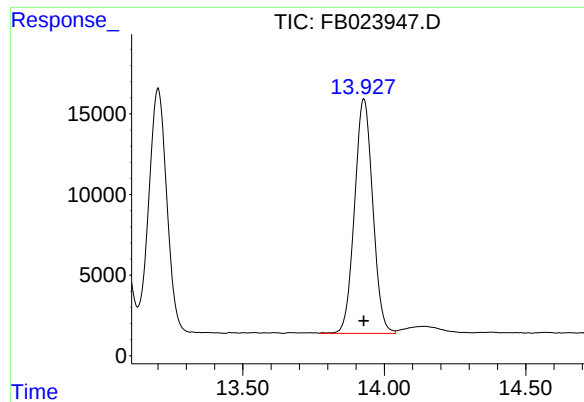

#9 O-Xylene

R.T.: 13.928 min
Delta R.T.: 0.000 min
Response: 650882
Conc: 18.30 ng/ml

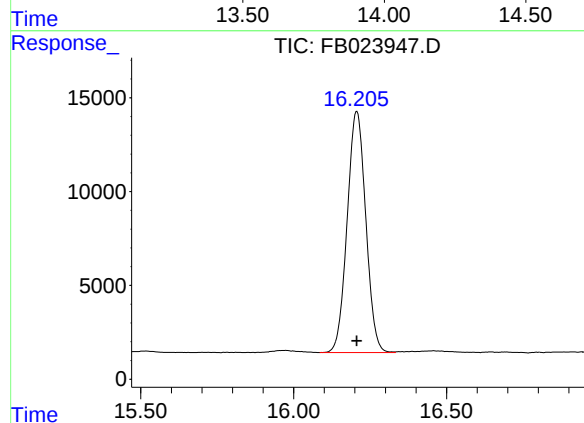

#10 1,2,4-Trimethylbenzene

R.T.: 16.207 min
Delta R.T.: 0.000 min
Response: 543644
Conc: 17.94 ng/ml