

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB031423\
 Data File : FB029475.D
 Signal(s) : FID2B.CH
 Acq On : 14 Mar 2023 11:24
 Operator : YP/AJ
 Sample : 01892-03 50X
 Misc : 5.09G/5.00 ML MEOH
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Mar 14 16:26:35 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030123.M
 Quant Title :
 QLast Update : Wed Mar 01 12:30:24 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.802	339576	28.028 ng/ml
Target Compounds			
2) t 2,2,4-Trimethylpentane	7.389	10114	0.600 ng/ml
3) t n-Heptane	7.755	31610	1.828 ng/ml
4) t Benzene	7.890	26446	1.303 ng/ml
6) t Toluene	10.627	325806	16.506 ng/ml
7) t Ethylbenzene	13.061	1686447	90.585 ng/ml
8) t m-Xylene	13.196	4272460	229.658 ng/ml
9) t O-Xylene	13.925	3552327	192.924 ng/ml
10) t 1,2,4-Trimethylbenzene	16.207	23015092	1235.658 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB031423\
Data File : FB029475.D
Signal(s) : FID2B.CH
Acq On : 14 Mar 2023 11:24
Operator : YP/AJ
Sample : 01892-03 50X
Misc : 5.09G/5.00 ML MEOH
ALS Vial : 8 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Mar 14 16:26:35 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030123.M
Quant Title :
QLast Update : Wed Mar 01 12:30:24 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

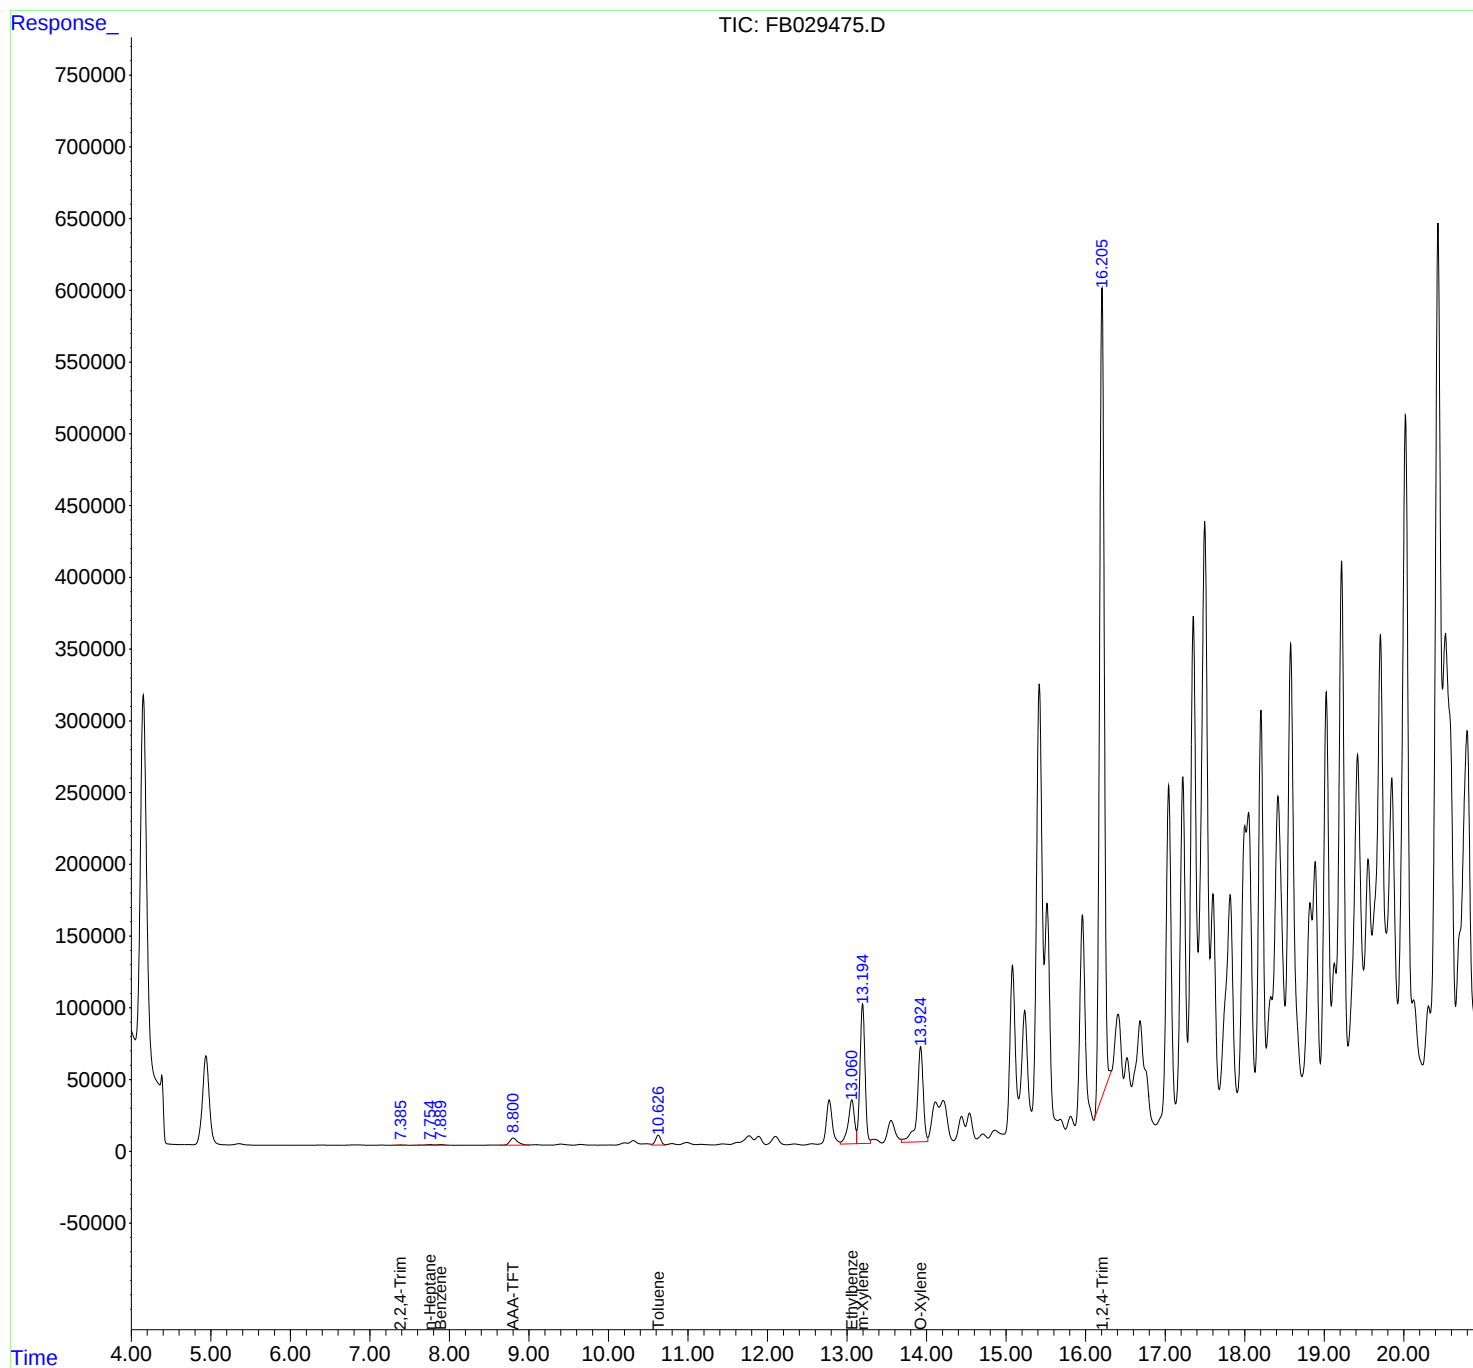


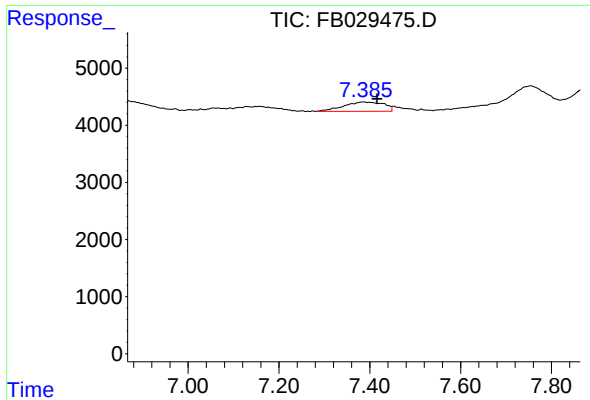

#2 2,2,4-Trimethylpentane


R.T.: 7.389 min
Delta R.T.: -0.027 min
Response: 10114
Conc: 0.60 ng/ml

Instrument :
FID_B
ClientSampleId :

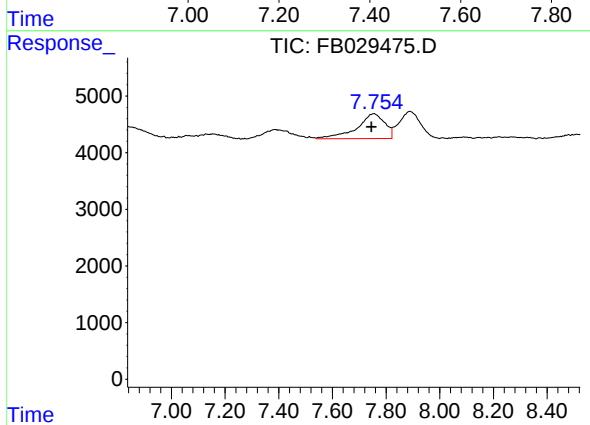


#3 n-Heptane

R.T.: 7.755 min
Delta R.T.: 0.009 min
Response: 31610
Conc: 1.83 ng/ml

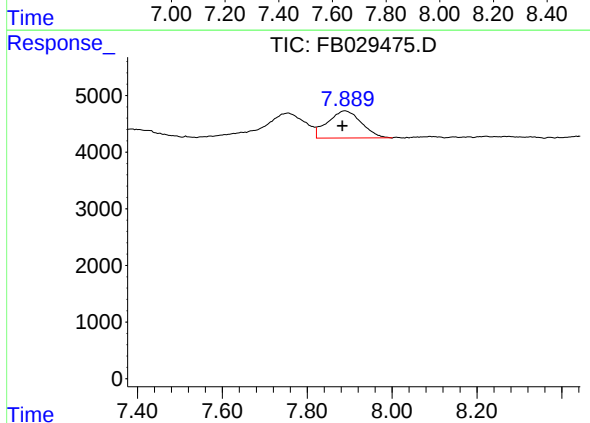


#4 Benzene

R.T.: 7.890 min
Delta R.T.: 0.006 min
Response: 26446
Conc: 1.30 ng/ml

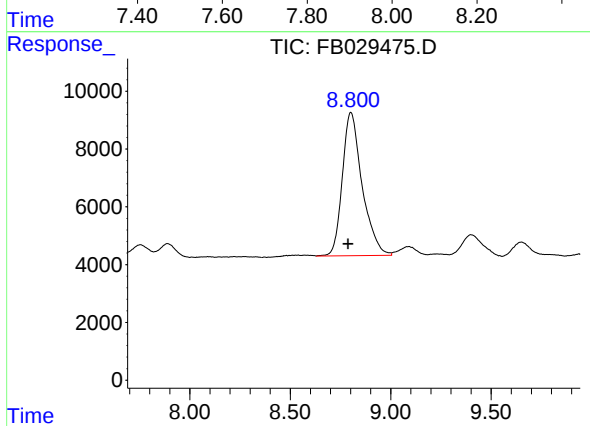

#5 AAA-TFT


R.T.: 8.802 min
Delta R.T.: 0.014 min
Response: 339576
Conc: 28.03 ng/ml

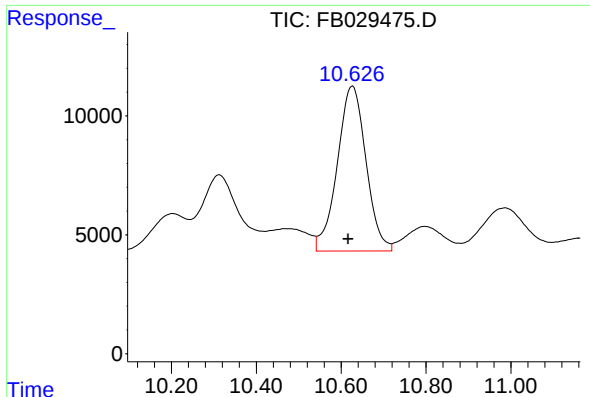

#6 Toluene


R.T.: 10.627 min
Delta R.T.: 0.011 min
Response: 325806
Conc: 16.51 ng/ml

Instrument :
FID_B
ClientSampleId :

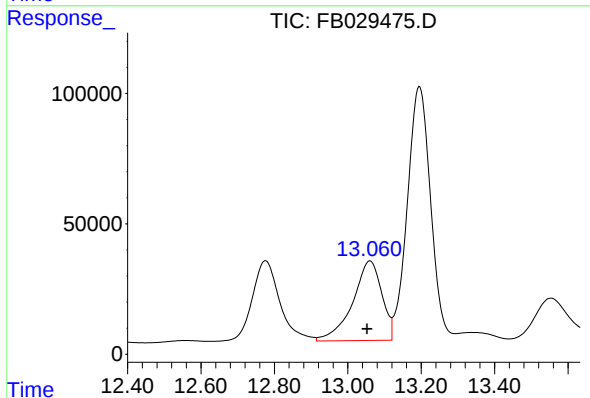


#7 Ethylbenzene

R.T.: 13.061 min
Delta R.T.: 0.008 min
Response: 1686447
Conc: 90.58 ng/ml

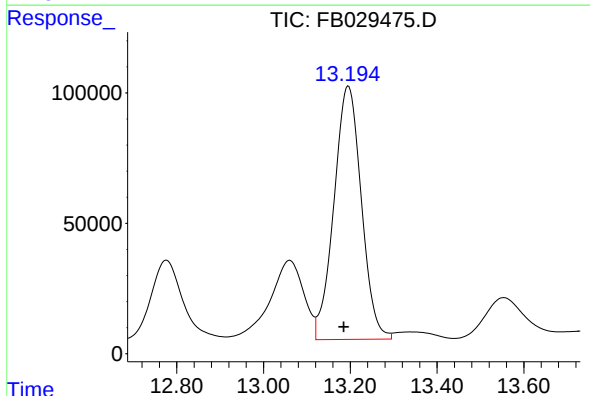


#8 m-Xylene

R.T.: 13.196 min
Delta R.T.: 0.011 min
Response: 4272460
Conc: 229.66 ng/ml

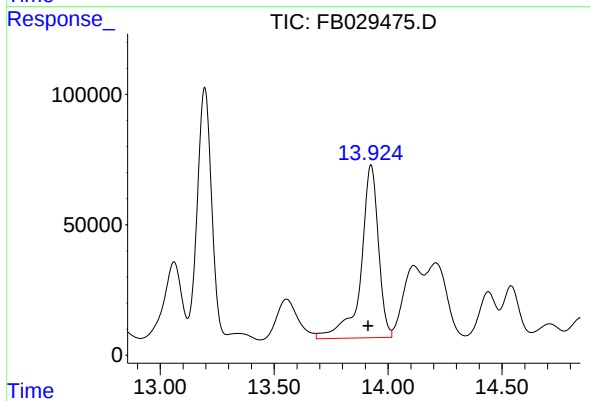

#9 O-Xylene

R.T.: 13.925 min
Delta R.T.: 0.013 min
Response: 3552327
Conc: 192.92 ng/ml

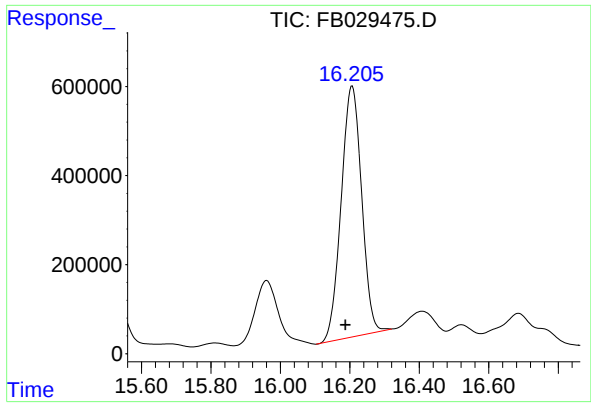

#10 1,2,4-Trimethylbenzene

R.T.: 16.207 min
Delta R.T.: 0.020 min
Response: 23015092
Conc: 1235.66 ng/ml

Instrument :
FID_B
ClientSampleId :