

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB031423\
 Data File : FB029477.D
 Signal(s) : FID2B.CH
 Acq On : 14 Mar 2023 12:40
 Operator : YP/AJ
 Sample : 01892-01 10X
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Mar 14 16:26:45 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030123.M
 Quant Title :
 QLast Update : Wed Mar 01 12:30:24 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	8.802	367881	30.364 ng/ml
Target Compounds				
2) t	2,2,4-Trimethylpentane	7.399	9982	0.593 ng/ml
3) t	n-Heptane	7.762	36565	2.114 ng/ml
4) t	Benzene	7.893	22038	1.086 ng/ml
6) t	Toluene	10.627	113317	5.741 ng/ml
7) t	Ethylbenzene	13.042	2025761	108.810 ng/ml
8) t	m-Xylene	13.193	1421635	76.417 ng/ml
9) t	O-Xylene	13.925	1460362	79.311 ng/ml
10) t	1,2,4-Trimethylbenzene	16.207	7304834	392.189 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB031423\
Data File : FB029477.D
Signal(s) : FID2B.CH
Acq On : 14 Mar 2023 12:40
Operator : YP/AJ
Sample : 01892-01 10X
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Mar 14 16:26:45 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030123.M
Quant Title :
QLast Update : Wed Mar 01 12:30:24 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

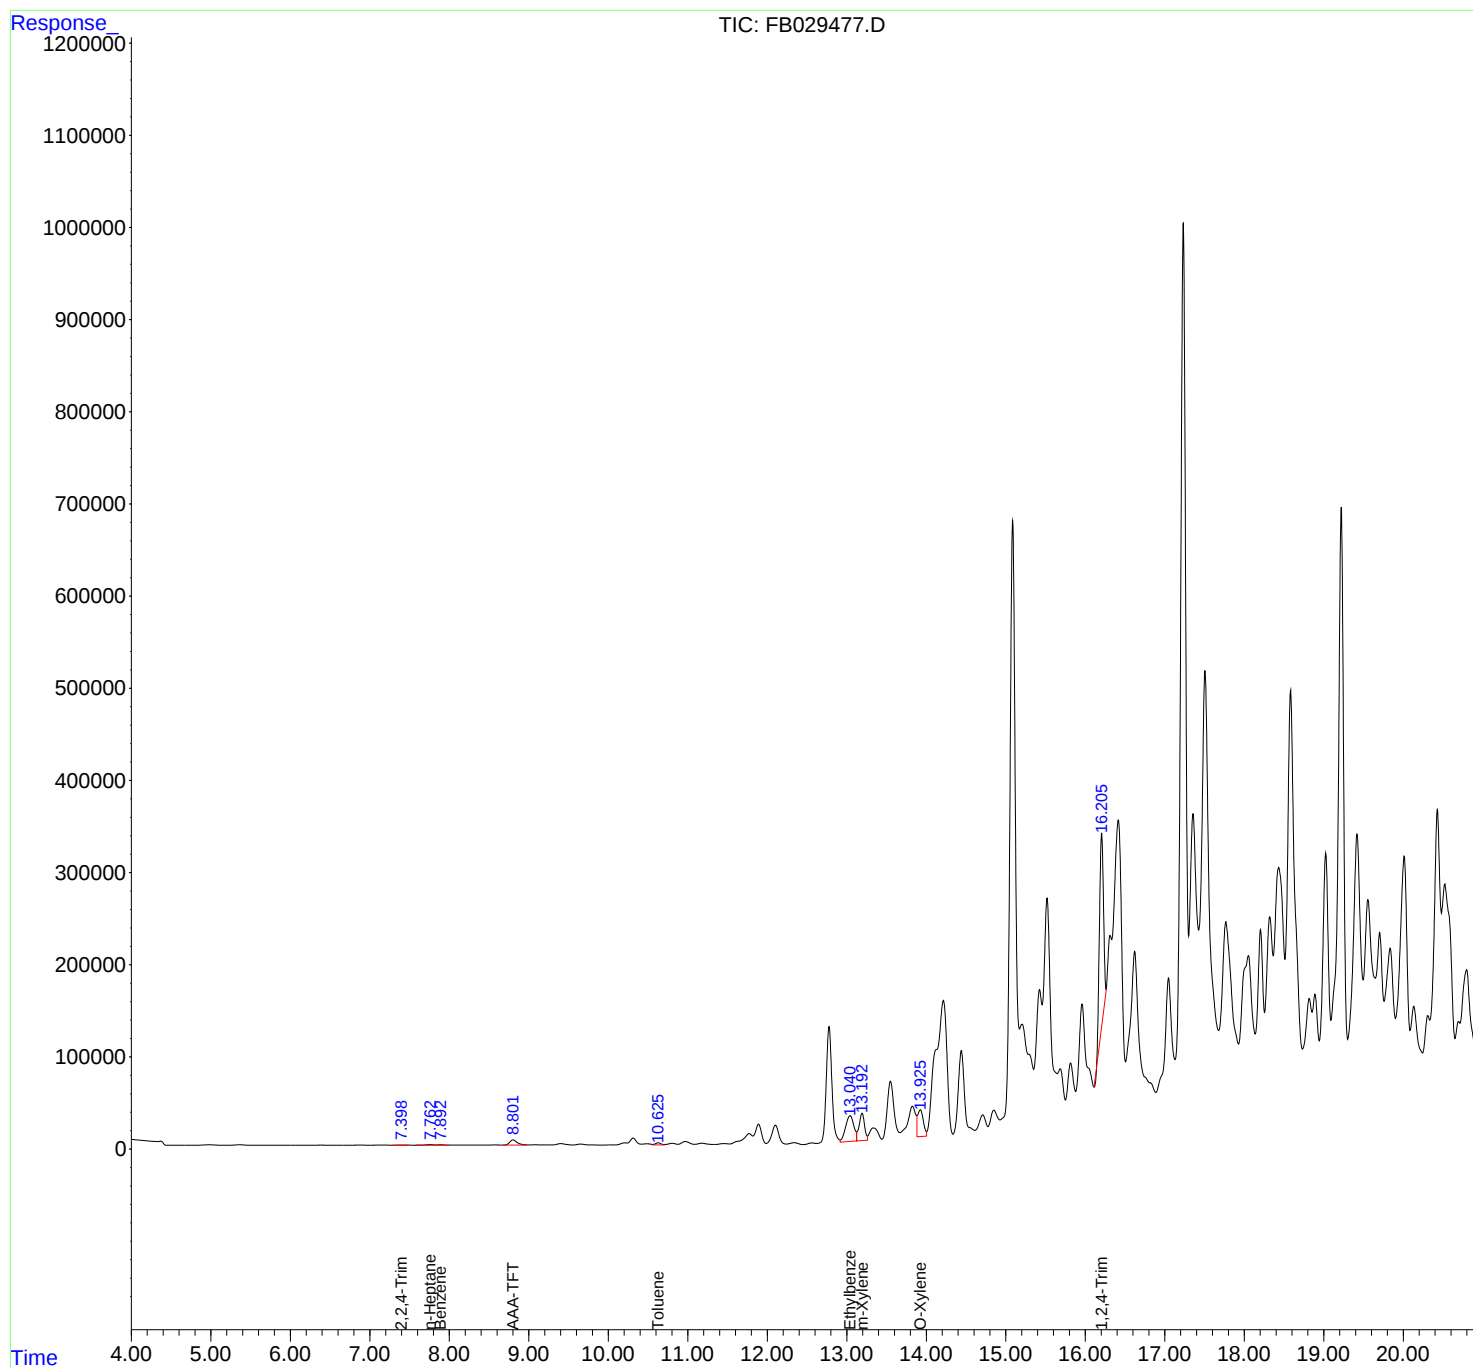


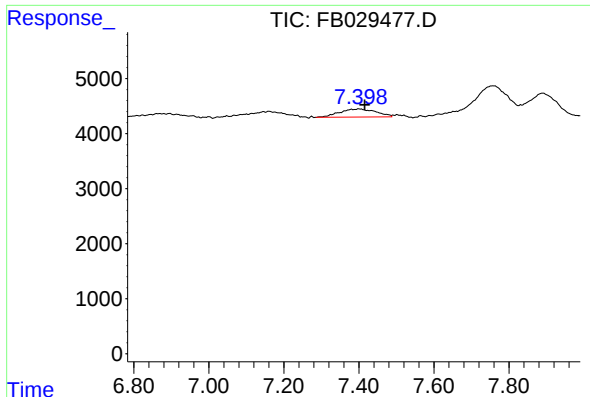

#2 2,2,4-Trimethylpentane


R.T.: 7.399 min
Delta R.T.: -0.016 min
Response: 9982
Conc: 0.59 ng/ml

Instrument :
FID_B
ClientSampleId :

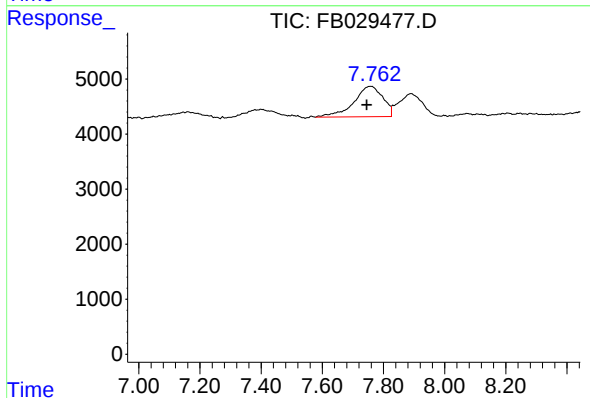


#3 n-Heptane

R.T.: 7.762 min
Delta R.T.: 0.016 min
Response: 36565
Conc: 2.11 ng/ml

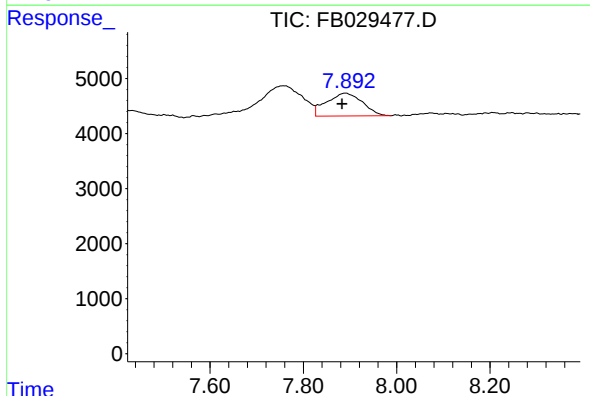


#4 Benzene

R.T.: 7.893 min
Delta R.T.: 0.009 min
Response: 22038
Conc: 1.09 ng/ml

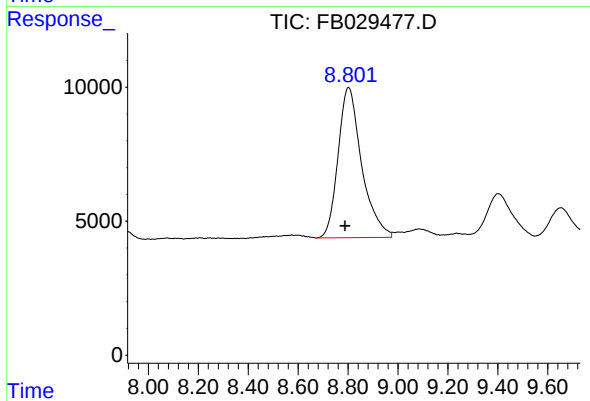

#5 AAA-TFT


R.T.: 8.802 min
Delta R.T.: 0.014 min
Response: 367881
Conc: 30.36 ng/ml

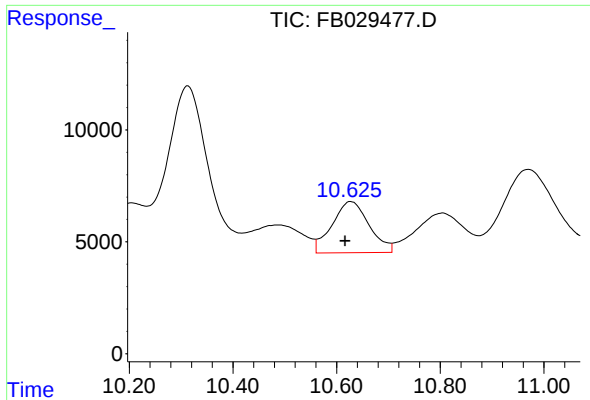

#6 Toluene


R.T.: 10.627 min
Delta R.T.: 0.011 min
Response: 113317
Conc: 5.74 ng/ml

Instrument :
FID_B
ClientSampleId :

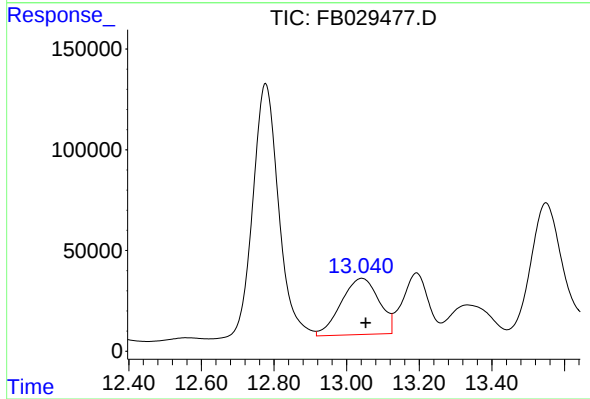


#7 Ethylbenzene

R.T.: 13.042 min
Delta R.T.: -0.011 min
Response: 2025761
Conc: 108.81 ng/ml

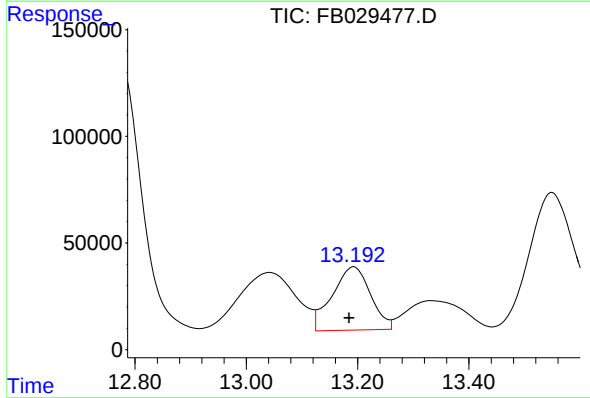


#8 m-Xylene

R.T.: 13.193 min
Delta R.T.: 0.008 min
Response: 1421635
Conc: 76.42 ng/ml

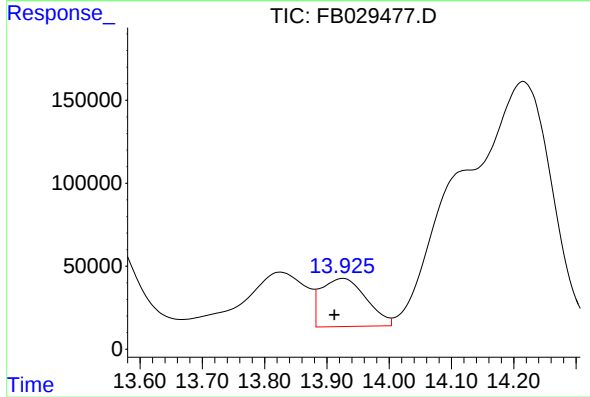

#9 O-Xylene

R.T.: 13.925 min
Delta R.T.: 0.013 min
Response: 1460362
Conc: 79.31 ng/ml

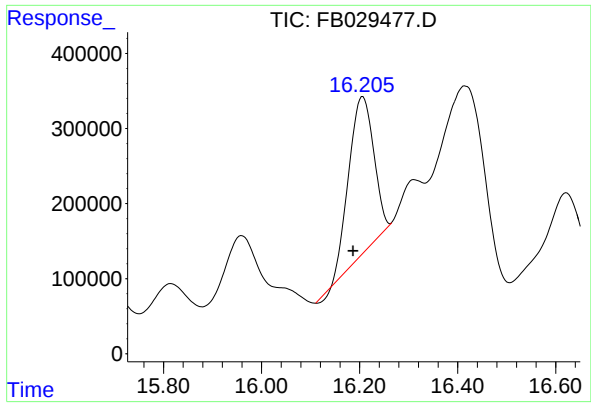

#10 1,2,4-Trimethylbenzene

R.T.: 16.207 min
Delta R.T.: 0.020 min
Response: 7304834
Conc: 392.19 ng/ml

Instrument :
FID_B
ClientSampleId :