

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB031423\
 Data File : FB029474.D
 Signal(s) : FID2B.CH
 Acq On : 14 Mar 2023 10:46
 Operator : YP/AJ
 Sample : BSF0314S2
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0314S2

Integration File: Calibration.e
 Quant Time: Mar 14 16:26:30 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030123.M
 Quant Title :
 QLast Update : Wed Mar 01 12:30:24 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.798	242967	20.054 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.717	456248	29.734 ng/ml
2) t 2,2,4-Trimethylpentane	7.427	531384	31.546 ng/ml
3) t n-Heptane	7.757	176680	10.215 ng/ml
4) t Benzene	7.894	207253	10.210 ng/ml
6) t Toluene	10.627	617618	31.289 ng/ml
7) t Ethylbenzene	13.064	193010	10.367 ng/ml
8) t m-Xylene	13.196	381608	20.513 ng/ml
9) t O-Xylene	13.923	364818	19.813 ng/ml
10) t 1,2,4-Trimethylbenzene	16.199	347114	18.636 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB031423\
Data File : FB029474.D
Signal(s) : FID2B.CH
Acq On : 14 Mar 2023 10:46
Operator : YP/AJ
Sample : BSF0314S2
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0314S2

Integration File: Calibration.e
Quant Time: Mar 14 16:26:30 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030123.M
Quant Title :
QLast Update : Wed Mar 01 12:30:24 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

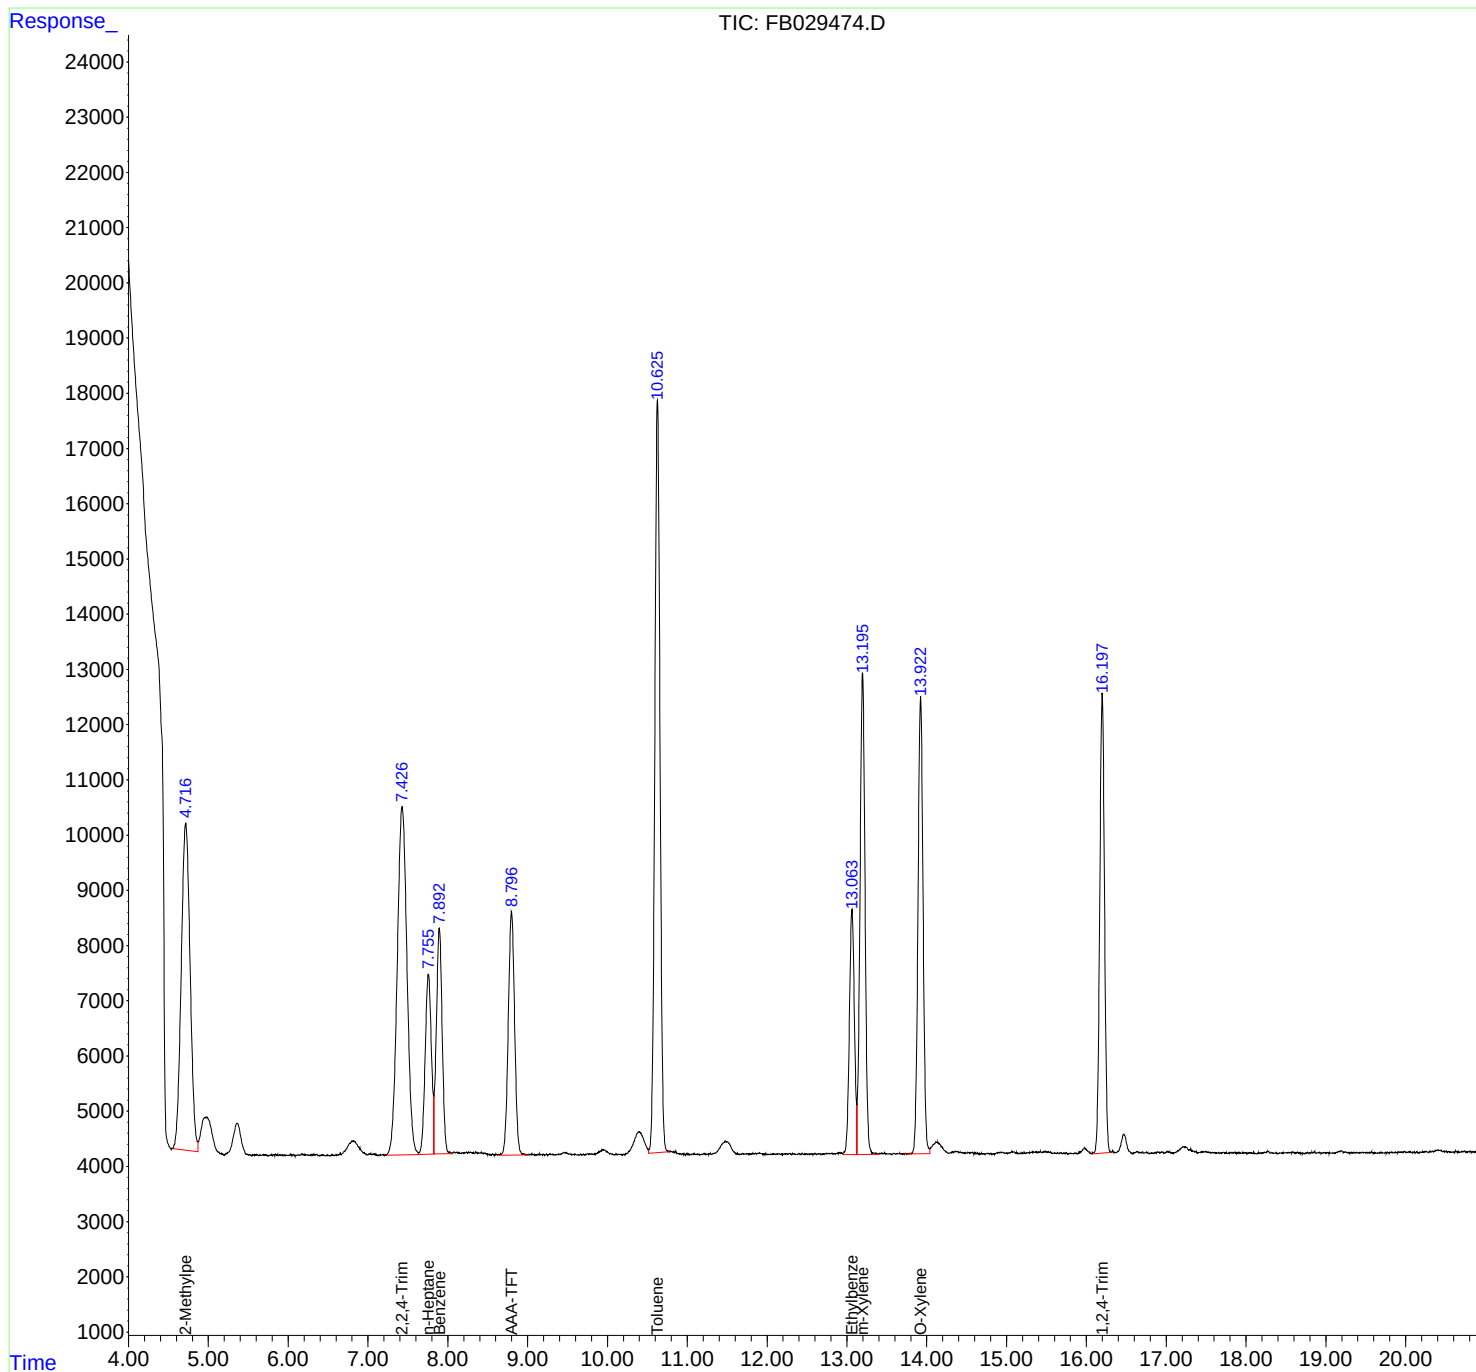


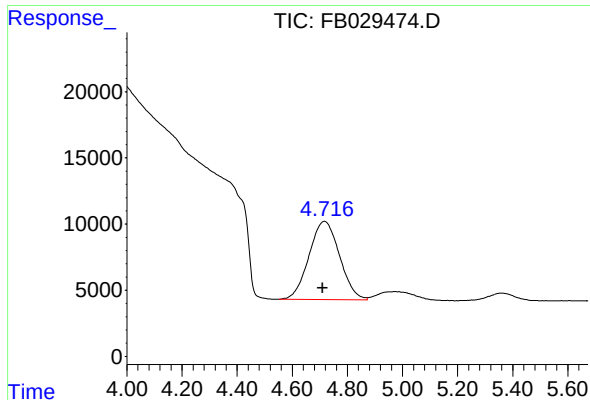

#1 2-Methylpentane


R.T.: 4.717 min
Delta R.T.: 0.007 min
Response: 456248
Conc: 29.73 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0314S2

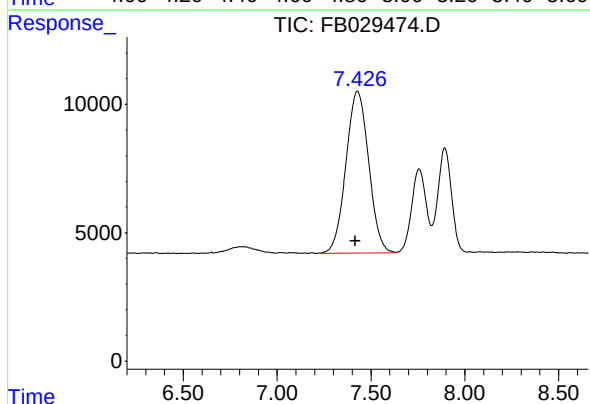


#2 2,2,4-Trimethylpentane

R.T.: 7.427 min
Delta R.T.: 0.012 min
Response: 531384
Conc: 31.55 ng/ml

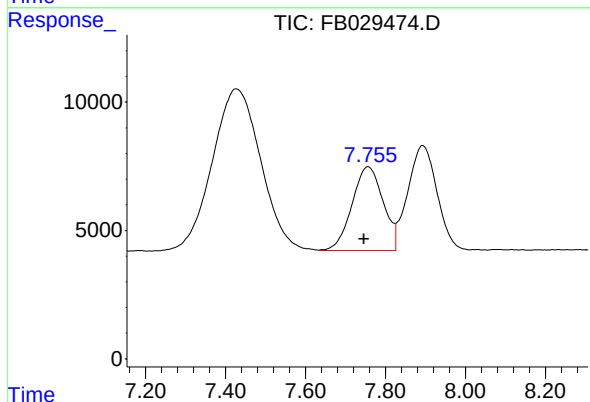


#3 n-Heptane

R.T.: 7.757 min
Delta R.T.: 0.011 min
Response: 176680
Conc: 10.22 ng/ml

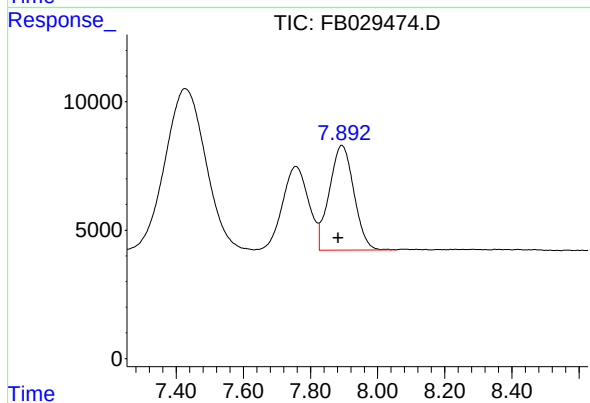

#4 Benzene


R.T.: 7.894 min
Delta R.T.: 0.010 min
Response: 207253
Conc: 10.21 ng/ml

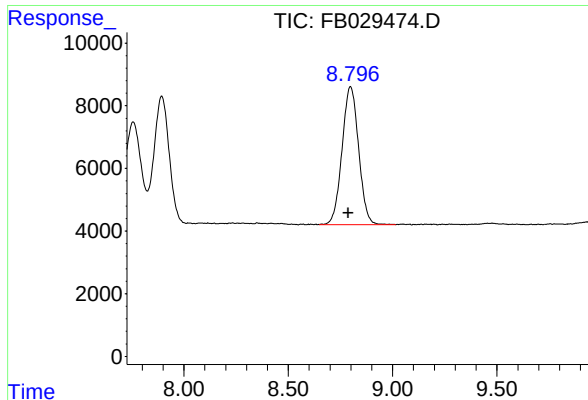

#5 AAA-TFT


R.T.: 8.798 min
Delta R.T.: 0.010 min
Response: 242967
Conc: 20.05 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0314S2

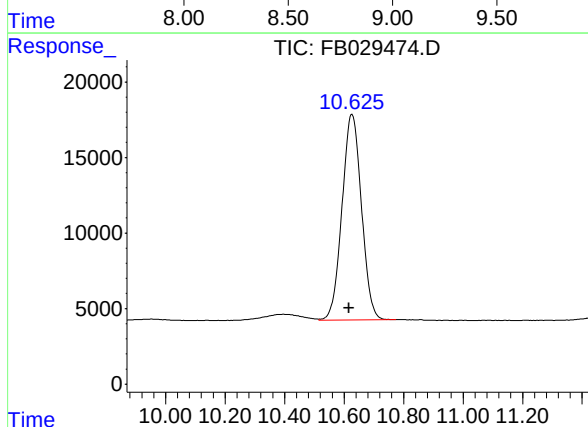


#6 Toluene

R.T.: 10.627 min
Delta R.T.: 0.011 min
Response: 617618
Conc: 31.29 ng/ml

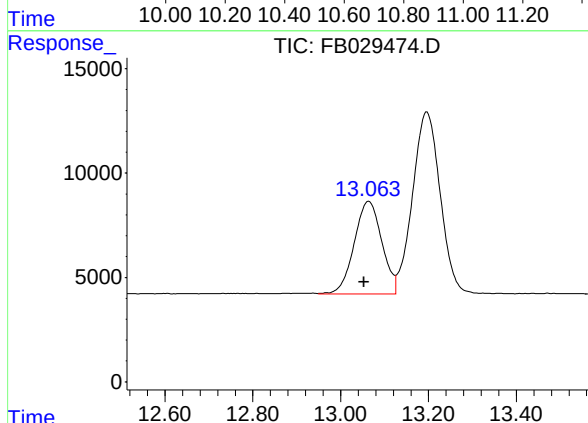


#7 Ethylbenzene

R.T.: 13.064 min
Delta R.T.: 0.011 min
Response: 193010
Conc: 10.37 ng/ml

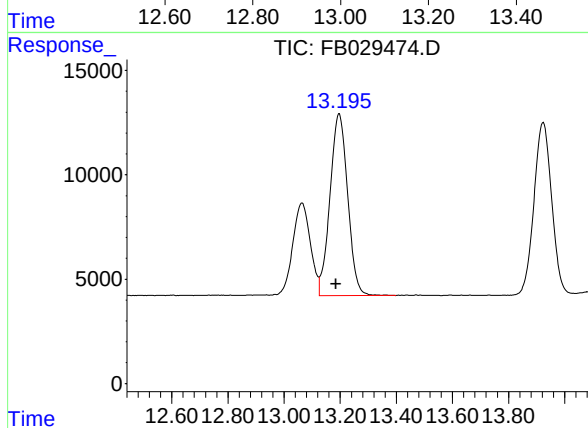

#8 m-Xylene


R.T.: 13.196 min
Delta R.T.: 0.012 min
Response: 381608
Conc: 20.51 ng/ml

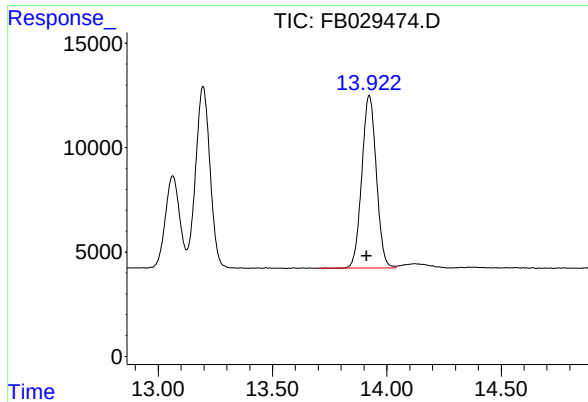

#9 O-Xylene

R.T.: 13.923 min
Delta R.T.: 0.011 min
Response: 364818
Conc: 19.81 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0314S2

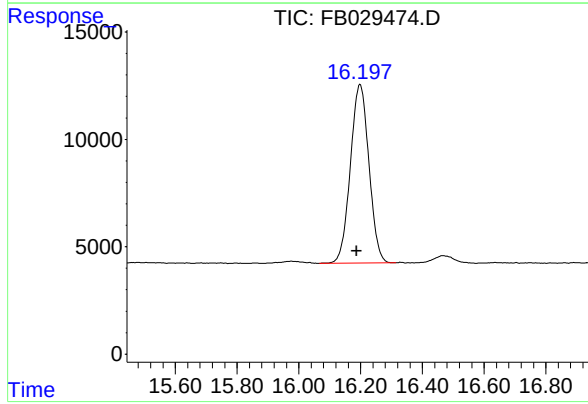

#10 1,2,4-Trimethylbenzene

R.T.: 16.199 min
Delta R.T.: 0.012 min
Response: 347114
Conc: 18.64 ng/ml