

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB031424\
 Data File : FB030644.D
 Signal(s) : FID2B.CH
 Acq On : 15 Mar 2024 5:13
 Operator : YP/AJ
 Sample : BSF0314S3
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Mar 15 05:13:43 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB031124.M
 Quant Title :
 QLast Update : Mon Mar 11 11:00:59 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.787	247894	18.307 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.704	619512	31.469 ng/ml
2) t 2,2,4-Trimethylpentane	7.411	574711	29.393 ng/ml
3) t n-Heptane	7.747	217612	9.869 ng/ml
4) t Benzene	7.883	253525	10.319 ng/ml
6) t Toluene	10.615	726903	30.739 ng/ml
7) t Ethylbenzene	13.052	223474	10.325 ng/ml
8) t m-Xylene	13.184	442334	20.439 ng/ml
9) t O-Xylene	13.911	418785	19.696 ng/ml
10) t 1,2,4-Trimethylbenzene	16.186	403970	19.031 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB031424\
Data File : FB030644.D
Signal(s) : FID2B.CH
Acq On : 15 Mar 2024 5:13
Operator : YP/AJ
Sample : BSF0314S3
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Mar 15 05:13:43 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB031124.M
Quant Title :
QLast Update : Mon Mar 11 11:00:59 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

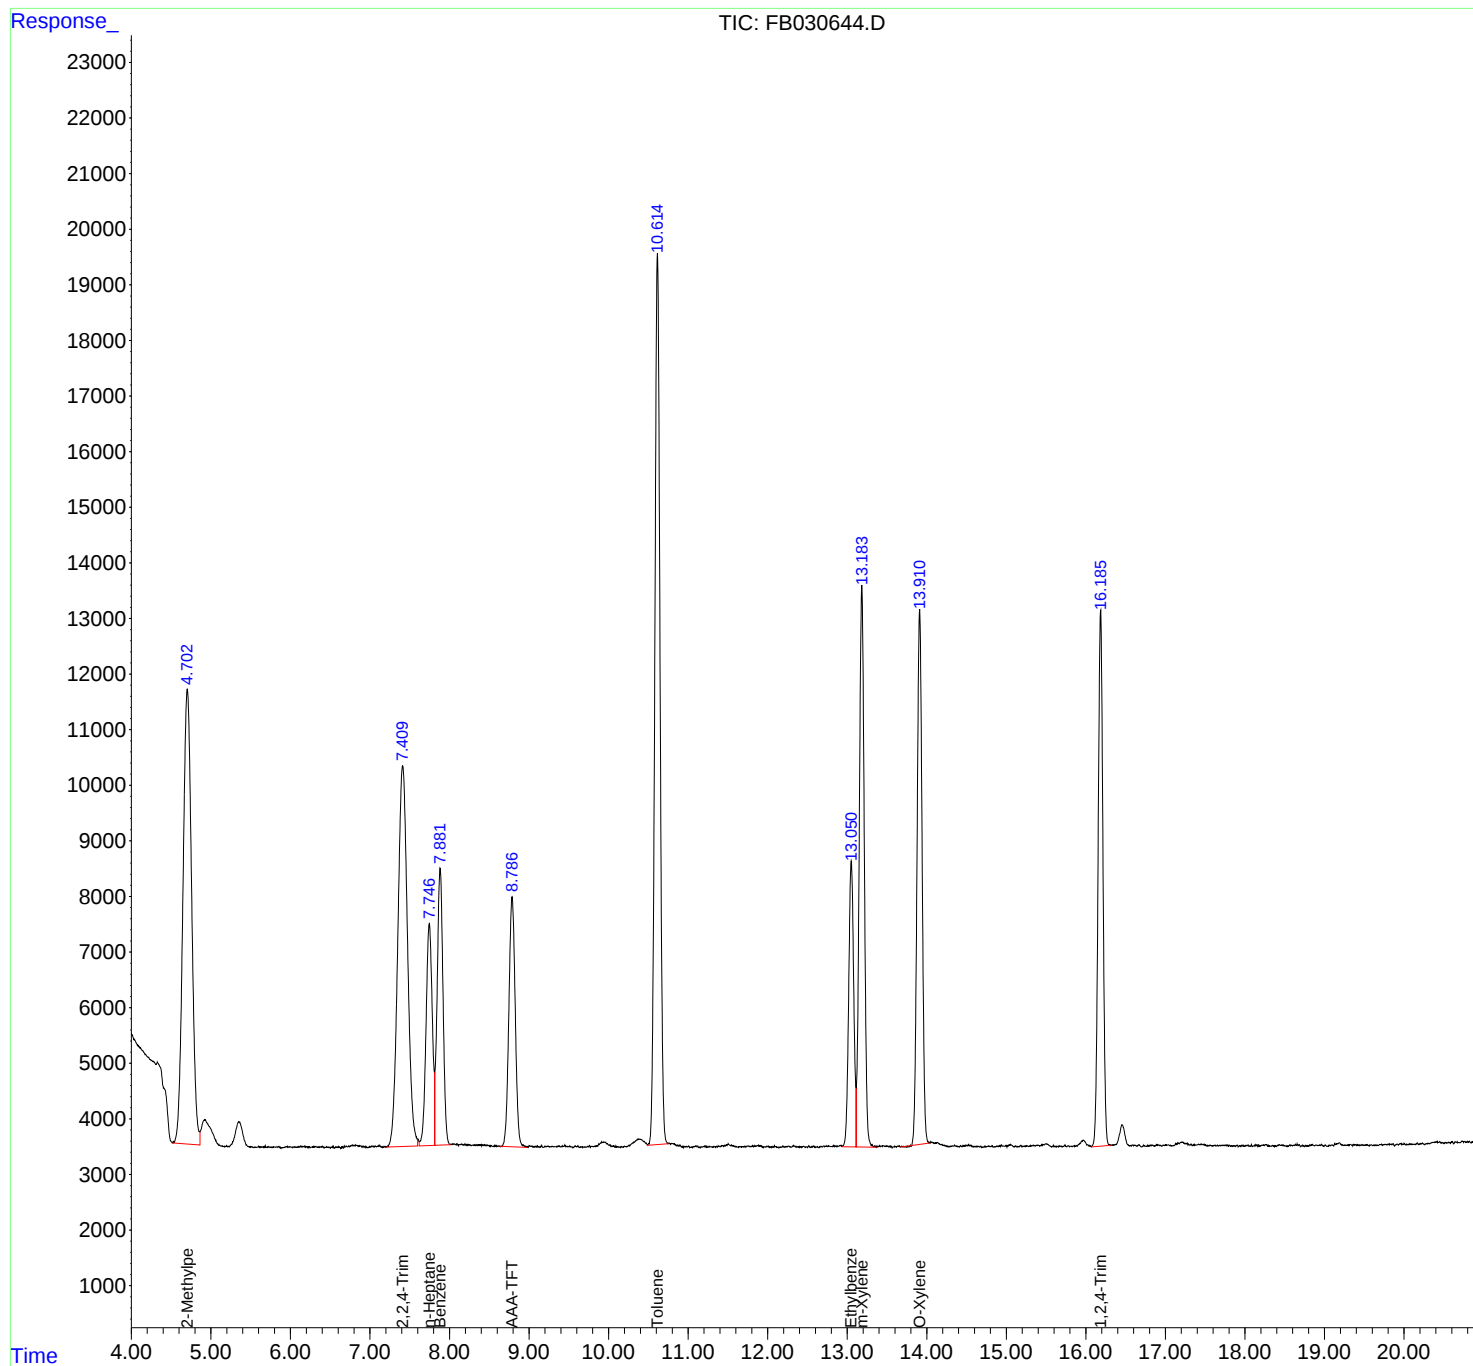


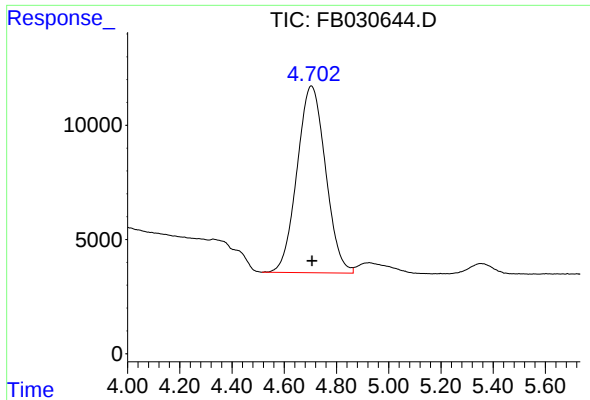

#1 2-Methylpentane


R.T.: 4.704 min
Delta R.T.: -0.003 min
Response: 619512
Conc: 31.47 ng/ml

Instrument :
FID_B
ClientSampleId :

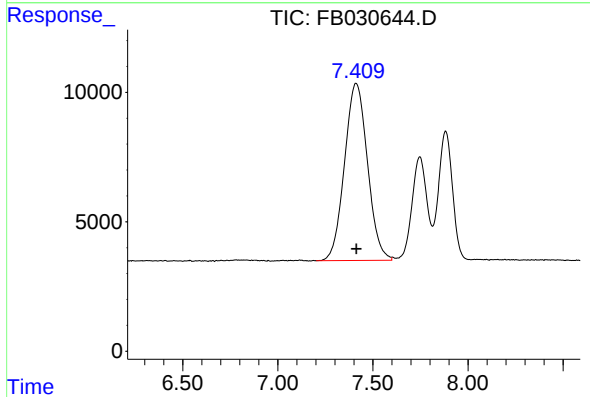


#2 2,2,4-Trimethylpentane

R.T.: 7.411 min
Delta R.T.: -0.002 min
Response: 574711
Conc: 29.39 ng/ml

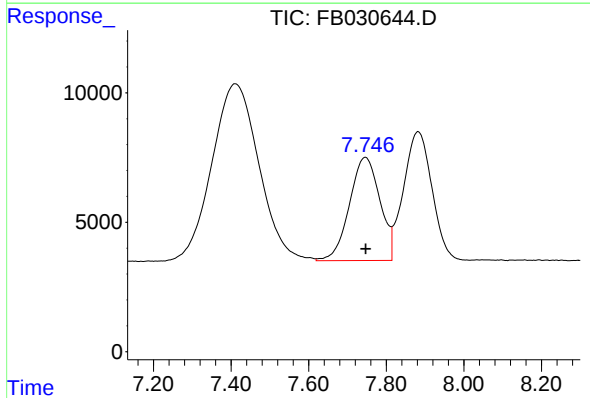


#3 n-Heptane

R.T.: 7.747 min
Delta R.T.: 0.000 min
Response: 217612
Conc: 9.87 ng/ml

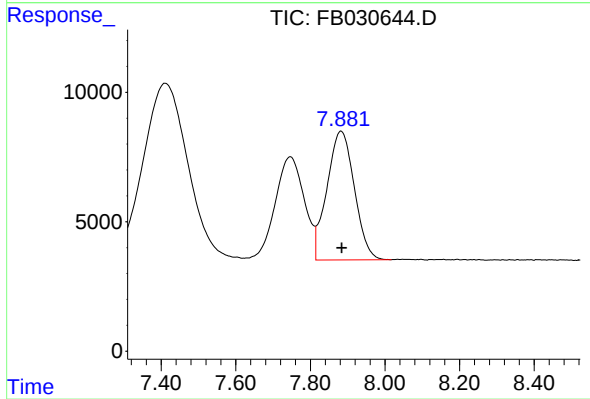

#4 Benzene


R.T.: 7.883 min
Delta R.T.: -0.001 min
Response: 253525
Conc: 10.32 ng/ml

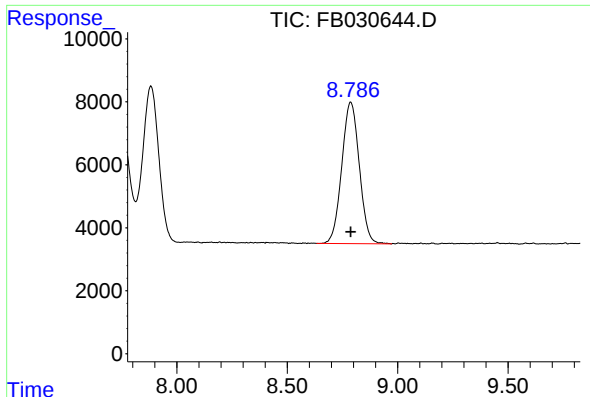

#5 AAA-TFT


R.T.: 8.787 min
Delta R.T.: 0.000 min
Response: 247894
Conc: 18.31 ng/ml

Instrument :
FID_B
ClientSampleId :

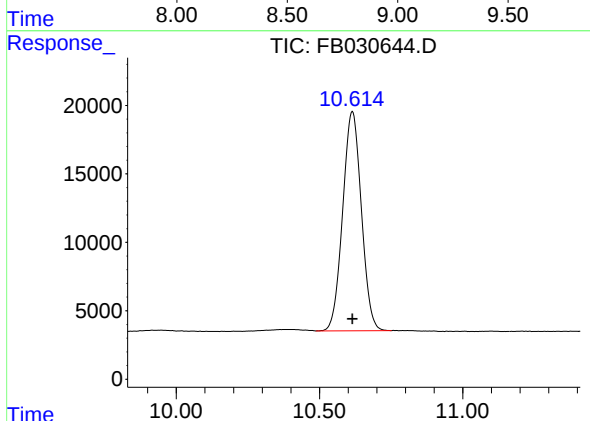


#6 Toluene

R.T.: 10.615 min
Delta R.T.: 0.000 min
Response: 726903
Conc: 30.74 ng/ml

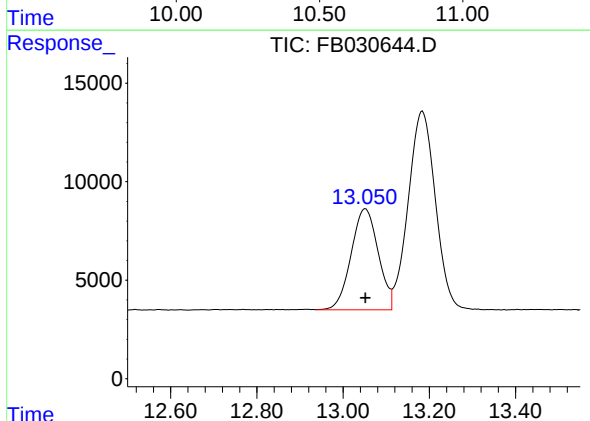


#7 Ethylbenzene

R.T.: 13.052 min
Delta R.T.: 0.000 min
Response: 223474
Conc: 10.33 ng/ml

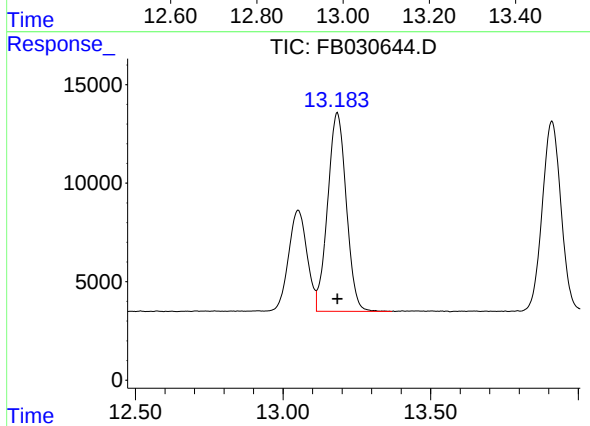

#8 m-Xylene


R.T.: 13.184 min
Delta R.T.: 0.000 min
Response: 442334
Conc: 20.44 ng/ml

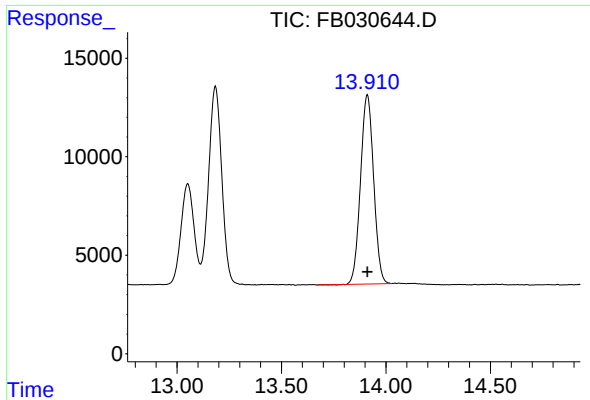

#9 O-Xylene

R.T.: 13.911 min
Delta R.T.: 0.000 min
Response: 418785
Conc: 19.70 ng/ml

Instrument :
FID_B
ClientSampleId :

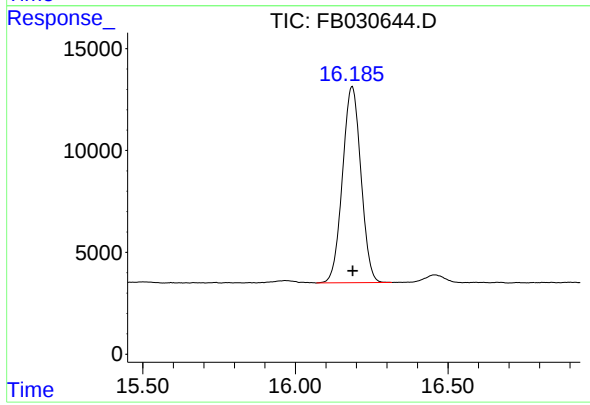

#10 1,2,4-Trimethylbenzene

R.T.: 16.186 min
Delta R.T.: -0.002 min
Response: 403970
Conc: 19.03 ng/ml