

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB031424\
 Data File : FB030626.D
 Signal(s) : FID2B.CH
 Acq On : 14 Mar 2024 15:42
 Operator : YP/AJ
 Sample : BSF0314S2
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0314S2

Integration File: Calibration.e
 Quant Time: Mar 15 03:00:39 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB031124.M
 Quant Title :
 QLast Update : Mon Mar 11 11:00:59 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.788	310545	22.934 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.707	562601	28.578 ng/ml
2) t 2,2,4-Trimethylpentane	7.415	551840	28.223 ng/ml
3) t n-Heptane	7.747	203193	9.215 ng/ml
4) t Benzene	7.884	232151	9.449 ng/ml
6) t Toluene	10.616	671554	28.398 ng/ml
7) t Ethylbenzene	13.053	208413	9.629 ng/ml
8) t m-Xylene	13.186	415433	19.196 ng/ml
9) t O-Xylene	13.913	401605	18.888 ng/ml
10) t 1,2,4-Trimethylbenzene	16.188	392074	18.470 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB031424\
Data File : FB030626.D
Signal(s) : FID2B.CH
Acq On : 14 Mar 2024 15:42
Operator : YP/AJ
Sample : BSF0314S2
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0314S2

Integration File: Calibration.e
Quant Time: Mar 15 03:00:39 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB031124.M
Quant Title :
QLast Update : Mon Mar 11 11:00:59 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

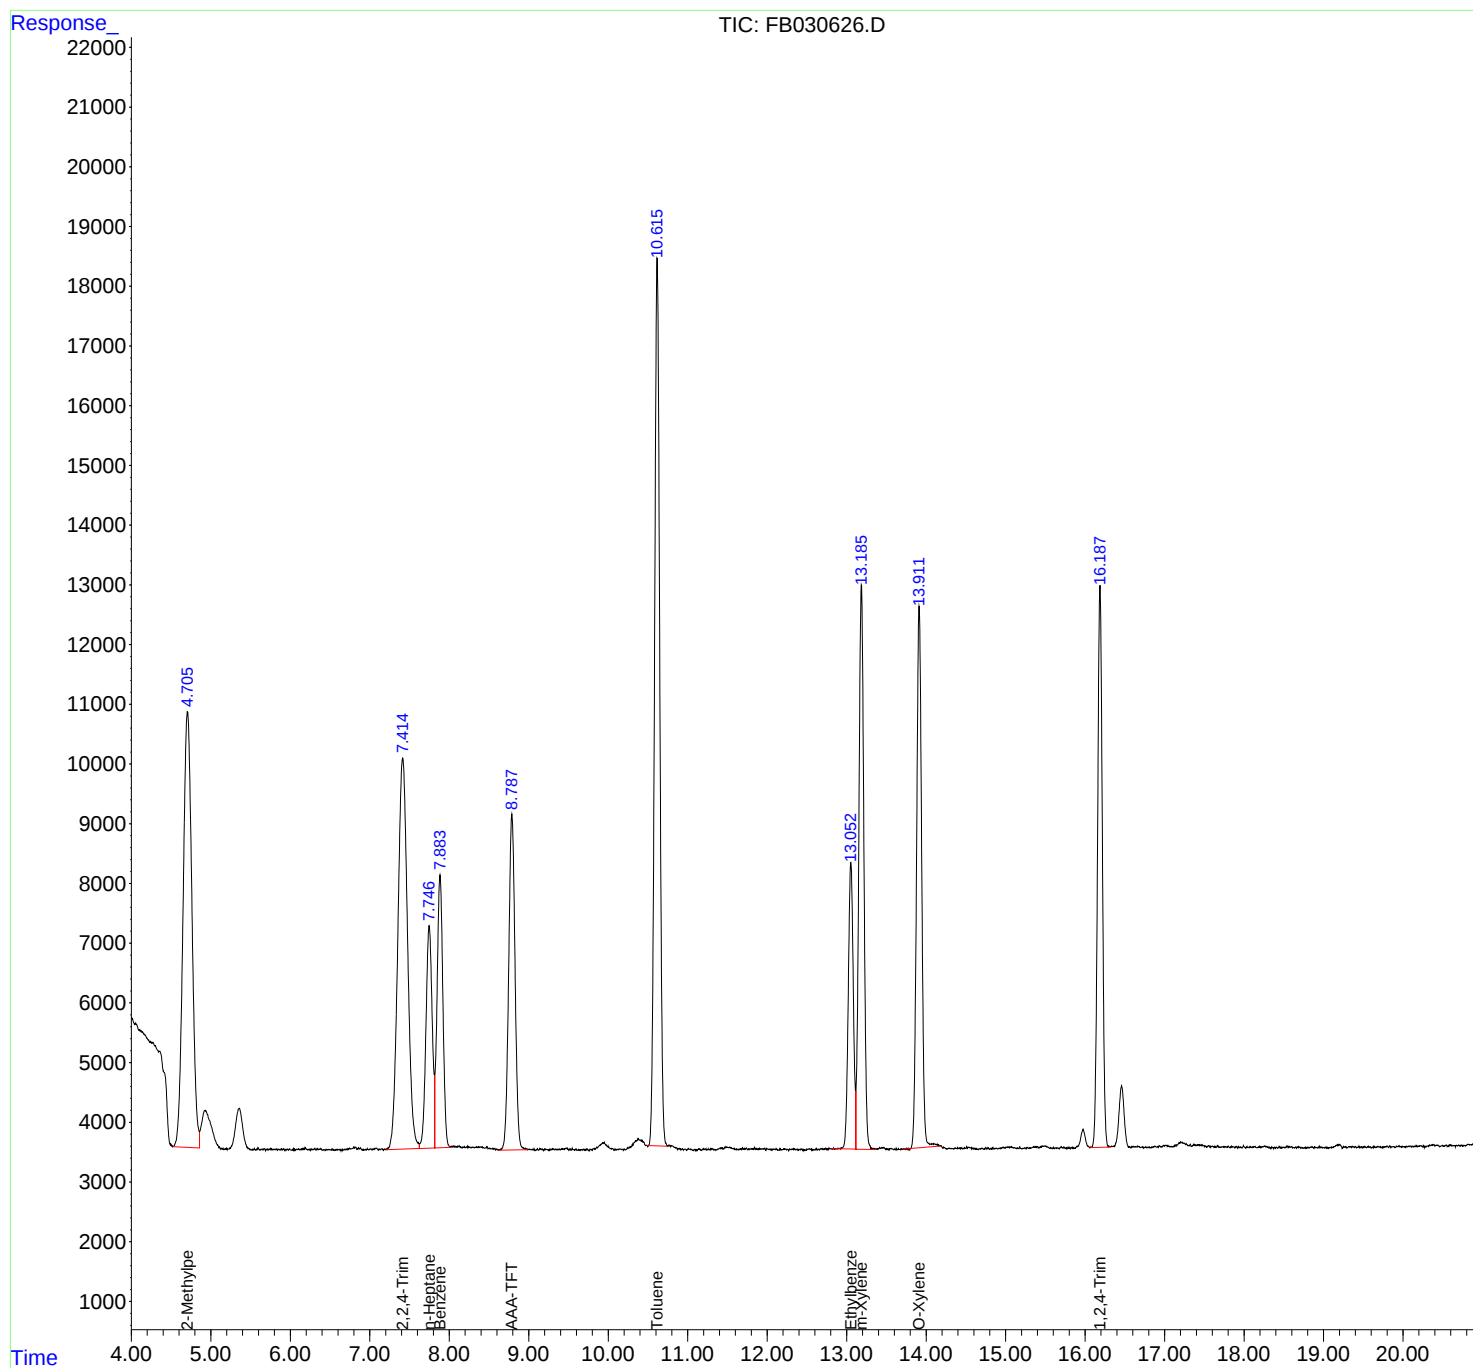


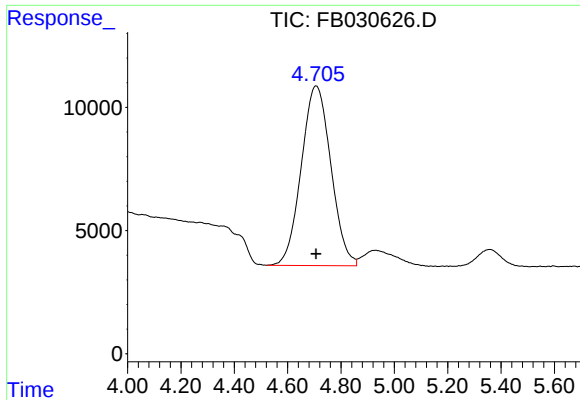

#1 2-Methylpentane


R.T.: 4.707 min
Delta R.T.: 0.000 min
Response: 562601
Conc: 28.58 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0314S2

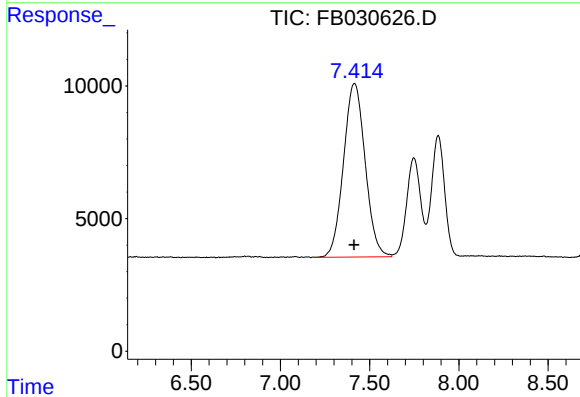


#2 2,2,4-Trimethylpentane

R.T.: 7.415 min
Delta R.T.: 0.003 min
Response: 551840
Conc: 28.22 ng/ml

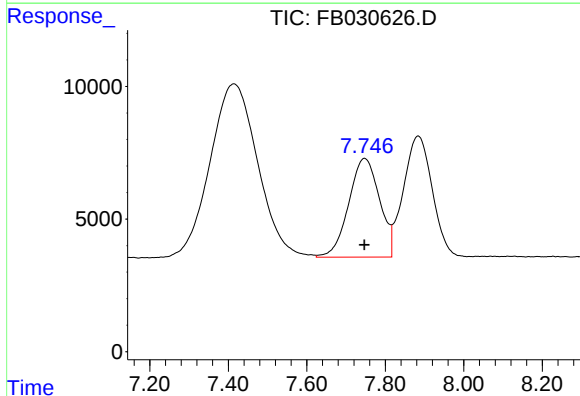


#3 n-Heptane

R.T.: 7.747 min
Delta R.T.: 0.000 min
Response: 203193
Conc: 9.22 ng/ml

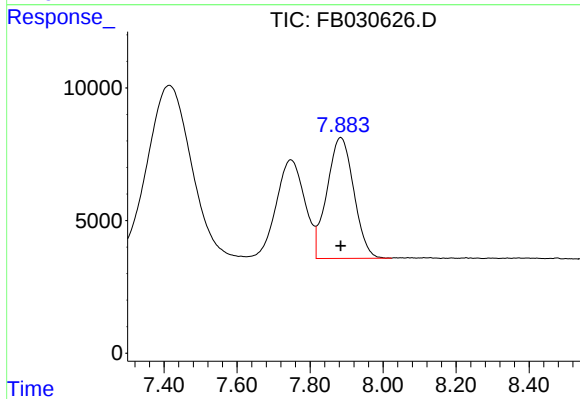

#4 Benzene


R.T.: 7.884 min
Delta R.T.: 0.000 min
Response: 232151
Conc: 9.45 ng/ml

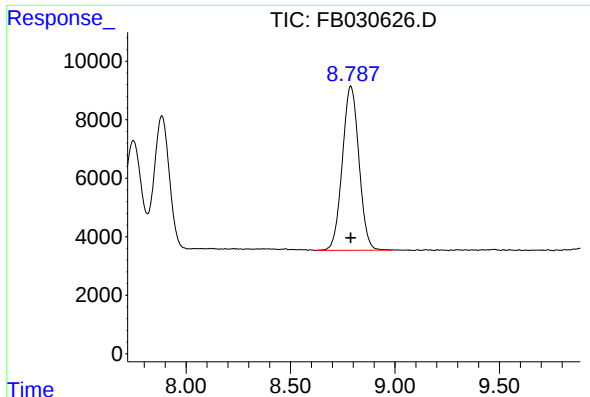

#5 AAA-TFT


R.T.: 8.788 min
Delta R.T.: 0.000 min
Response: 310545
Conc: 22.93 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0314S2

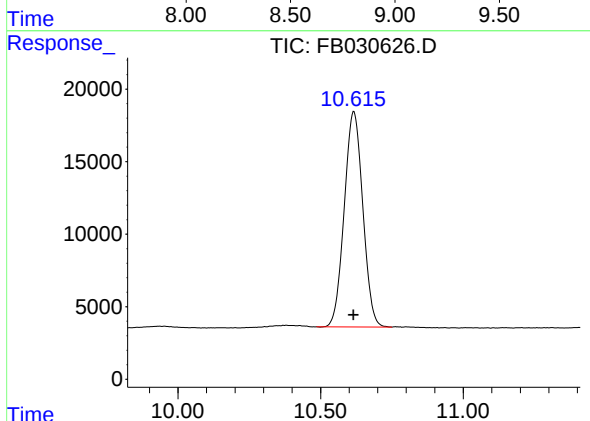


#6 Toluene

R.T.: 10.616 min
Delta R.T.: 0.001 min
Response: 671554
Conc: 28.40 ng/ml

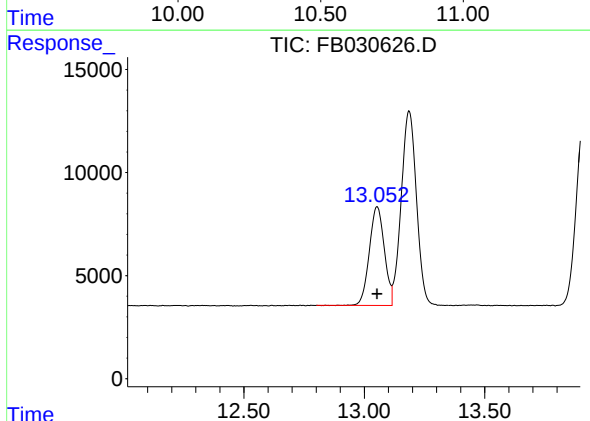


#7 Ethylbenzene

R.T.: 13.053 min
Delta R.T.: 0.001 min
Response: 208413
Conc: 9.63 ng/ml

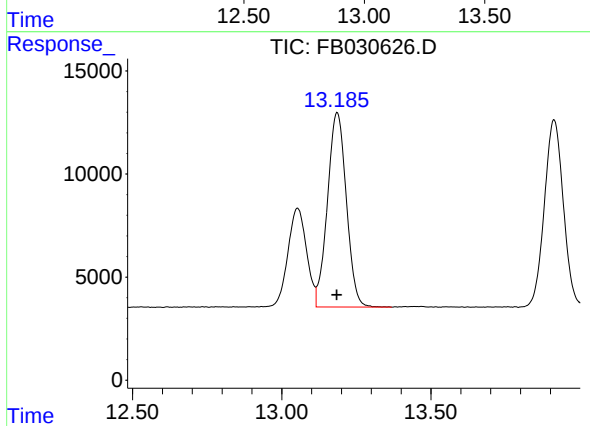

#8 m-Xylene


R.T.: 13.186 min
Delta R.T.: 0.002 min
Response: 415433
Conc: 19.20 ng/ml

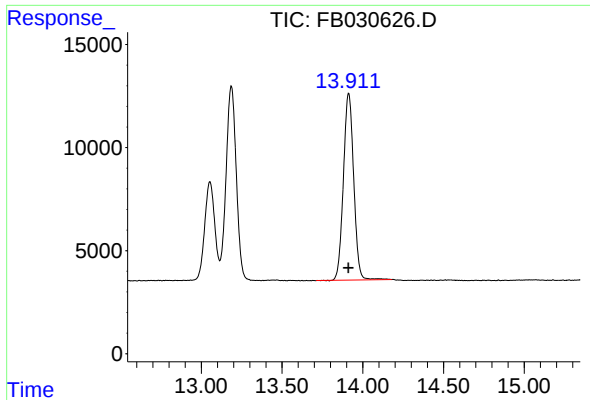

#9 O-Xylene

R.T.: 13.913 min
Delta R.T.: 0.001 min
Response: 401605
Conc: 18.89 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0314S2

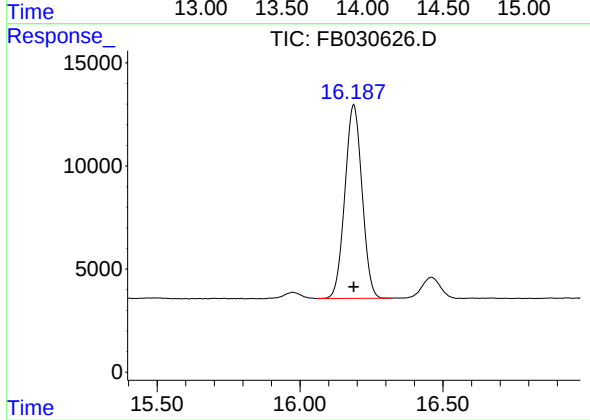

#10 1,2,4-Trimethylbenzene

R.T.: 16.188 min
Delta R.T.: 0.000 min
Response: 392074
Conc: 18.47 ng/ml