

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB031424\
 Data File : FB030636.D
 Signal(s) : FID2B.CH
 Acq On : 14 Mar 2024 22:48
 Operator : YP/AJ
 Sample : P1746-20MS 50X
 Misc : 5.02G/5.00 ML MEOH
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 SB-06-COMPMS

Integration File: Calibration.e
 Quant Time: Mar 15 03:01:54 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB031124.M
 Quant Title :
 QLast Update : Mon Mar 11 11:00:59 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.783	244119	18.028 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.701	489578	24.869 ng/ml
2) t 2,2,4-Trimethylpentane	7.408	497059	25.421 ng/ml
3) t n-Heptane	7.743	178446	8.093 ng/ml
4) t Benzene	7.878	229476	9.340 ng/ml
6) t Toluene	10.611	639165	27.029 ng/ml
7) t Ethylbenzene	13.048	197116	9.107 ng/ml
8) t m-Xylene	13.181	389909	18.017 ng/ml
9) t O-Xylene	13.908	378577	17.805 ng/ml
10) t 1,2,4-Trimethylbenzene	16.183	347901	16.389 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB031424\
Data File : FB030636.D
Signal(s) : FID2B.CH
Acq On : 14 Mar 2024 22:48
Operator : YP/AJ
Sample : P1746-20MS 50X
Misc : 5.02G/5.00 ML MEOH
ALS Vial : 21 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
SB-06-COMPMS

Integration File: Calibration.e
Quant Time: Mar 15 03:01:54 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB031124.M
Quant Title :
QLast Update : Mon Mar 11 11:00:59 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

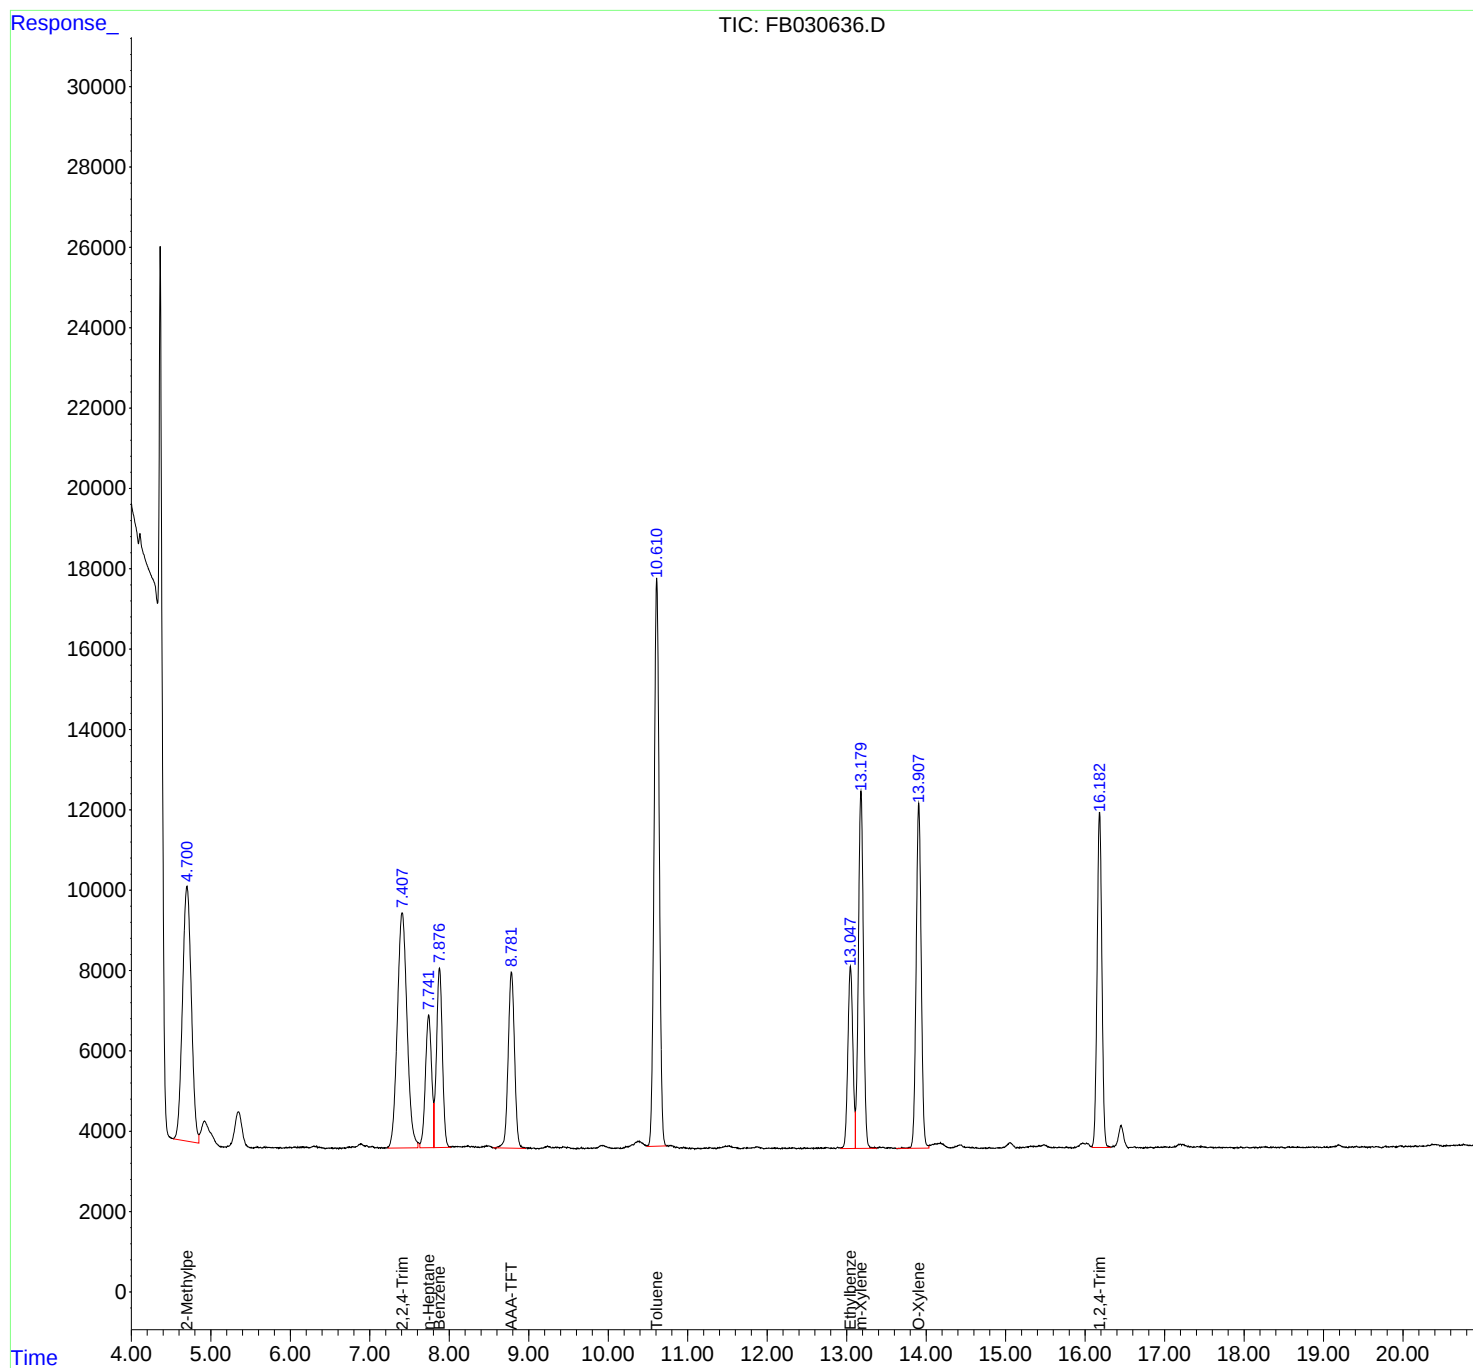


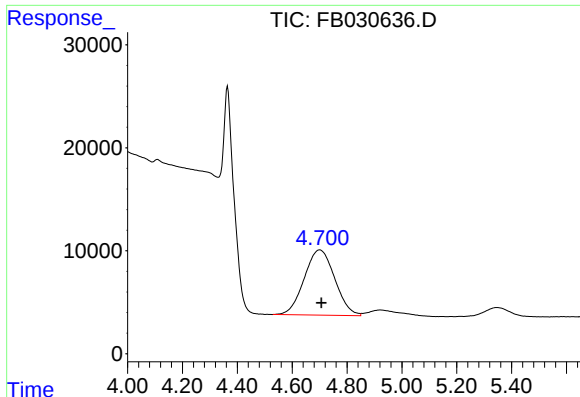

#1 2-Methylpentane


R.T.: 4.701 min
Delta R.T.: -0.006 min
Response: 489578
Conc: 24.87 ng/ml

Instrument :
FID_B
ClientSampleId :
SB-06-COMPMS

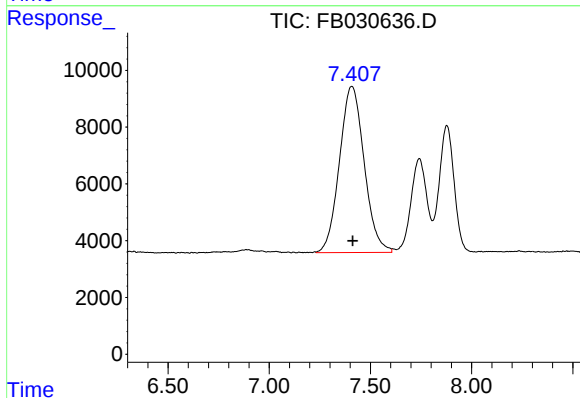


#2 2,2,4-Trimethylpentane

R.T.: 7.408 min
Delta R.T.: -0.004 min
Response: 497059
Conc: 25.42 ng/ml

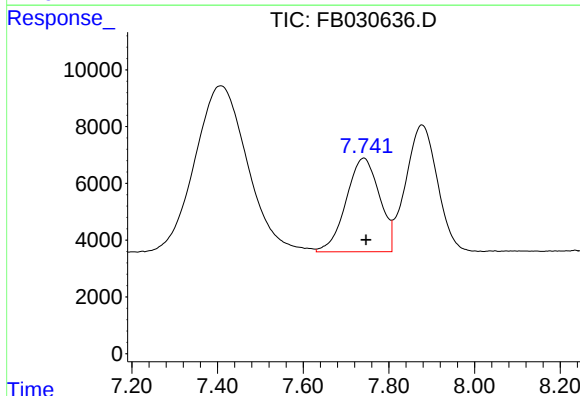


#3 n-Heptane

R.T.: 7.743 min
Delta R.T.: -0.005 min
Response: 178446
Conc: 8.09 ng/ml

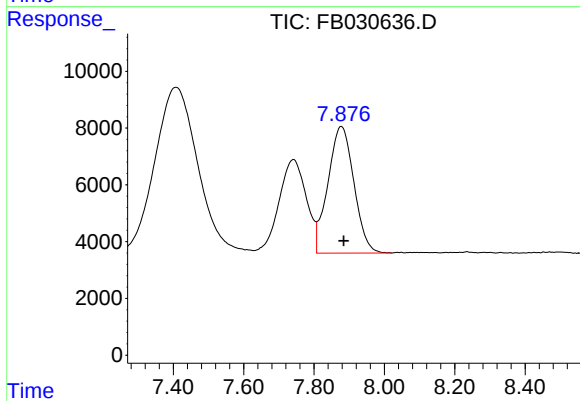

#4 Benzene


R.T.: 7.878 min
Delta R.T.: -0.006 min
Response: 229476
Conc: 9.34 ng/ml

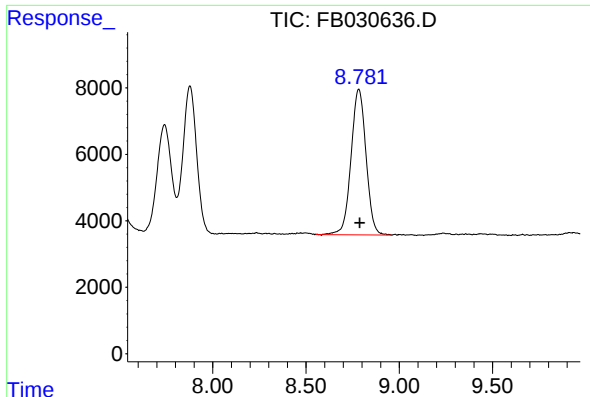

#5 AAA-TFT


R.T.: 8.783 min
Delta R.T.: -0.005 min
Response: 244119
Conc: 18.03 ng/ml

Instrument :
FID_B
ClientSampleId :
SB-06-COMPMS

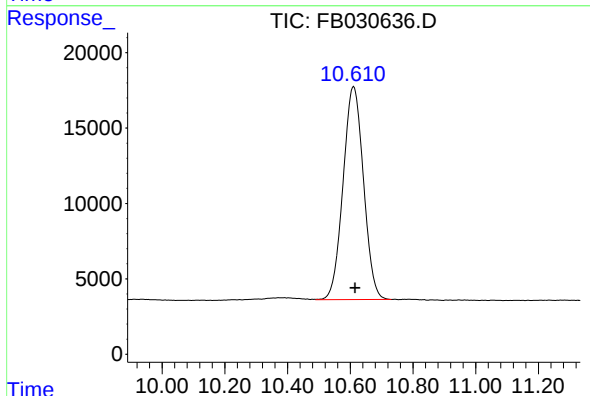


#6 Toluene

R.T.: 10.611 min
Delta R.T.: -0.004 min
Response: 639165
Conc: 27.03 ng/ml

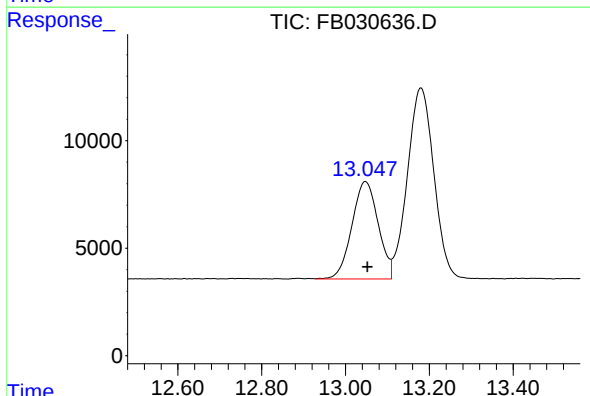


#7 Ethylbenzene

R.T.: 13.048 min
Delta R.T.: -0.004 min
Response: 197116
Conc: 9.11 ng/ml

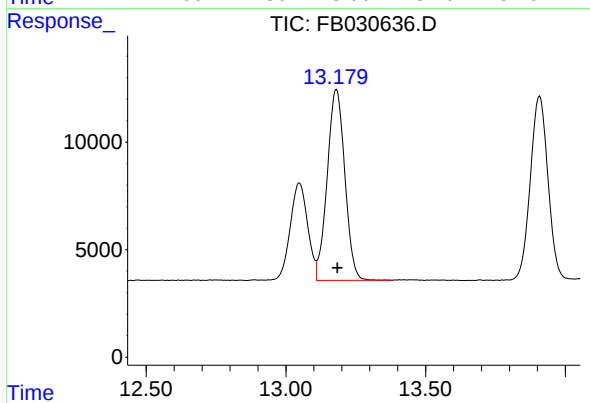

#8 m-Xylene


R.T.: 13.181 min
Delta R.T.: -0.004 min
Response: 389909
Conc: 18.02 ng/ml

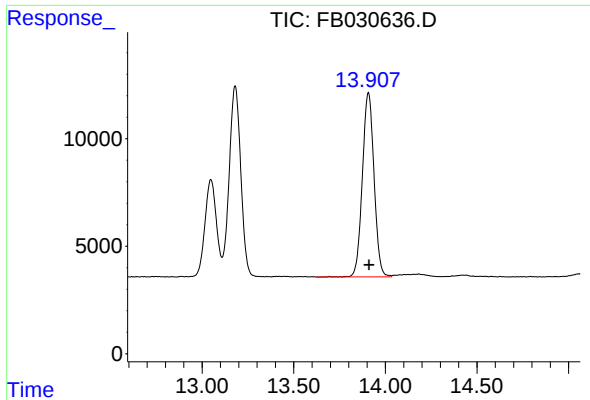

#9 O-Xylene

R.T.: 13.908 min
Delta R.T.: -0.004 min
Response: 378577
Conc: 17.80 ng/ml

Instrument :
FID_B
ClientSampleId :
SB-06-COMPMS

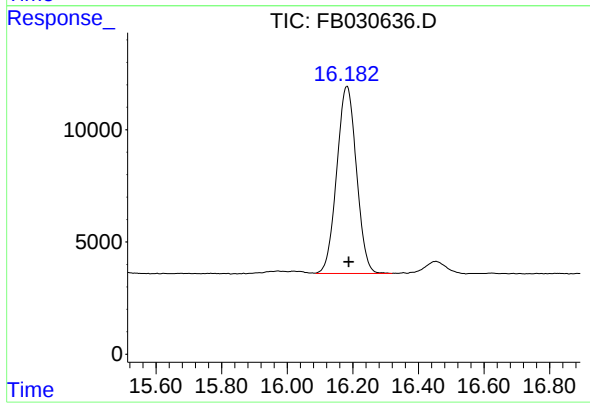

#10 1,2,4-Trimethylbenzene

R.T.: 16.183 min
Delta R.T.: -0.005 min
Response: 347901
Conc: 16.39 ng/ml