

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB031424\
 Data File : FB030637.D
 Signal(s) : FID2B.CH
 Acq On : 14 Mar 2024 23:26
 Operator : YP/AJ
 Sample : P1746-20MSD 50X
 Misc : 5.06G/5.00 ML MEOH
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 SB-06-COMPMSD

Integration File: Calibration.e
 Quant Time: Mar 15 03:02:02 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB031124.M
 Quant Title :
 QLast Update : Mon Mar 11 11:00:59 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.784	215385	15.906 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.700	457795	23.255 ng/ml
2) t 2,2,4-Trimethylpentane	7.408	513016	26.237 ng/ml
3) t n-Heptane	7.742	163422	7.412 ng/ml
4) t Benzene	7.878	208792	8.498 ng/ml
6) t Toluene	10.611	588123	24.870 ng/ml
7) t Ethylbenzene	13.049	185116	8.553 ng/ml
8) t m-Xylene	13.182	368654	17.035 ng/ml
9) t O-Xylene	13.909	364906	17.162 ng/ml
10) t 1,2,4-Trimethylbenzene	16.184	361365	17.024 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB031424\
Data File : FB030637.D
Signal(s) : FID2B.CH
Acq On : 14 Mar 2024 23:26
Operator : YP/AJ
Sample : P1746-20MSD 50X
Misc : 5.06G/5.00 ML MEOH
ALS Vial : 22 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
SB-06-COMPMSD

Integration File: Calibration.e
Quant Time: Mar 15 03:02:02 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB031124.M
Quant Title :
QLast Update : Mon Mar 11 11:00:59 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

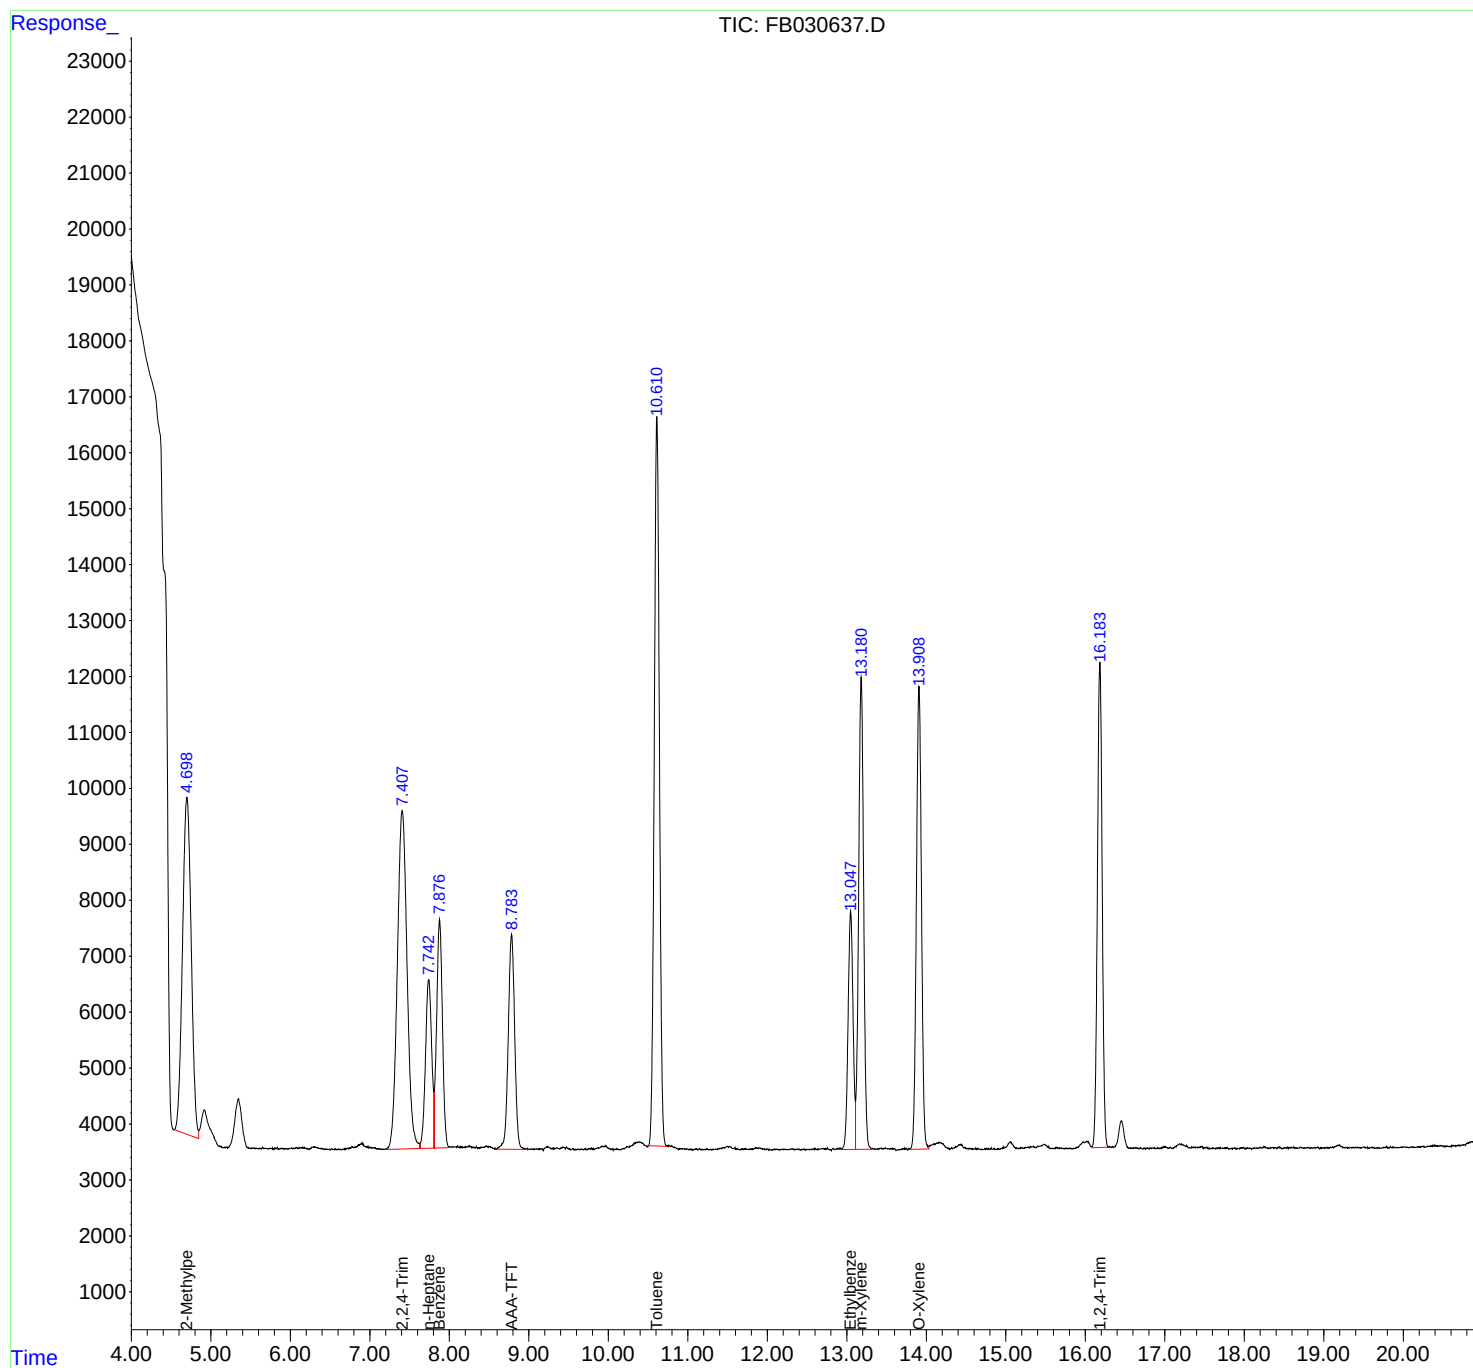


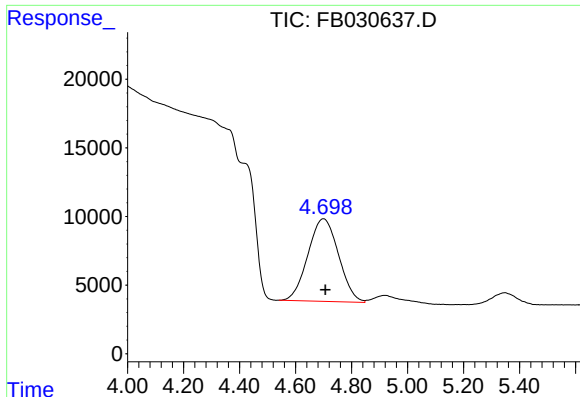

#1 2-Methylpentane


R.T.: 4.700 min
Delta R.T.: -0.007 min
Response: 457795
Conc: 23.25 ng/ml

Instrument :
FID_B
ClientSampleId :
SB-06-COMPMSD

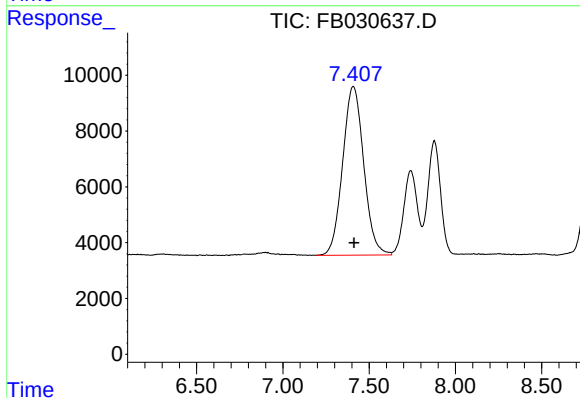


#2 2,2,4-Trimethylpentane

R.T.: 7.408 min
Delta R.T.: -0.004 min
Response: 513016
Conc: 26.24 ng/ml

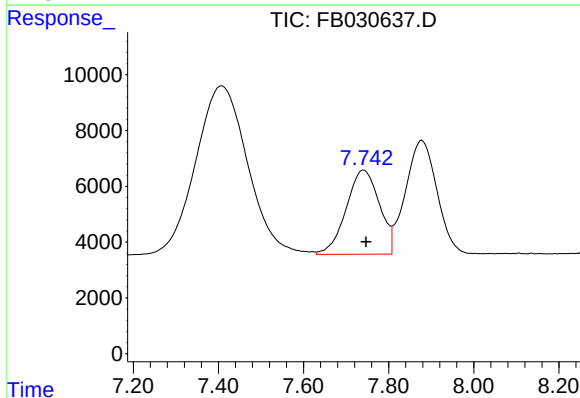


#3 n-Heptane

R.T.: 7.742 min
Delta R.T.: -0.005 min
Response: 163422
Conc: 7.41 ng/ml

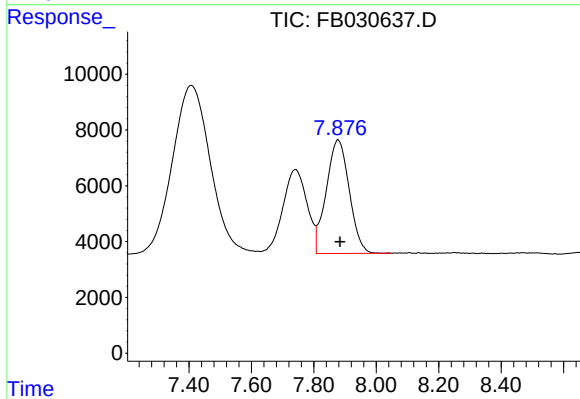

#4 Benzene


R.T.: 7.878 min
Delta R.T.: -0.006 min
Response: 208792
Conc: 8.50 ng/ml

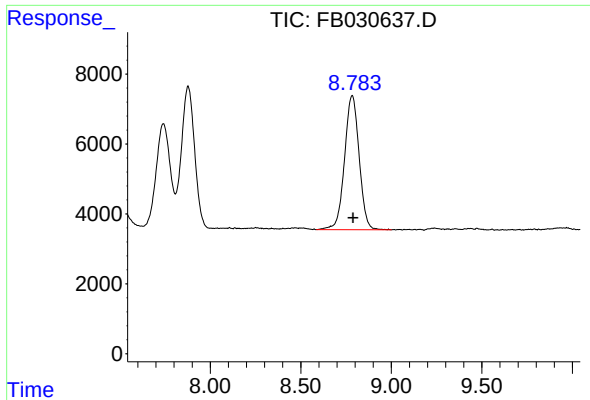

#5 AAA-TFT


R.T.: 8.784 min
Delta R.T.: -0.004 min
Response: 215385
Conc: 15.91 ng/ml

Instrument :
FID_B
ClientSampleId :
SB-06-COMPMSD

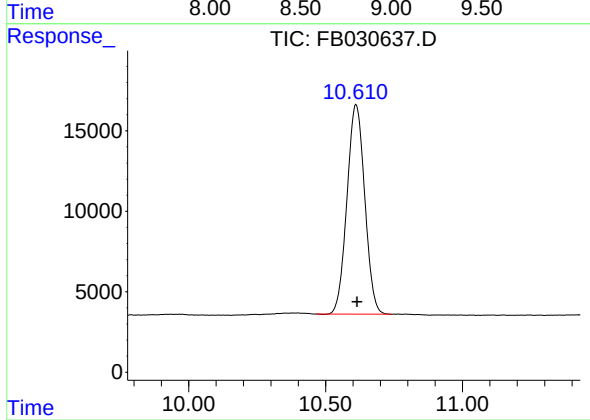


#6 Toluene

R.T.: 10.611 min
Delta R.T.: -0.004 min
Response: 588123
Conc: 24.87 ng/ml

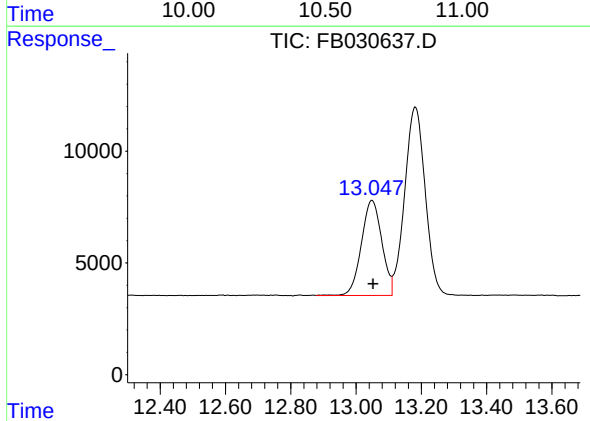


#7 Ethylbenzene

R.T.: 13.049 min
Delta R.T.: -0.003 min
Response: 185116
Conc: 8.55 ng/ml

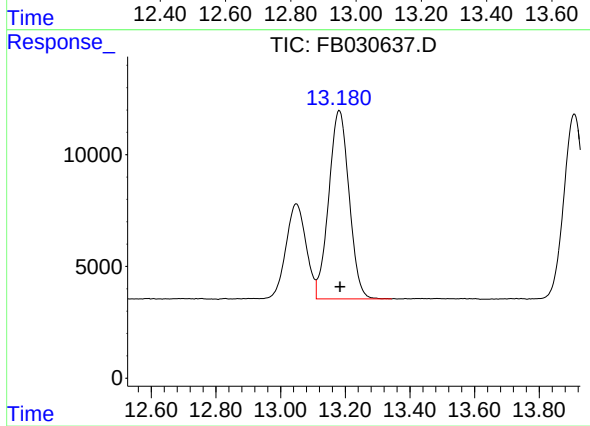

#8 m-Xylene


R.T.: 13.182 min
Delta R.T.: -0.002 min
Response: 368654
Conc: 17.03 ng/ml

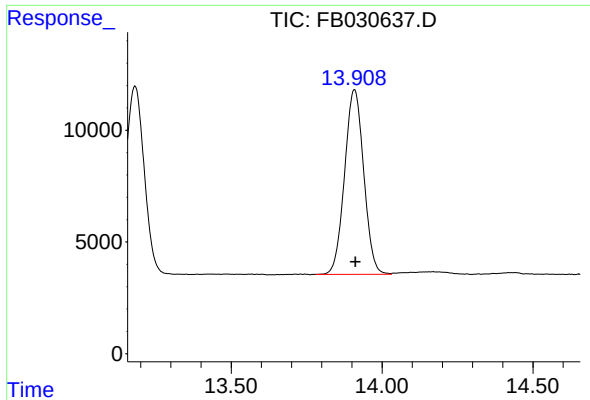

#9 O-Xylene

R.T.: 13.909 min
Delta R.T.: -0.002 min
Response: 364906
Conc: 17.16 ng/ml

Instrument :
FID_B
ClientSampleId :
SB-06-COMPMSD

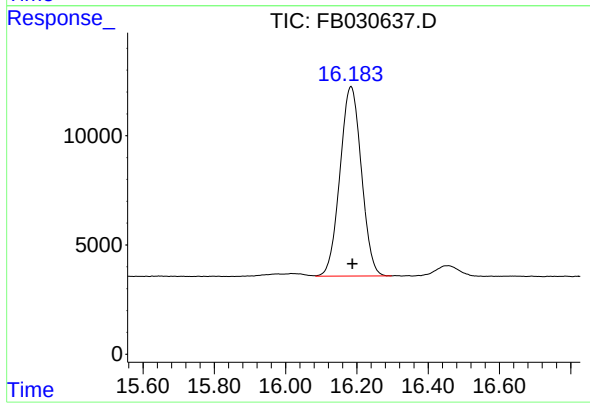

#10 1,2,4-Trimethylbenzene

R.T.: 16.184 min
Delta R.T.: -0.003 min
Response: 361365
Conc: 17.02 ng/ml