

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB031519\
 Data File : FB020225.D
 Signal(s) : FID2B.CH
 Acq On : 15 Mar 2019 9:57
 Operator : MJ/SJ
 Sample : BSF0315S1
 Misc : 5.03g/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0315S1

Integration File: Calibration.e
 Quant Time: Mar 15 12:45:16 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB031119.M
 Quant Title :
 QLast Update : Mon Mar 11 13:44:46 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.042	494089	18.820 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.900	991141	29.382 ng/ml
2) t 2,2,4-Trimethylpentane	7.663	907761	27.681 ng/ml
3) t n-Heptane	7.997	398288	9.570 ng/ml
4) t Benzene	8.134	420119	9.024 ng/ml
6) t Toluene	10.889	959578	25.968 ng/ml
7) t Ethylbenzene	13.342	210594	8.951 ng/ml
8) t m-Xylene	13.475	412601	19.342 ng/ml
9) t O-Xylene	14.207	404700	21.364 ng/ml
10) t 1,2,4-Trimethylbenzene	16.493	425349	21.448 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB031519\
Data File : FB020225.D
Signal(s) : FID2B.CH
Acq On : 15 Mar 2019 9:57
Operator : MJ/SJ
Sample : BSF0315S1
Misc : 5.03g/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0315S1

Integration File: Calibration.e
Quant Time: Mar 15 12:45:16 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB031119.M
Quant Title :
QLast Update : Mon Mar 11 13:44:46 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

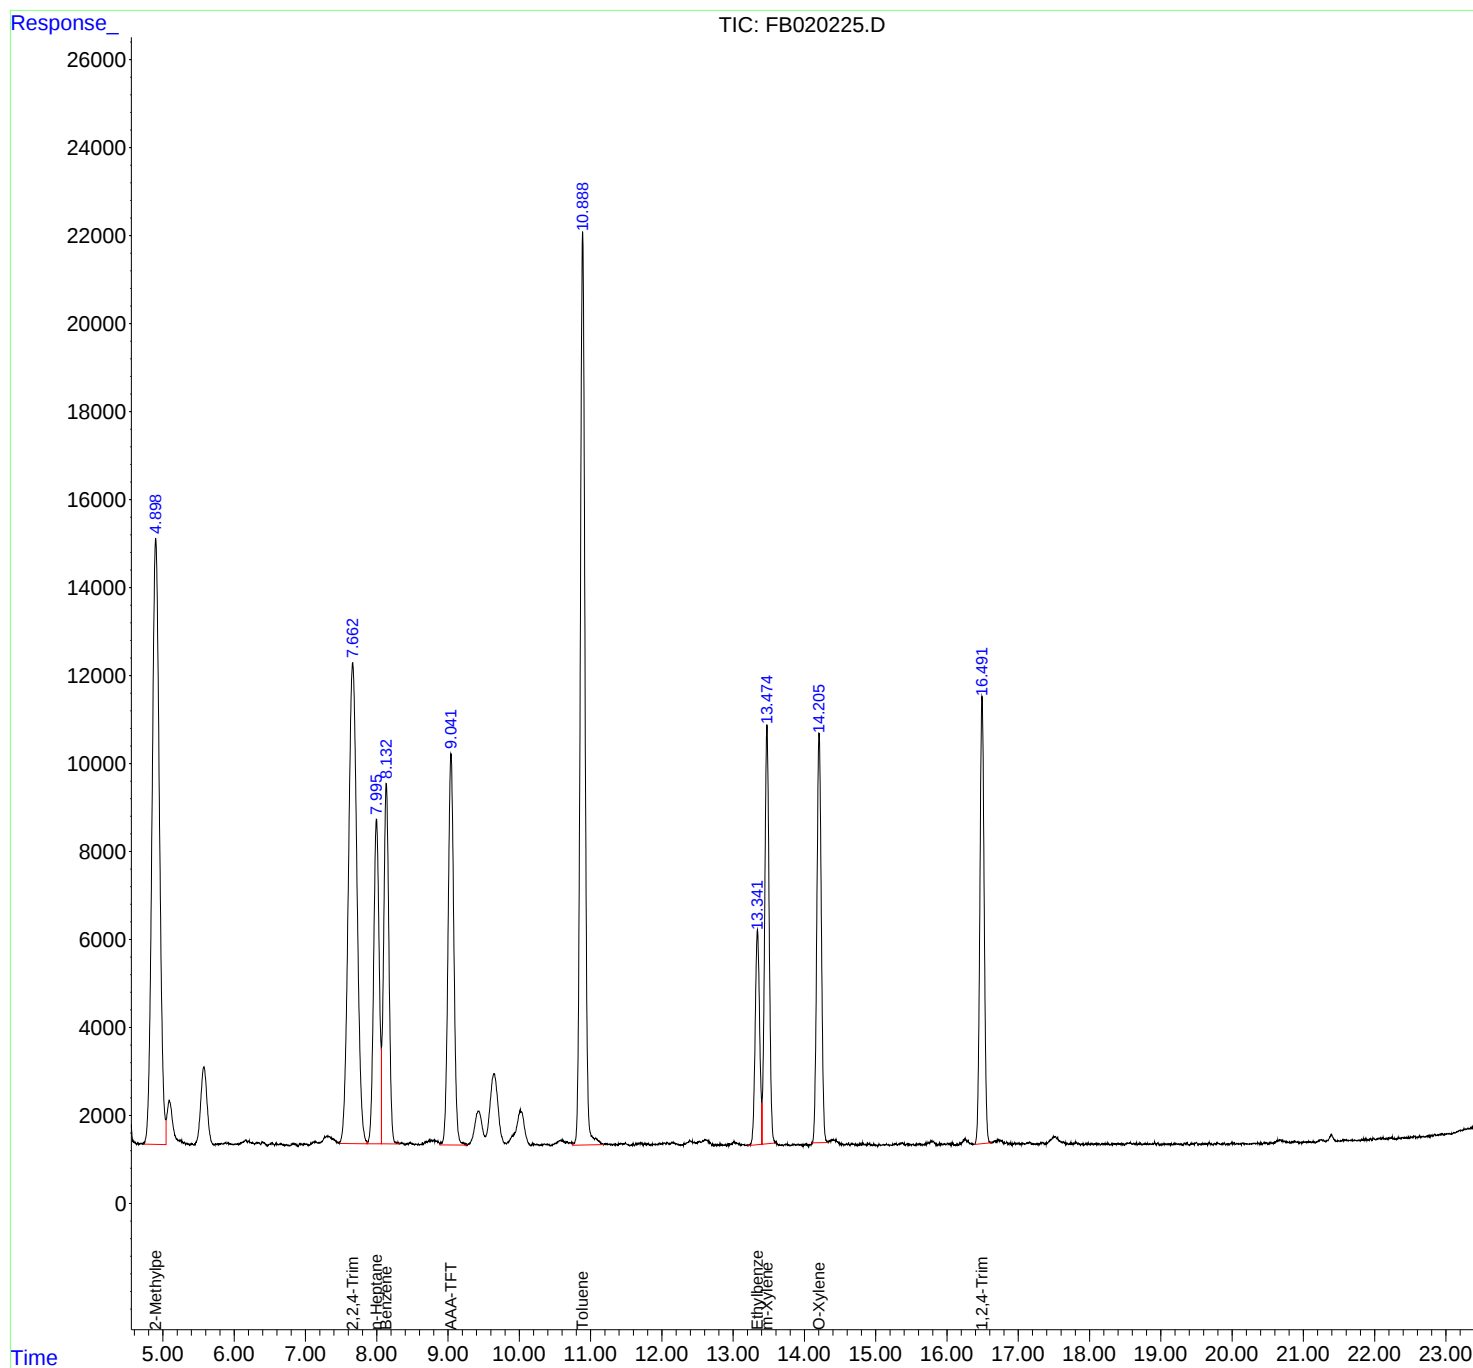


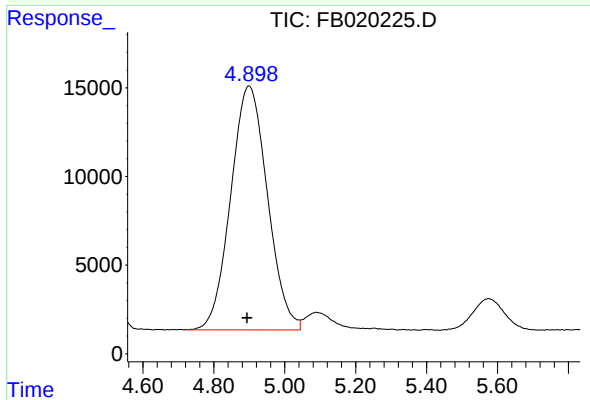

#1 2-Methylpentane


R.T.: 4.900 min
Delta R.T.: 0.006 min
Response: 991141
Conc: 29.38 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0315S1

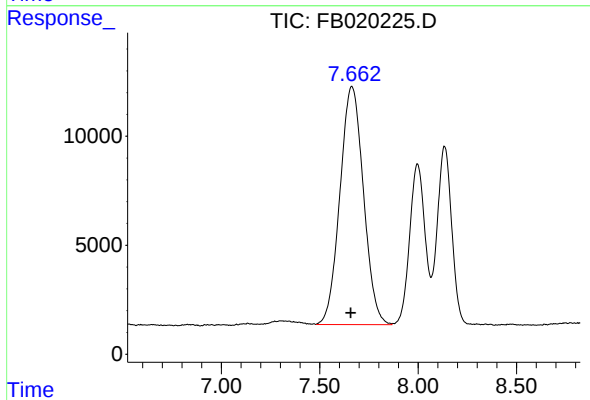


#2 2,2,4-Trimethylpentane

R.T.: 7.663 min
Delta R.T.: 0.006 min
Response: 907761
Conc: 27.68 ng/ml

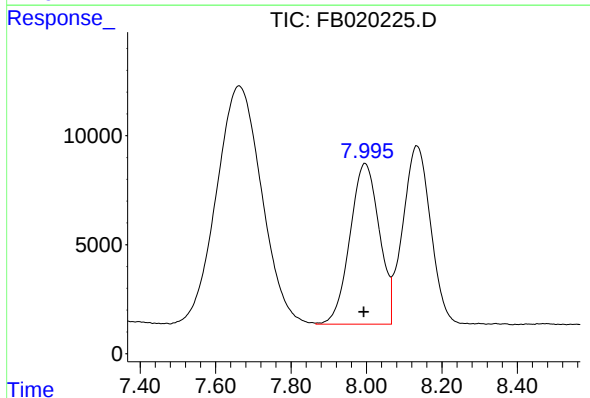


#3 n-Heptane

R.T.: 7.997 min
Delta R.T.: 0.004 min
Response: 398288
Conc: 9.57 ng/ml

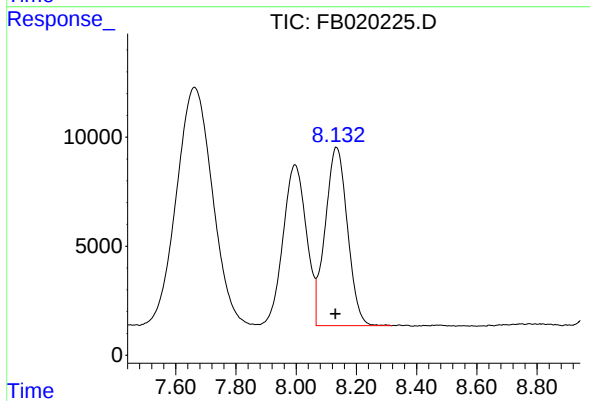

#4 Benzene


R.T.: 8.134 min
Delta R.T.: 0.004 min
Response: 420119
Conc: 9.02 ng/ml

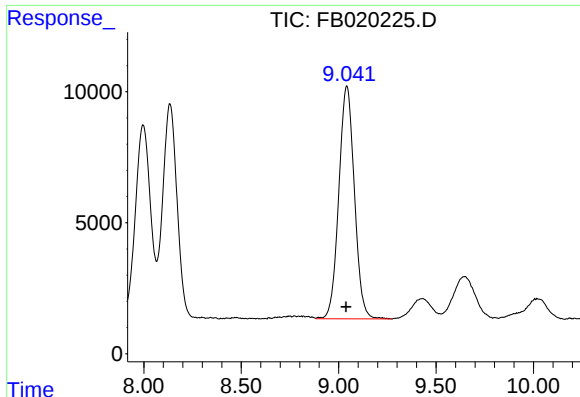

#5 AAA-TFT


R.T.: 9.042 min
Delta R.T.: 0.004 min
Response: 494089
Conc: 18.82 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0315S1

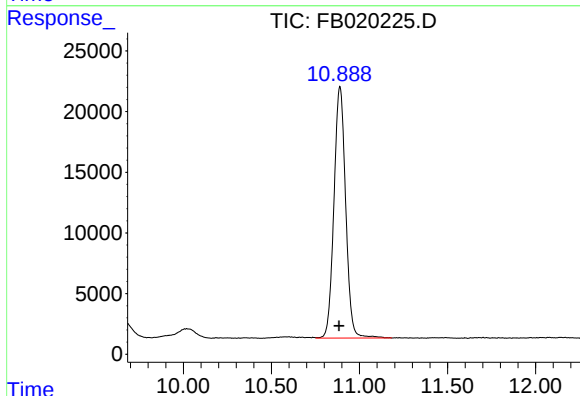


#6 Toluene

R.T.: 10.889 min
Delta R.T.: 0.004 min
Response: 959578
Conc: 25.97 ng/ml

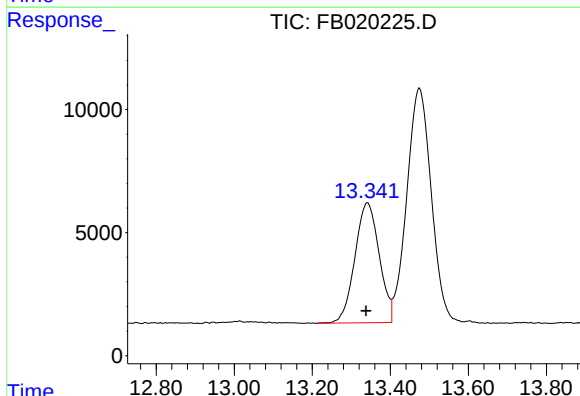


#7 Ethylbenzene

R.T.: 13.342 min
Delta R.T.: 0.004 min
Response: 210594
Conc: 8.95 ng/ml

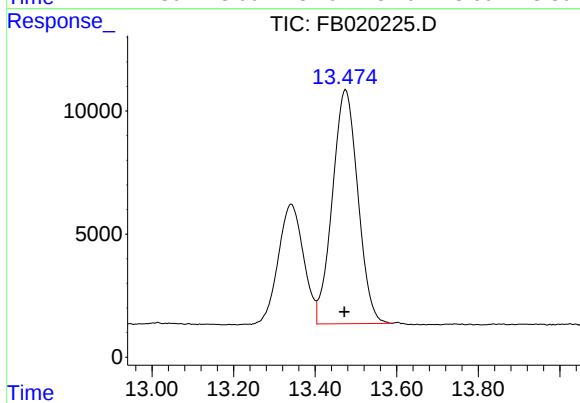

#8 m-Xylene

R.T.: 13.475 min
Delta R.T.: 0.004 min
Response: 412601
Conc: 19.34 ng/ml

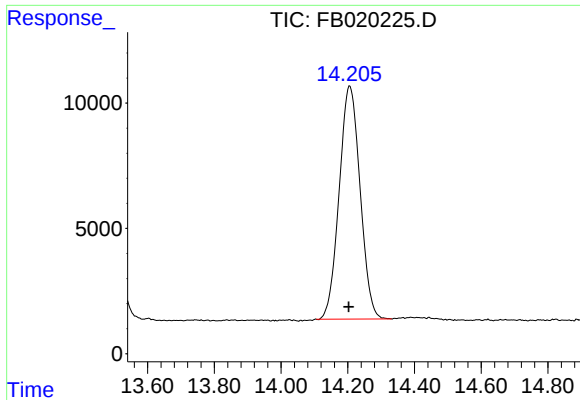

#9 O-Xylene


R.T.: 14.207 min

Delta R.T.: 0.003 min

Response: 404700

Conc: 21.36 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0315S1

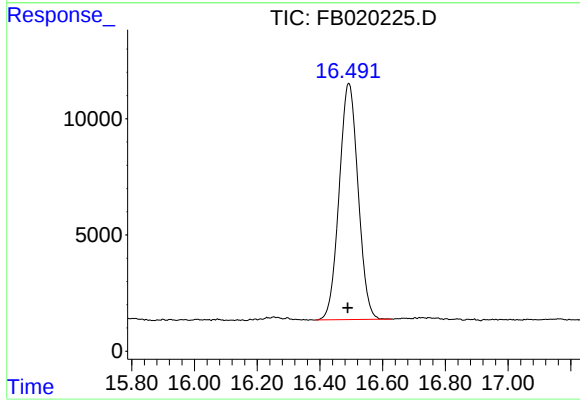

#10 1,2,4-Trimethylbenzene

R.T.: 16.493 min

Delta R.T.: 0.004 min

Response: 425349

Conc: 21.45 ng/ml