

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB031519\
 Data File : FB020229.D
 Signal(s) : FID2B.CH
 Acq On : 15 Mar 2019 11:58
 Operator : MJ/SJ
 Sample : K1930-07
 Misc : 5.05g/5.00ml DI WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 TP-4-B

Integration File: Calibration.e
 Quant Time: Mar 15 12:45:29 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB031119.M
 Quant Title :
 QLast Update : Mon Mar 11 13:44:46 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.045	449614	17.126 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.890	11516	0.341 ng/ml
2) t 2,2,4-Trimethylpentane	7.667	46740	1.425 ng/ml
3) t n-Heptane	7.992	5104	0.123 ng/ml
4) t Benzene	8.141	6945	0.149 ng/ml
6) t Toluene	10.895	11372	0.308 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB031519\
Data File : FB020229.D
Signal(s) : FID2B.CH
Acq On : 15 Mar 2019 11:58
Operator : MJ/SJ
Sample : K1930-07
Misc : 5.05g/5.00ml DI WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
TP-4-B

Integration File: Calibration.e
Quant Time: Mar 15 12:45:29 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB031119.M
Quant Title :
QLast Update : Mon Mar 11 13:44:46 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

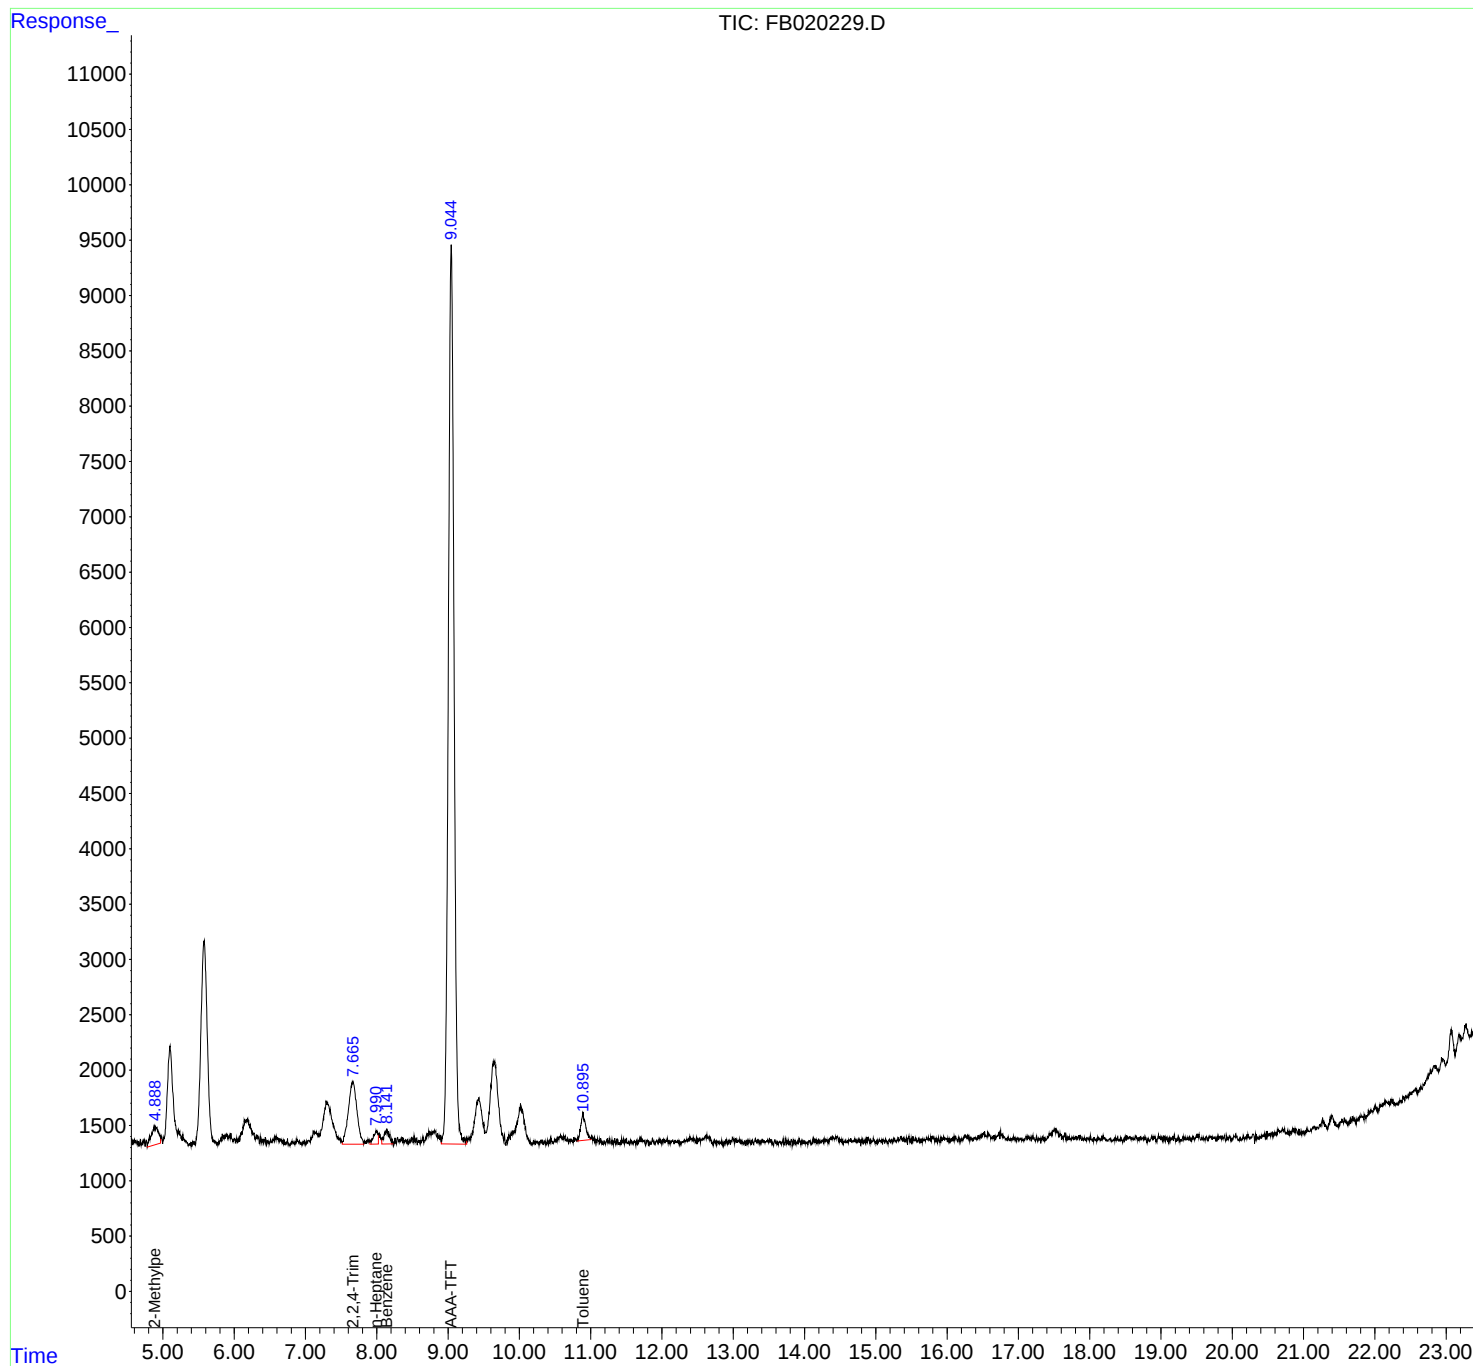


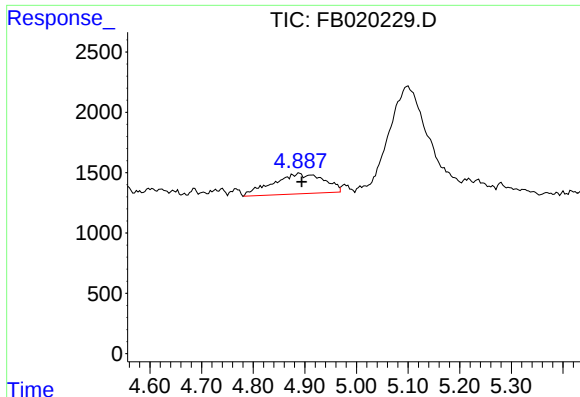

#1 2-Methylpentane


R.T.: 4.890 min
Delta R.T.: -0.004 min
Response: 11516
Conc: 0.34 ng/ml

Instrument :
FID_B
ClientSampleId :
TP-4-B

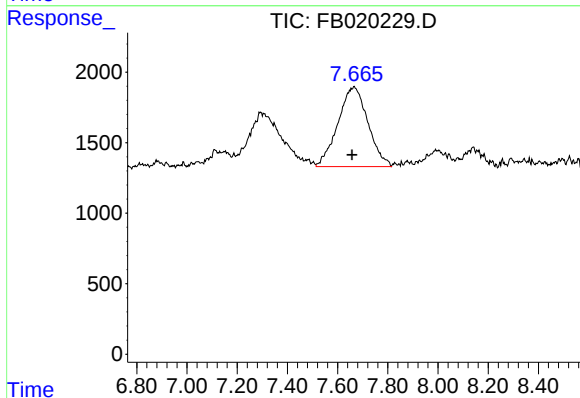


#2 2,2,4-Trimethylpentane

R.T.: 7.667 min
Delta R.T.: 0.010 min
Response: 46740
Conc: 1.43 ng/ml

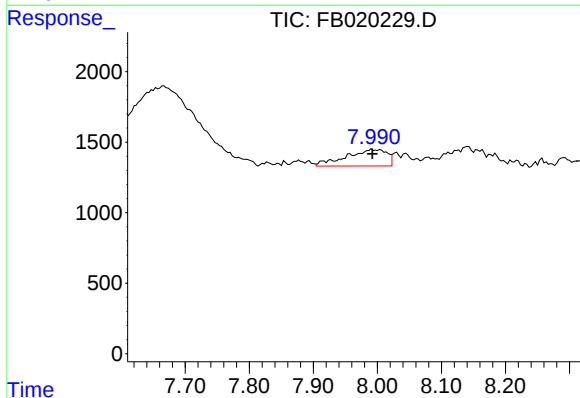


#3 n-Heptane

R.T.: 7.992 min
Delta R.T.: 0.000 min
Response: 5104
Conc: 0.12 ng/ml

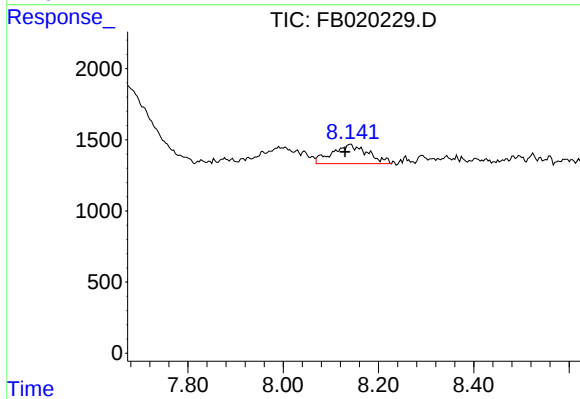

#4 Benzene


R.T.: 8.141 min
Delta R.T.: 0.011 min
Response: 6945
Conc: 0.15 ng/ml

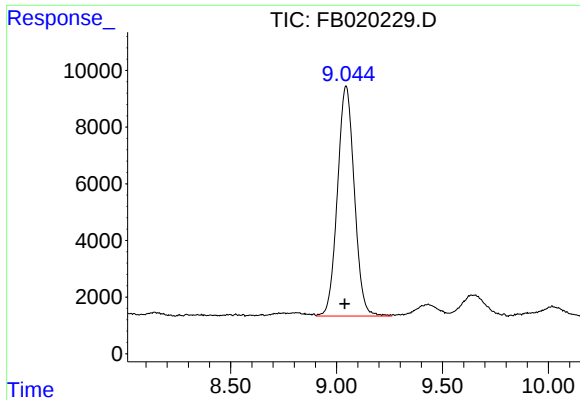

#5 AAA-TFT

R.T.: 9.045 min
Delta R.T.: 0.007 min
Response: 449614
Conc: 17.13 ng/ml

Instrument :
FID_B
ClientSampleId :
TP-4-B

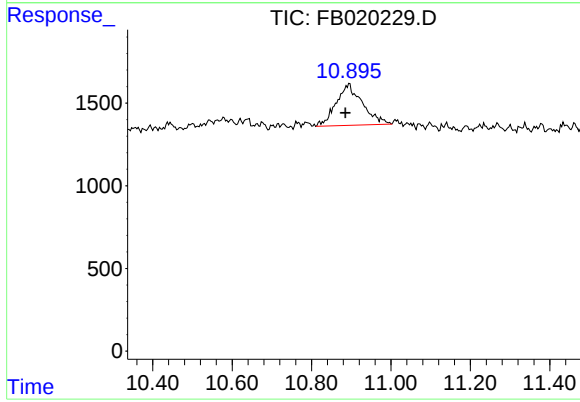

#6 Toluene

R.T.: 10.895 min
Delta R.T.: 0.010 min
Response: 11372
Conc: 0.31 ng/ml