

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB031519\
Data File : FB020231.D
Signal(s) : FID2B.CH
Acq On : 15 Mar 2019 12:58
Operator : MJ/SJ
Sample : K1873-03
Misc : 5.02g/5.00ml DI WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
371-B

Integration File: Calibration.e
Quant Time: Mar 15 13:42:36 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB031119.M
Quant Title :
QLast Update : Mon Mar 11 13:44:46 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.045	468966	17.864 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.882	3300	0.098 ng/ml
2) t 2,2,4-Trimethylpentane	7.665	47269	1.441 ng/ml
3) t n-Heptane	7.999	6985	0.168 ng/ml
4) t Benzene	8.150	5723	0.123 ng/ml
6) t Toluene	10.889	15560	0.421 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB031519\
Data File : FB020231.D
Signal(s) : FID2B.CH
Acq On : 15 Mar 2019 12:58
Operator : MJ/SJ
Sample : K1873-03
Misc : 5.02g/5.00ml DI WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
371-B

Integration File: Calibration.e
Quant Time: Mar 15 13:42:36 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB031119.M
Quant Title :
QLast Update : Mon Mar 11 13:44:46 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

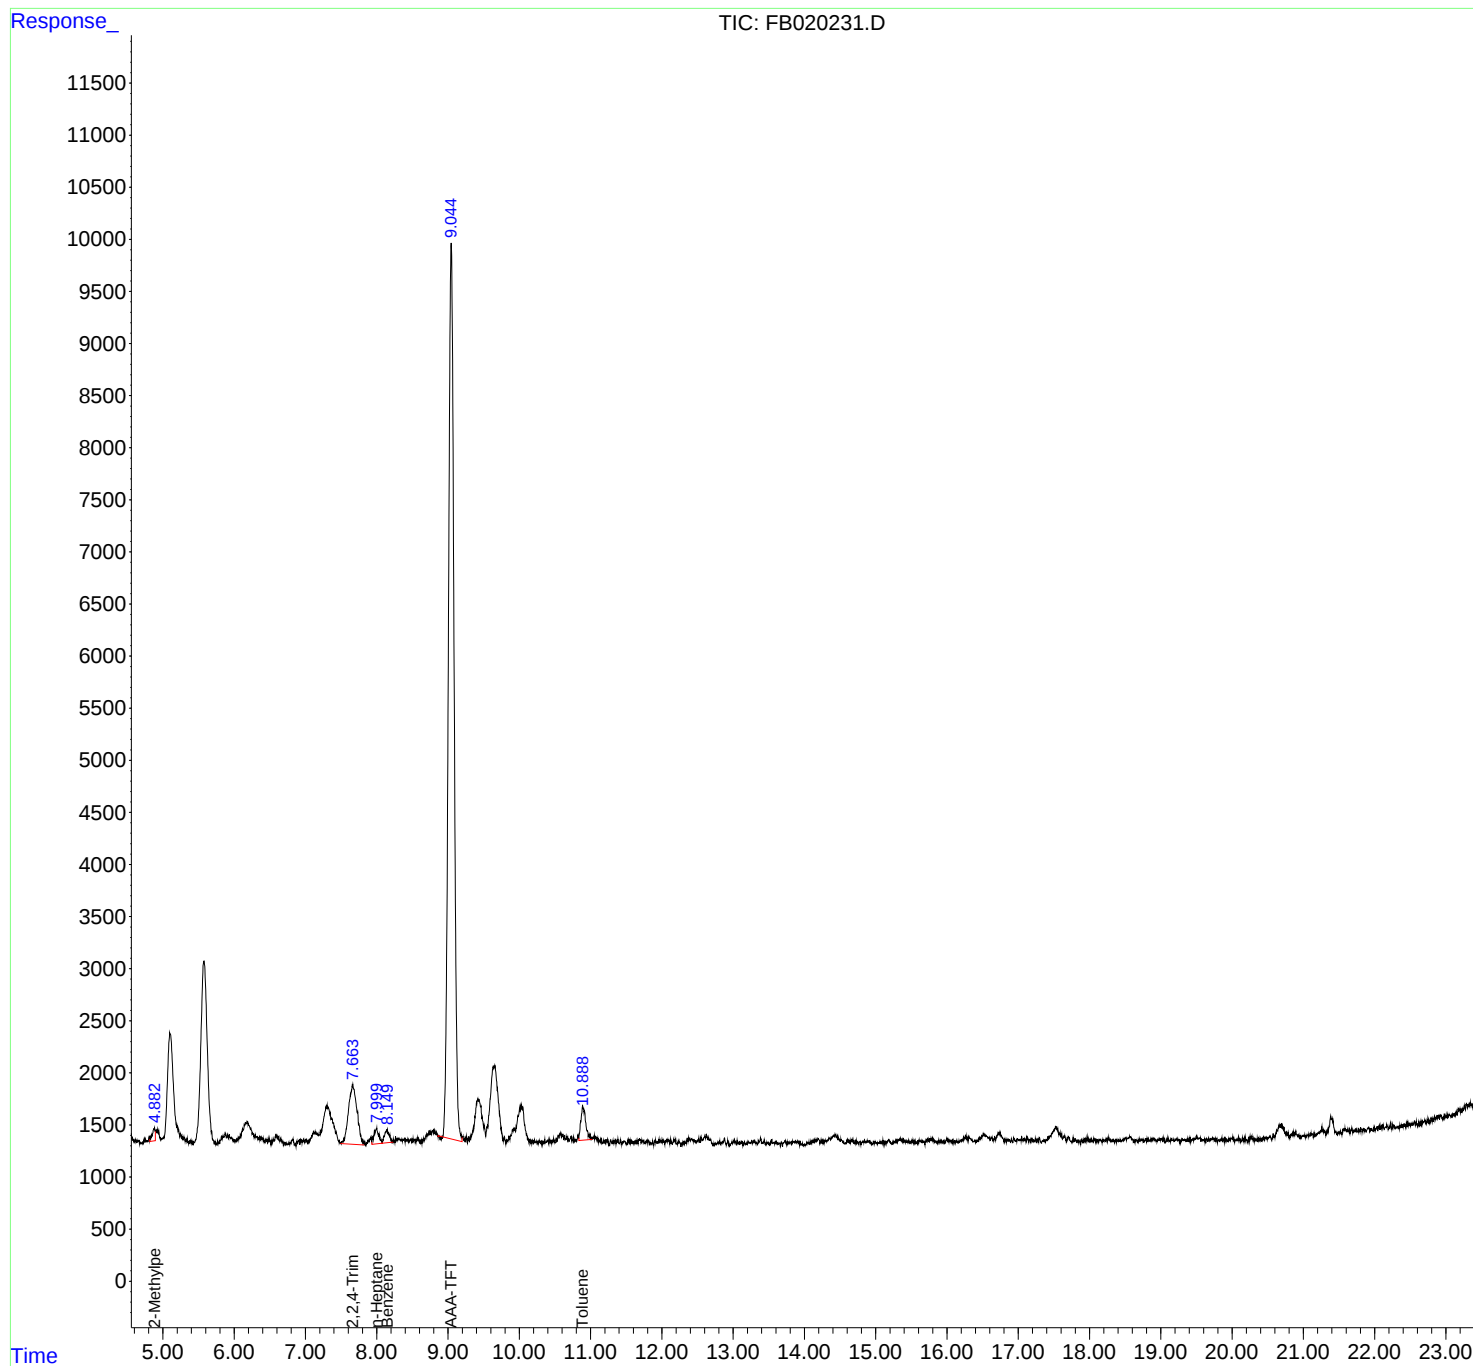


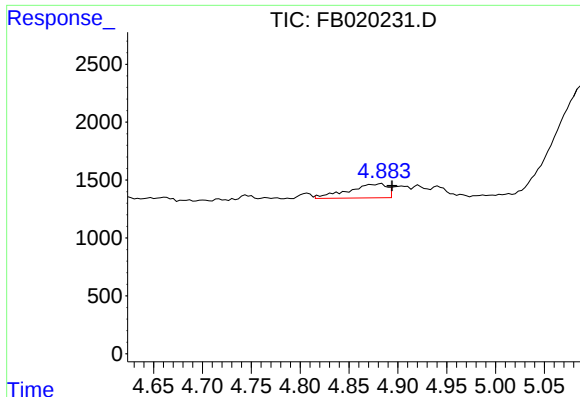

#1 2-Methylpentane


R.T.: 4.882 min
Delta R.T.: -0.012 min
Response: 3300
Conc: 0.10 ng/ml

Instrument :
FID_B
ClientSampleId :
371-B

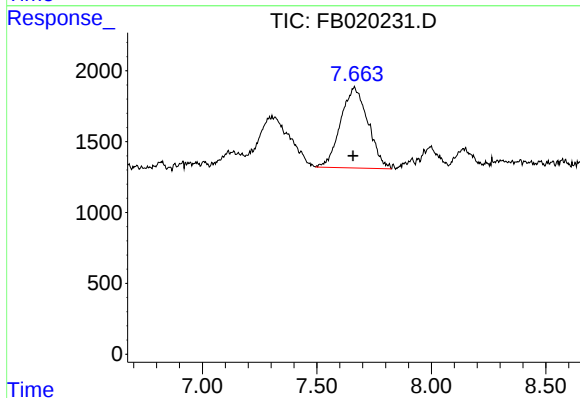


#2 2,2,4-Trimethylpentane

R.T.: 7.665 min
Delta R.T.: 0.008 min
Response: 47269
Conc: 1.44 ng/ml

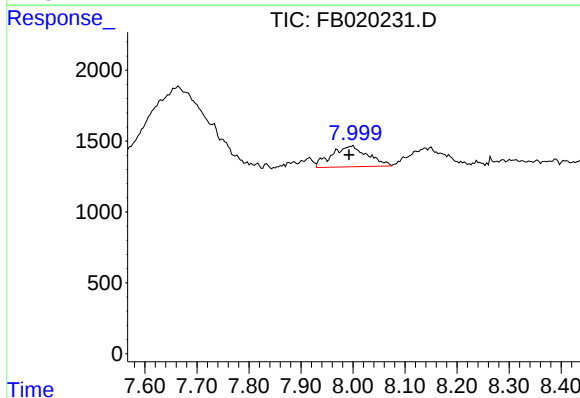


#3 n-Heptane

R.T.: 7.999 min
Delta R.T.: 0.006 min
Response: 6985
Conc: 0.17 ng/ml

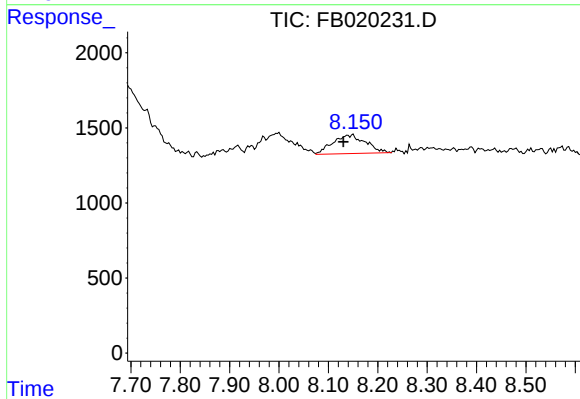

#4 Benzene


R.T.: 8.150 min
Delta R.T.: 0.020 min
Response: 5723
Conc: 0.12 ng/ml

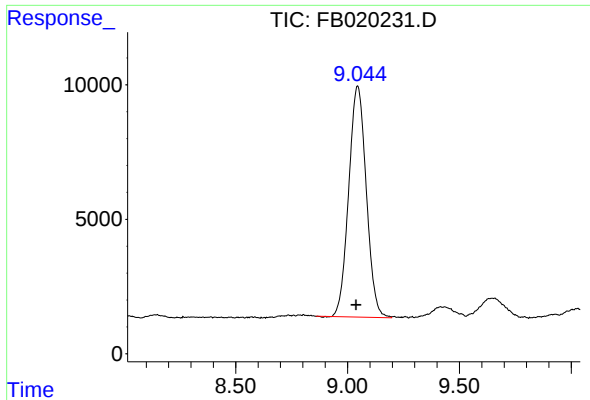

#5 AAA-TFT

R.T.: 9.045 min
Delta R.T.: 0.007 min
Response: 468966
Conc: 17.86 ng/ml

Instrument :
FID_B
ClientSampleId :
371-B

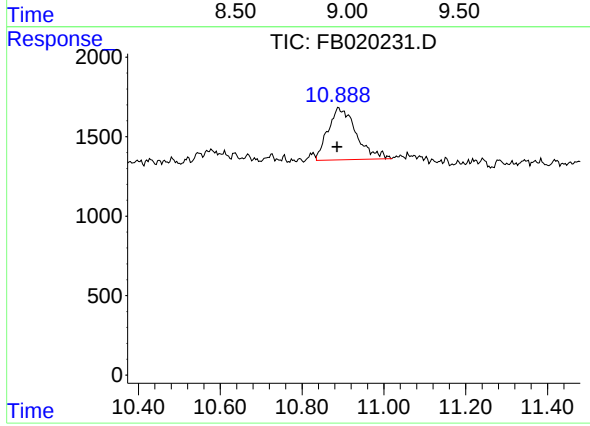

#6 Toluene

R.T.: 10.889 min
Delta R.T.: 0.004 min
Response: 15560
Conc: 0.42 ng/ml