

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB031519\
 Data File : FB020233.D
 Signal(s) : FID2B.CH
 Acq On : 15 Mar 2019 13:59
 Operator : MJ/SJ
 Sample : K1922-02 50X
 Misc : 5.00g/5.00ml DI WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 ORG-031419

Integration File: Calibration.e
 Quant Time: Mar 15 14:16:10 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB031119.M
 Quant Title :
 QLast Update : Mon Mar 11 13:44:46 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.046	551489	21.007 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.898	29506	0.875 ng/ml
2) t 2,2,4-Trimethylpentane	7.672	86757	2.646 ng/ml
3) t n-Heptane	8.000	175314	4.213 ng/ml
4) t Benzene	8.142	7067	0.152 ng/ml
6) t Toluene	10.914	37144	1.005 ng/ml
7) t Ethylbenzene	13.316	72750	3.092 ng/ml
8) t m-Xylene	13.432	6458	0.303 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB031519\
Data File : FB020233.D
Signal(s) : FID2B.CH
Acq On : 15 Mar 2019 13:59
Operator : MJ/SJ
Sample : K1922-02 50X
Misc : 5.00g/5.00ml DI WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
ORG-031419

Integration File: Calibration.e
Quant Time: Mar 15 14:16:10 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB031119.M
Quant Title :
QLast Update : Mon Mar 11 13:44:46 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

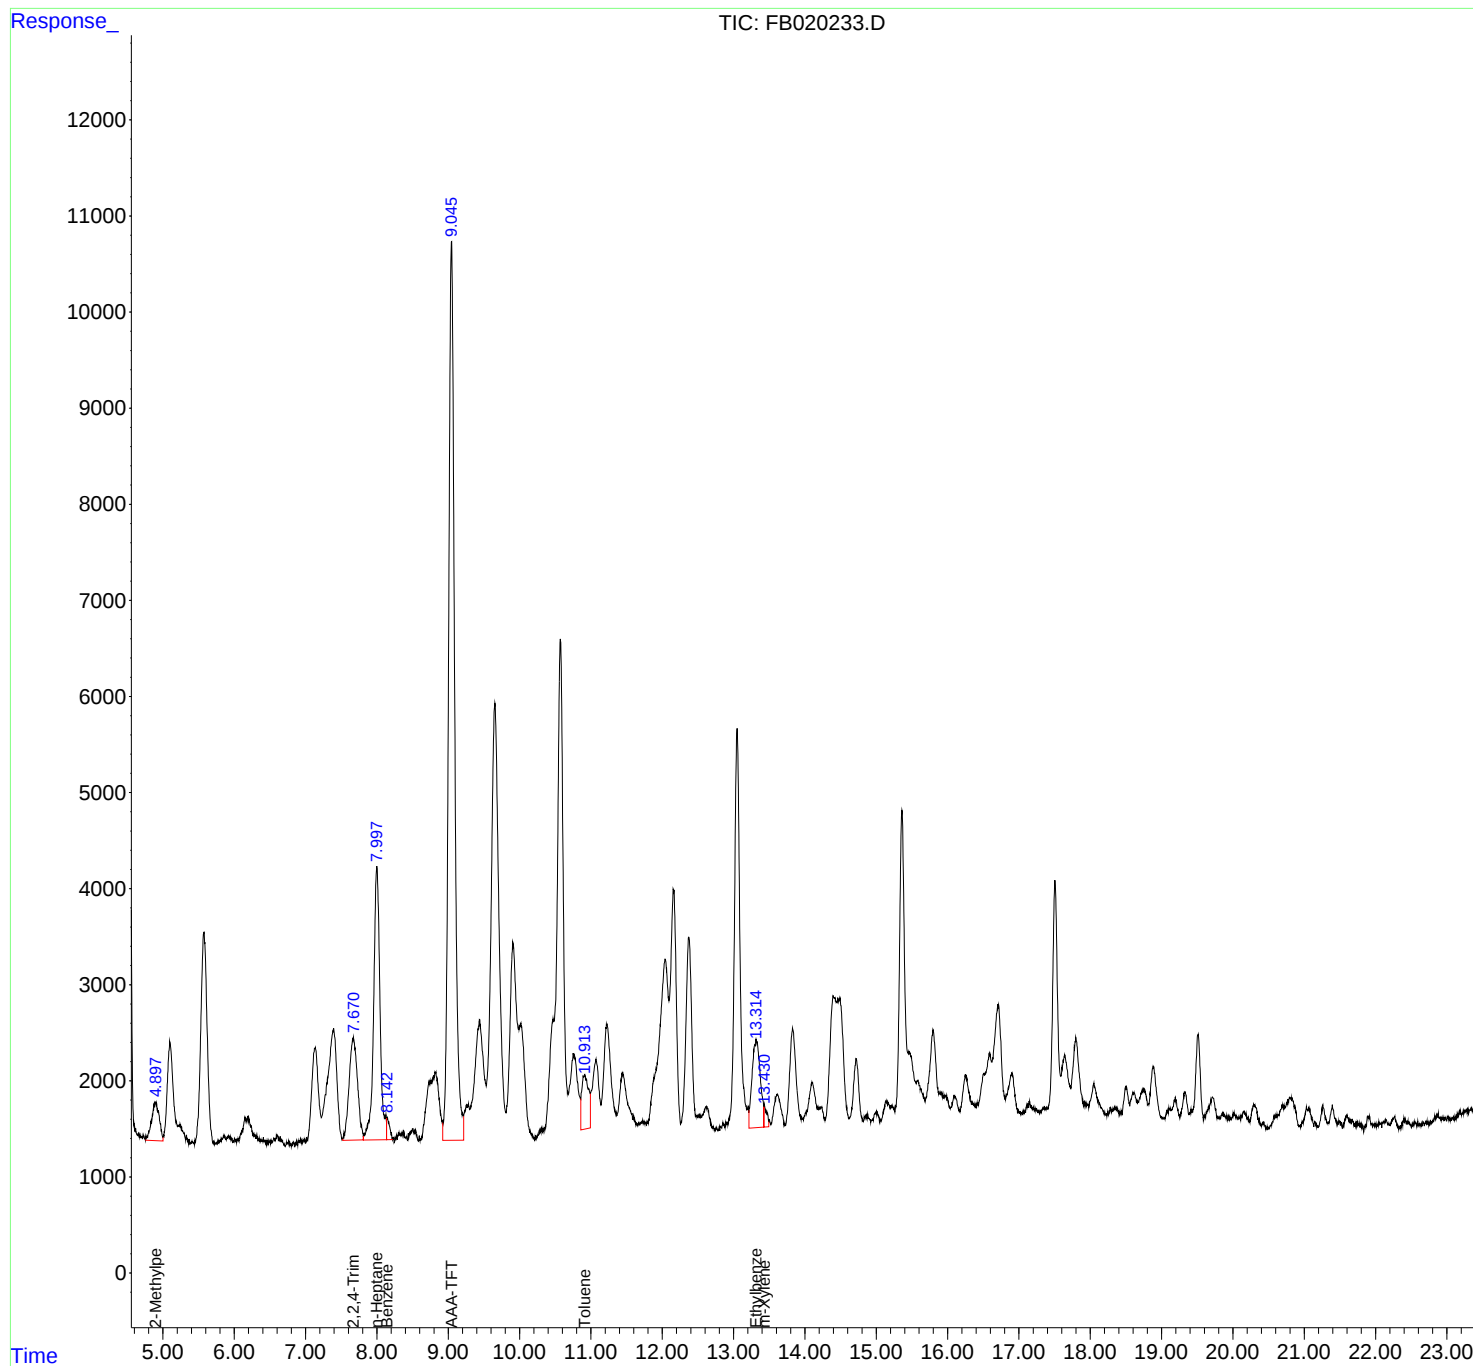


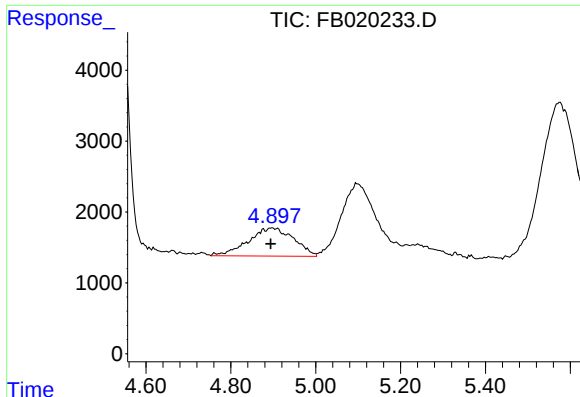

#1 2-Methylpentane


R.T.: 4.898 min
Delta R.T.: 0.004 min
Response: 29506
Conc: 0.87 ng/ml

Instrument :
FID_B
ClientSampleId :
ORG-031419

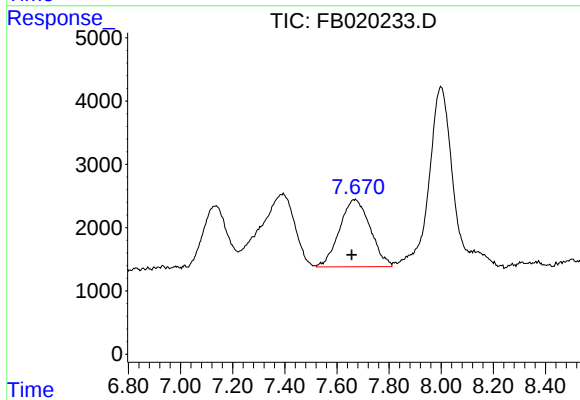


#2 2,2,4-Trimethylpentane

R.T.: 7.672 min
Delta R.T.: 0.014 min
Response: 86757
Conc: 2.65 ng/ml

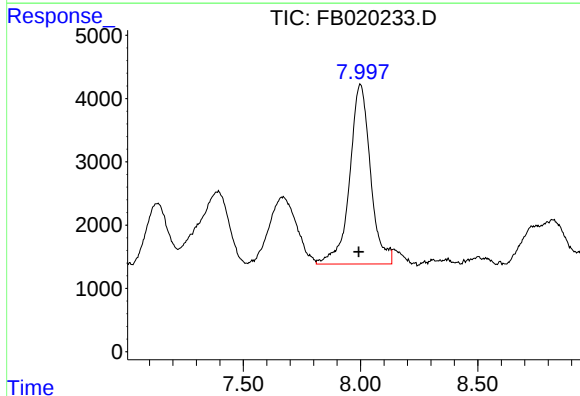


#3 n-Heptane

R.T.: 8.000 min
Delta R.T.: 0.007 min
Response: 175314
Conc: 4.21 ng/ml

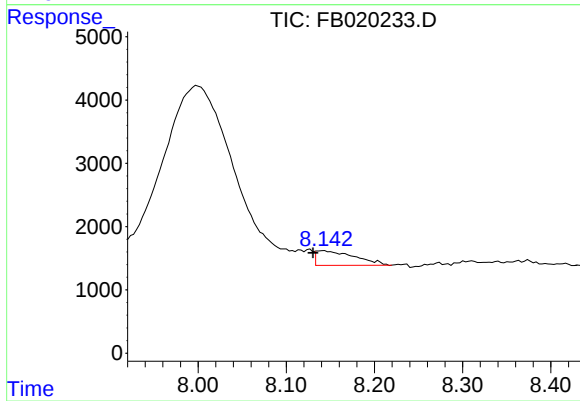

#4 Benzene


R.T.: 8.142 min
Delta R.T.: 0.012 min
Response: 7067
Conc: 0.15 ng/ml

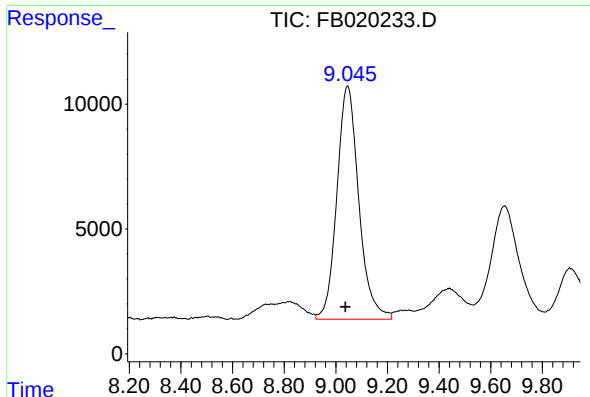

#5 AAA-TFT


R.T.: 9.046 min
Delta R.T.: 0.008 min
Response: 551489
Conc: 21.01 ng/ml

Instrument :
FID_B
ClientSampleId :
ORG-031419

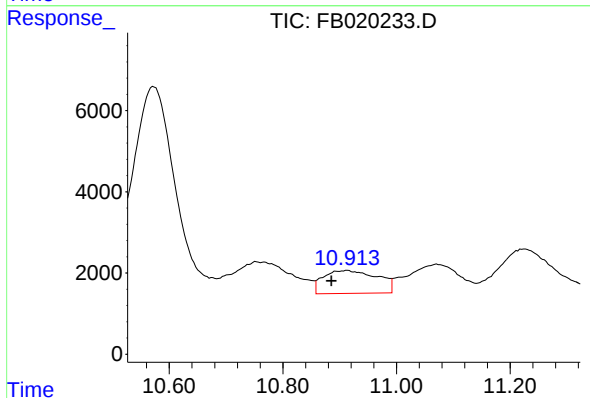


#6 Toluene

R.T.: 10.914 min
Delta R.T.: 0.029 min
Response: 37144
Conc: 1.01 ng/ml

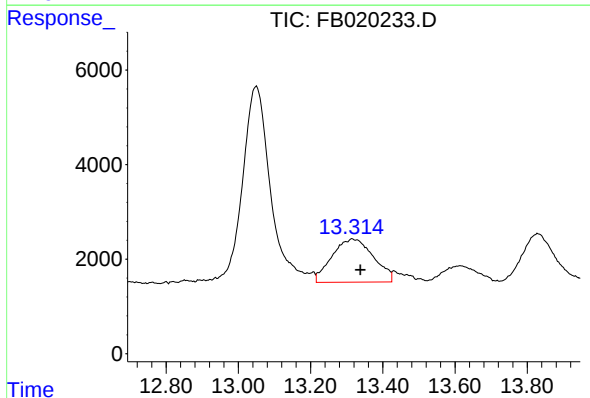

#7 Ethylbenzene

R.T.: 13.316 min
Delta R.T.: -0.022 min
Response: 72750
Conc: 3.09 ng/ml

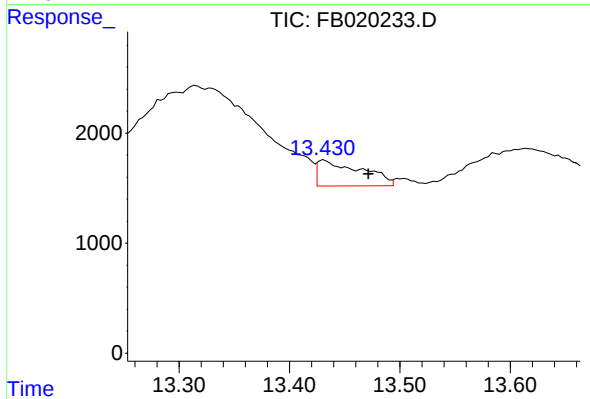

#8 m-Xylene

R.T.: 13.432 min
Delta R.T.: -0.040 min
Response: 6458
Conc: 0.30 ng/ml