

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB031519\
 Data File : FB020234.D
 Signal(s) : FID2B.CH
 Acq On : 15 Mar 2019 14:30
 Operator : MJ/SJ
 Sample : K1930-02MS
 Misc : 5.02g/5.00ml DI WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 TP-3-AMS

Integration File: Calibration.e
 Quant Time: Mar 15 15:33:54 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB031119.M
 Quant Title :
 QLast Update : Mon Mar 11 13:44:46 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.045	441849	16.831 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.901	786090	23.303 ng/ml
2) t 2,2,4-Trimethylpentane	7.667	689582	21.028 ng/ml
3) t n-Heptane	8.000	293661	7.056 ng/ml
4) t Benzene	8.138	394409	8.471 ng/ml
6) t Toluene	10.893	858482	23.232 ng/ml
7) t Ethylbenzene	13.346	181560	7.717 ng/ml
8) t m-Xylene	13.479	344389	16.144 ng/ml
9) t O-Xylene	14.212	335436	17.708 ng/ml
10) t 1,2,4-Trimethylbenzene	16.497	332461	16.764 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB031519\
Data File : FB020234.D
Signal(s) : FID2B.CH
Acq On : 15 Mar 2019 14:30
Operator : MJ/SJ
Sample : K1930-02MS
Misc : 5.02g/5.00ml DI WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
TP-3-AMS

Integration File: Calibration.e
Quant Time: Mar 15 15:33:54 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB031119.M
Quant Title :
QLast Update : Mon Mar 11 13:44:46 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

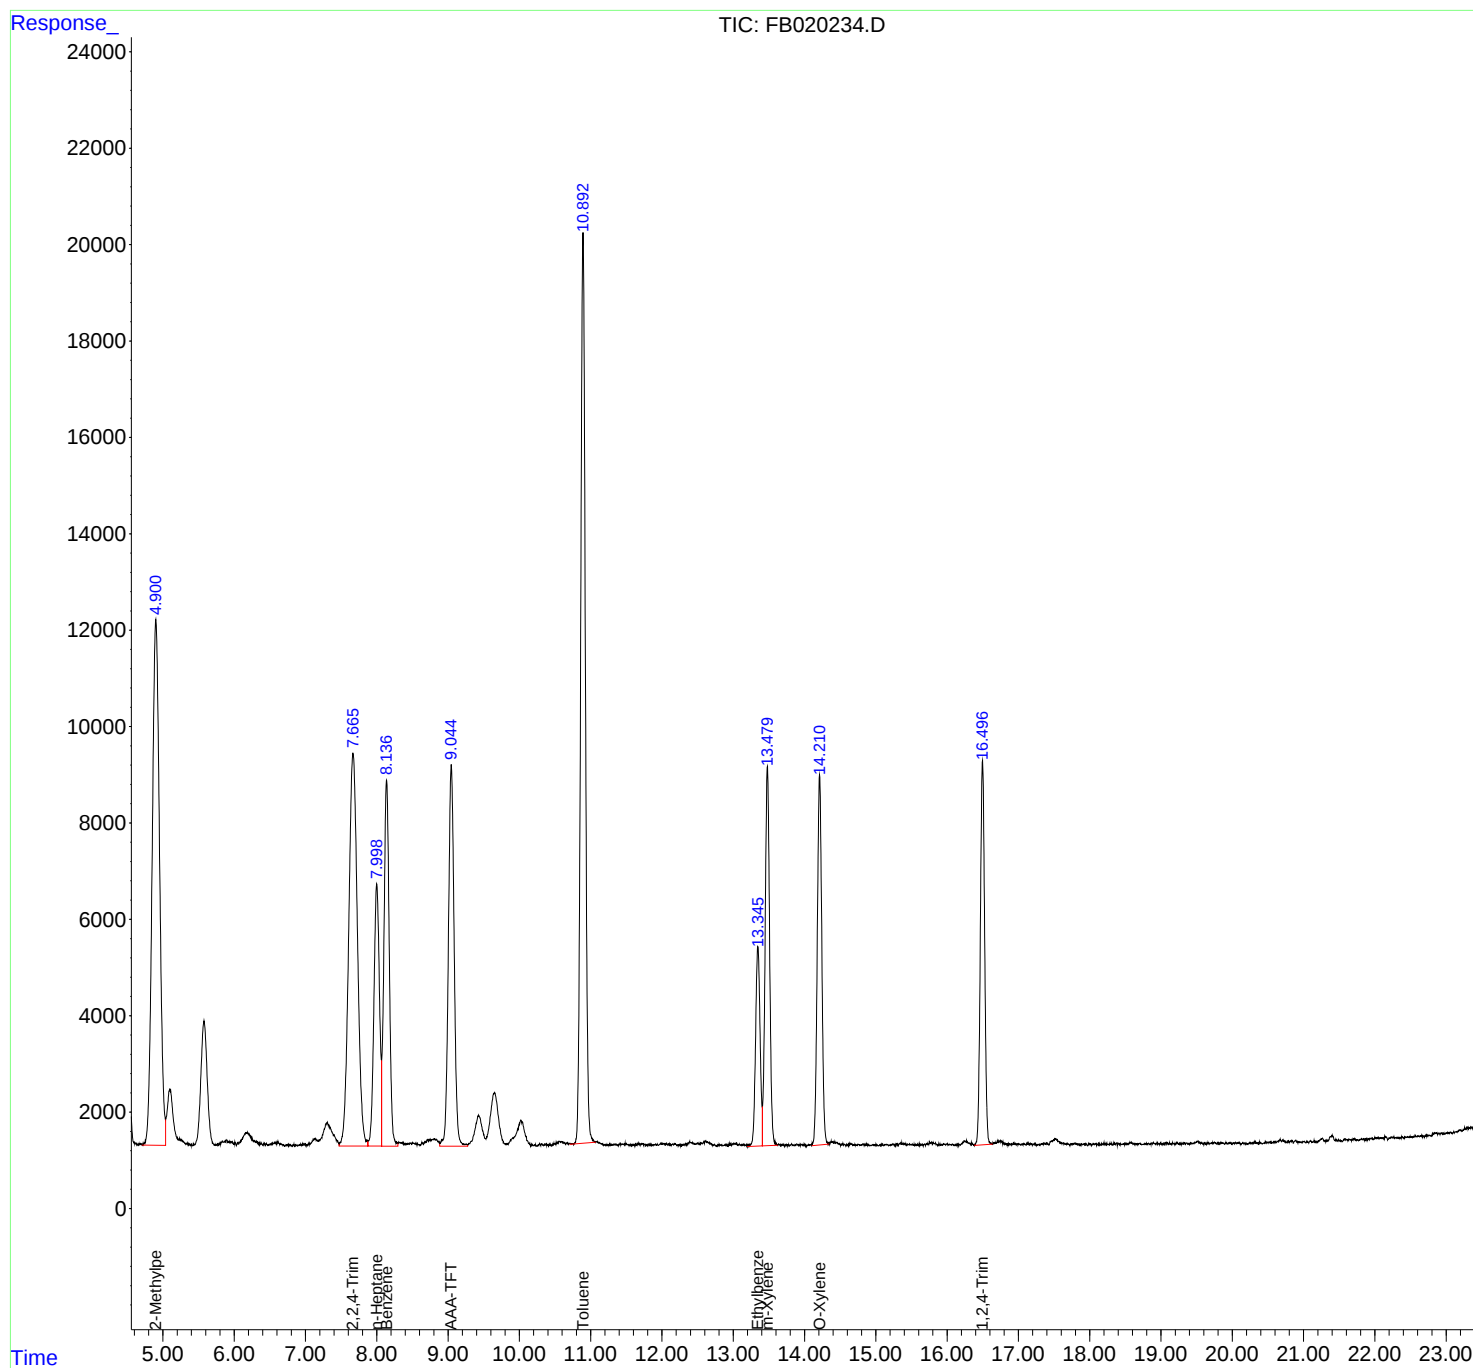


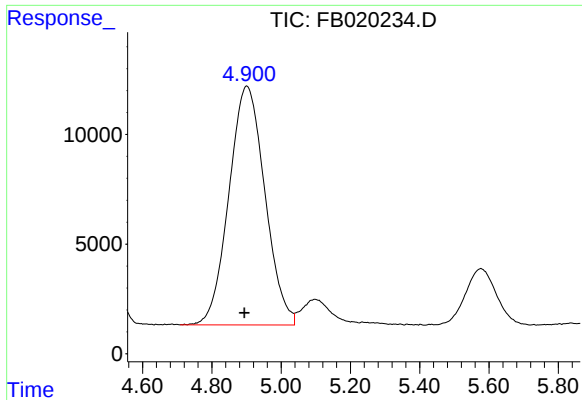

#1 2-Methylpentane


R.T.: 4.901 min
Delta R.T.: 0.007 min
Response: 786090
Conc: 23.30 ng/ml

Instrument :
FID_B
ClientSampleId :
TP-3-AMS

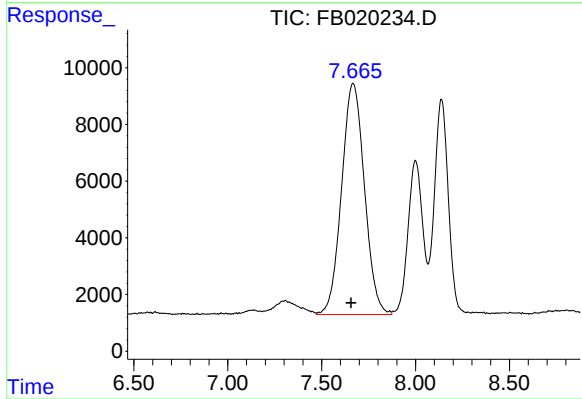


#2 2,2,4-Trimethylpentane

R.T.: 7.667 min
Delta R.T.: 0.010 min
Response: 689582
Conc: 21.03 ng/ml

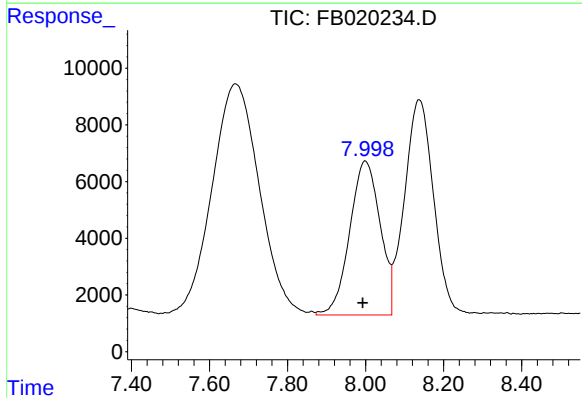


#3 n-Heptane

R.T.: 8.000 min
Delta R.T.: 0.007 min
Response: 293661
Conc: 7.06 ng/ml

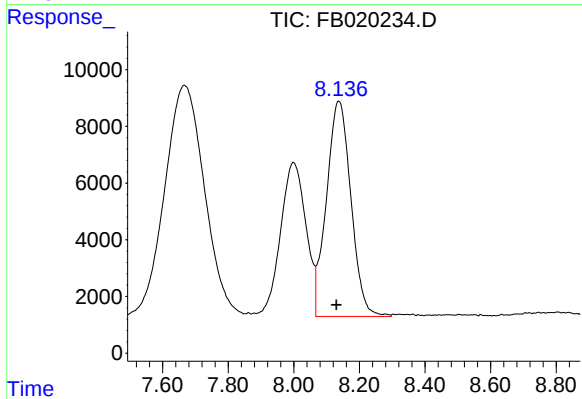

#4 Benzene


R.T.: 8.138 min
Delta R.T.: 0.008 min
Response: 394409
Conc: 8.47 ng/ml

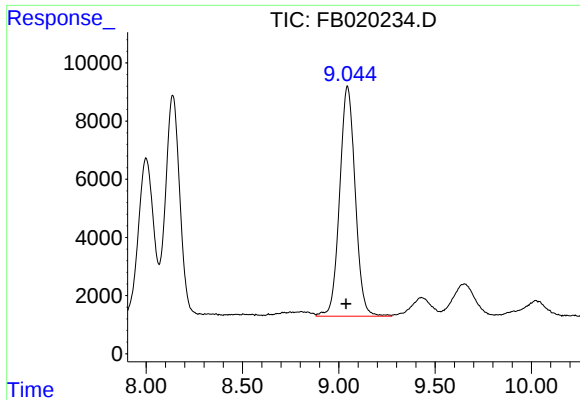

#5 AAA-TFT


R.T.: 9.045 min
Delta R.T.: 0.007 min
Response: 441849
Conc: 16.83 ng/ml

Instrument :
FID_B
ClientSampleId :
TP-3-AMS

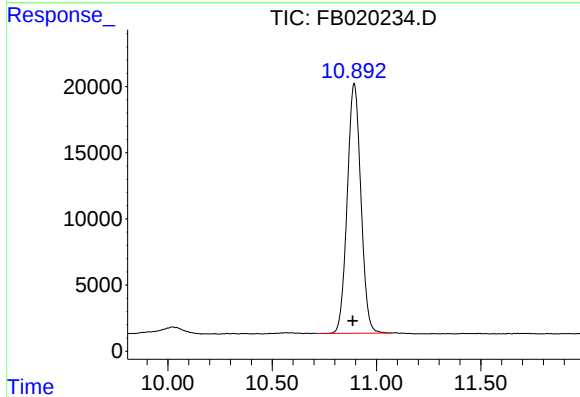


#6 Toluene

R.T.: 10.893 min
Delta R.T.: 0.008 min
Response: 858482
Conc: 23.23 ng/ml

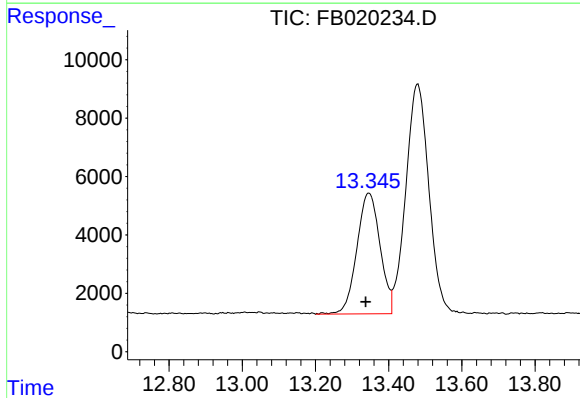


#7 Ethylbenzene

R.T.: 13.346 min
Delta R.T.: 0.008 min
Response: 181560
Conc: 7.72 ng/ml

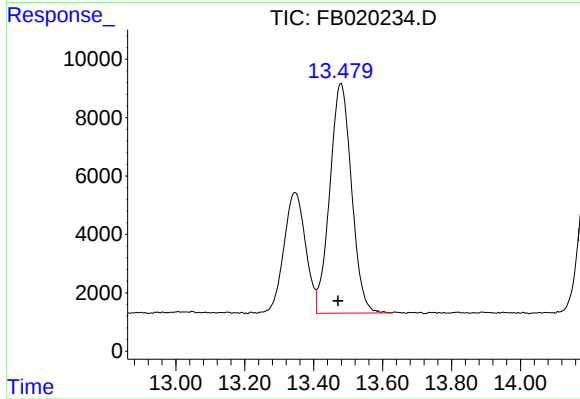

#8 m-Xylene


R.T.: 13.479 min
Delta R.T.: 0.008 min
Response: 344389
Conc: 16.14 ng/ml

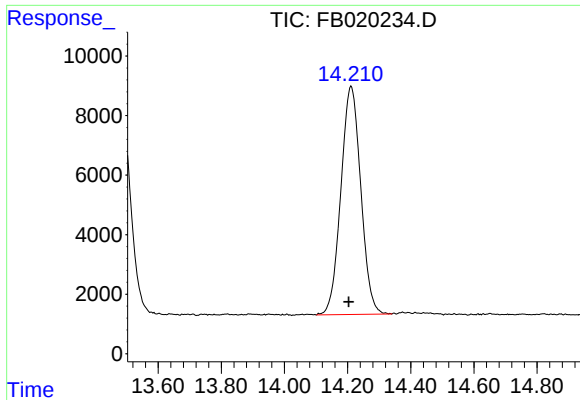

#9 O-Xylene

R.T.: 14.212 min
Delta R.T.: 0.008 min
Response: 335436
Conc: 17.71 ng/ml

Instrument :
FID_B
ClientSampleId :
TP-3-AMS

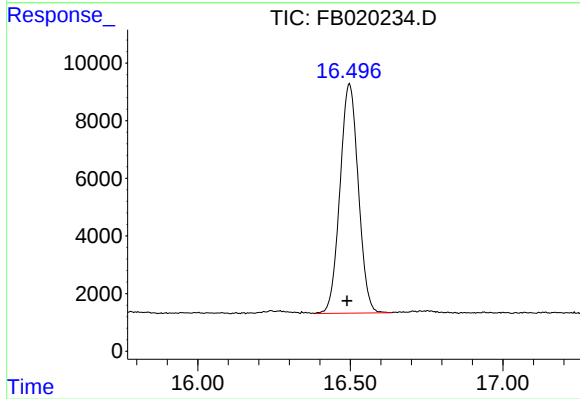

#10 1,2,4-Trimethylbenzene

R.T.: 16.497 min
Delta R.T.: 0.008 min
Response: 332461
Conc: 16.76 ng/ml