

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB031519\
 Data File : FB020235.D
 Signal(s) : FID2B.CH
 Acq On : 15 Mar 2019 15:00
 Operator : MJ/SJ
 Sample : K1930-02MSD
 Misc : 5.01g/5.00ml DI WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 TP-3-AMSD

Integration File: Calibration.e
 Quant Time: Mar 15 15:34:00 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB031119.M
 Quant Title :
 QLast Update : Mon Mar 11 13:44:46 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.045	427104	16.269 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.903	766226	22.714 ng/ml
2) t 2,2,4-Trimethylpentane	7.669	644131	19.642 ng/ml
3) t n-Heptane	8.000	277665	6.672 ng/ml
4) t Benzene	8.139	378287	8.125 ng/ml
6) t Toluene	10.893	843428	22.824 ng/ml
7) t Ethylbenzene	13.346	176629	7.507 ng/ml
8) t m-Xylene	13.480	337654	15.829 ng/ml
9) t O-Xylene	14.211	332189	17.536 ng/ml
10) t 1,2,4-Trimethylbenzene	16.497	328738	16.576 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB031519\
Data File : FB020235.D
Signal(s) : FID2B.CH
Acq On : 15 Mar 2019 15:00
Operator : MJ/SJ
Sample : K1930-02MSD
Misc : 5.01g/5.00ml DI WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
TP-3-AMSD

Integration File: Calibration.e
Quant Time: Mar 15 15:34:00 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB031119.M
Quant Title :
QLast Update : Mon Mar 11 13:44:46 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

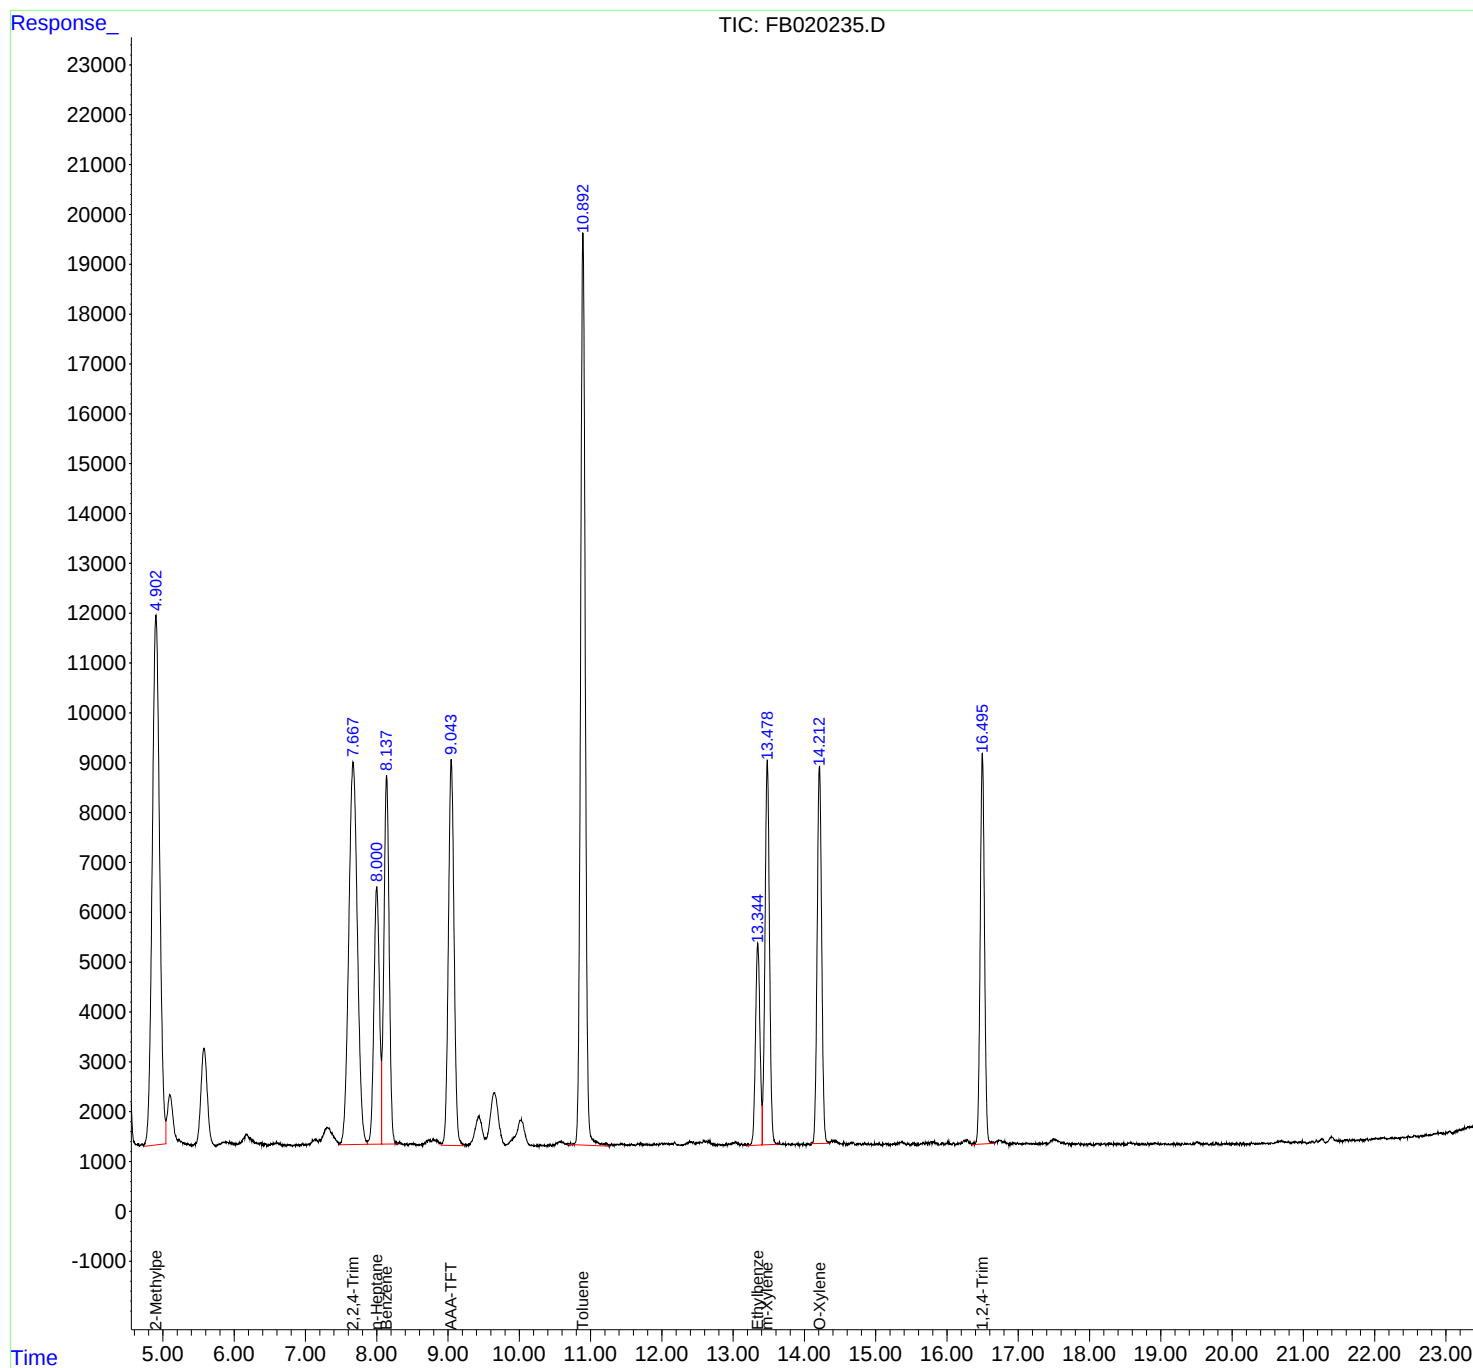


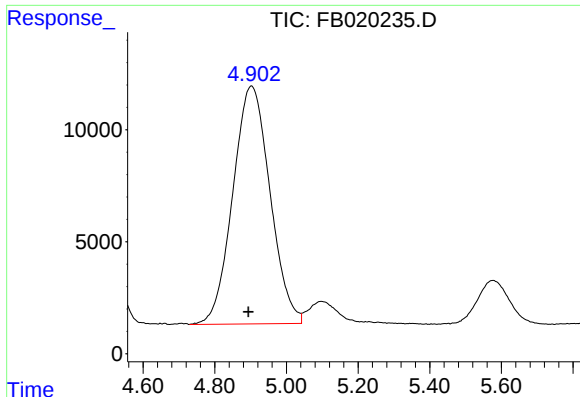

#1 2-Methylpentane


R.T.: 4.903 min
Delta R.T.: 0.009 min
Response: 766226
Conc: 22.71 ng/ml

Instrument :
FID_B
ClientSampleId :
TP-3-AMSD

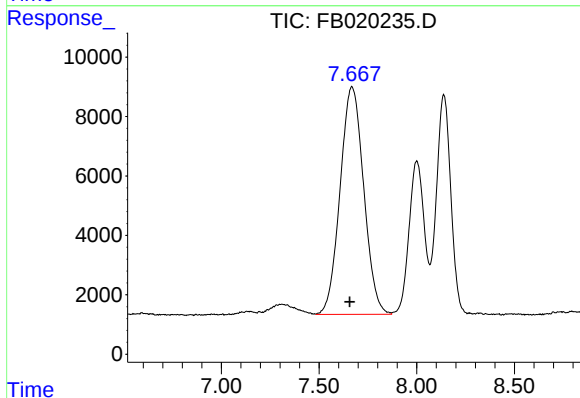


#2 2,2,4-Trimethylpentane

R.T.: 7.669 min
Delta R.T.: 0.011 min
Response: 644131
Conc: 19.64 ng/ml

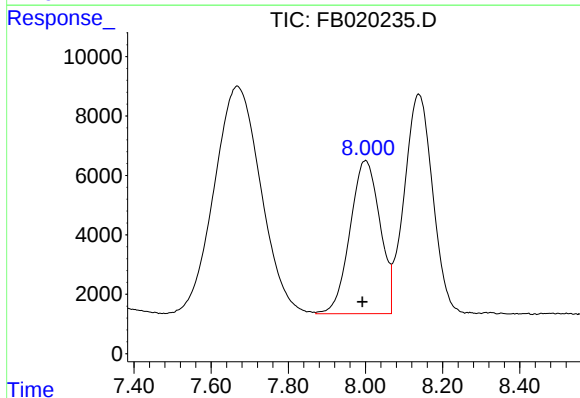


#3 n-Heptane

R.T.: 8.000 min
Delta R.T.: 0.008 min
Response: 277665
Conc: 6.67 ng/ml

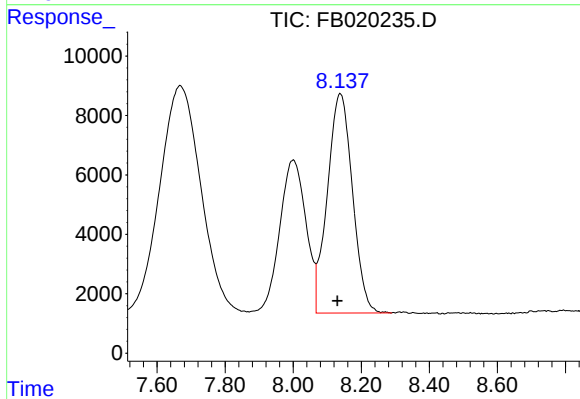

#4 Benzene


R.T.: 8.139 min
Delta R.T.: 0.009 min
Response: 378287
Conc: 8.13 ng/ml

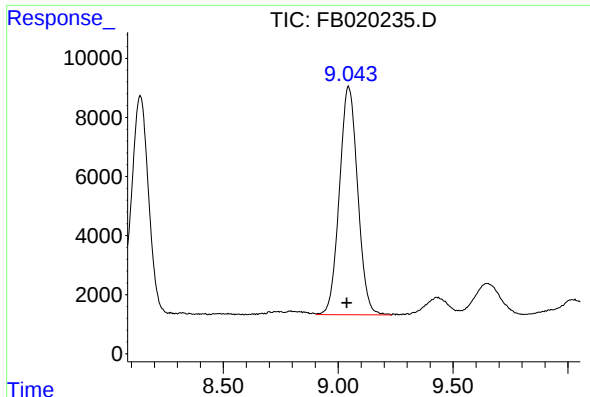

#5 AAA-TFT


R.T.: 9.045 min
Delta R.T.: 0.007 min
Response: 427104
Conc: 16.27 ng/ml

Instrument :
FID_B
ClientSampleId :
TP-3-AMSD

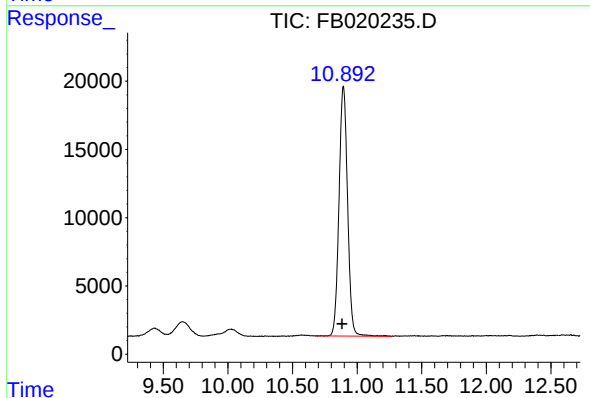


#6 Toluene

R.T.: 10.893 min
Delta R.T.: 0.008 min
Response: 843428
Conc: 22.82 ng/ml

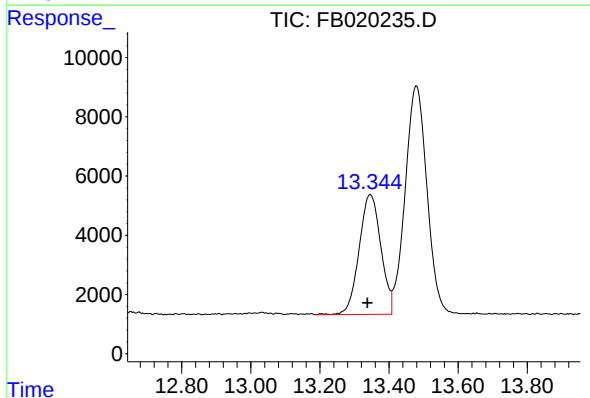


#7 Ethylbenzene

R.T.: 13.346 min
Delta R.T.: 0.008 min
Response: 176629
Conc: 7.51 ng/ml

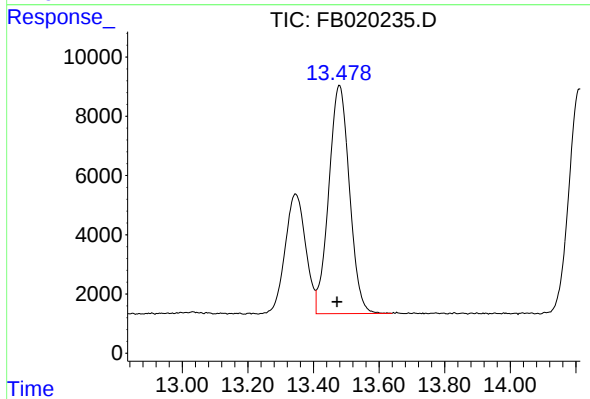

#8 m-Xylene


R.T.: 13.480 min
Delta R.T.: 0.008 min
Response: 337654
Conc: 15.83 ng/ml

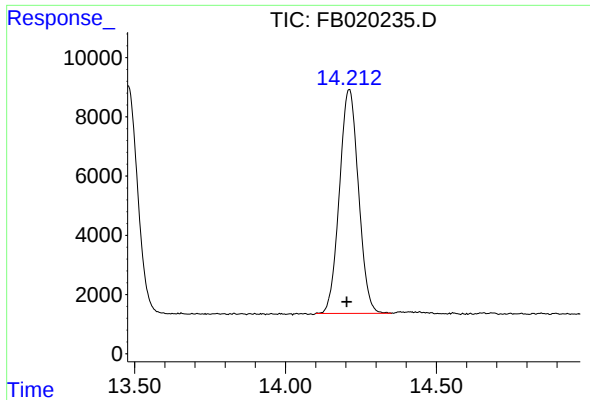

#9 O-Xylene

R.T.: 14.211 min
Delta R.T.: 0.008 min
Response: 332189
Conc: 17.54 ng/ml

Instrument :
FID_B
ClientSampleId :
TP-3-AMSD

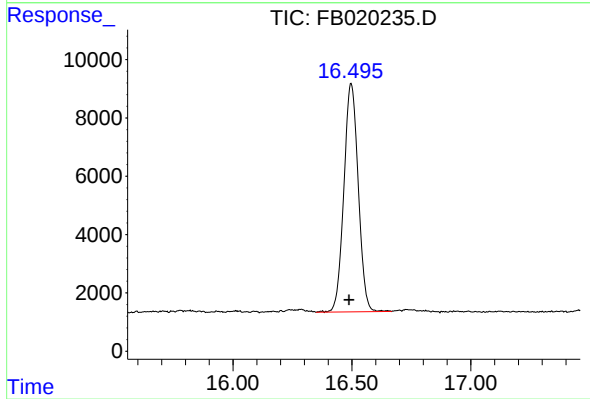

#10 1,2,4-Trimethylbenzene

R.T.: 16.497 min
Delta R.T.: 0.008 min
Response: 328738
Conc: 16.58 ng/ml