

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB031519\
Data File : FB020237.D
Signal(s) : FID2B.CH
Acq On : 15 Mar 2019 16:01
Operator : MJ/SJ
Sample : K1930-11
Misc : 5.06g/5.00ml DI WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
TP-5-A

Integration File: Calibration.e
Quant Time: Mar 16 00:26:20 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB031119.M
Quant Title :
QLast Update : Mon Mar 11 13:44:46 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.046	477872	18.203 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.884	4549	0.135 ng/ml
2) t 2,2,4-Trimethylpentane	7.671	48730	1.486 ng/ml
3) t n-Heptane	8.005	7638	0.184 ng/ml
4) t Benzene	8.126	6127	0.132 ng/ml
6) t Toluene	10.902	17585	0.476 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB031519\
Data File : FB020237.D
Signal(s) : FID2B.CH
Acq On : 15 Mar 2019 16:01
Operator : MJ/SJ
Sample : K1930-11
Misc : 5.06g/5.00ml DI WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
TP-5-A

Integration File: Calibration.e
Quant Time: Mar 16 00:26:20 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB031119.M
Quant Title :
QLast Update : Mon Mar 11 13:44:46 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

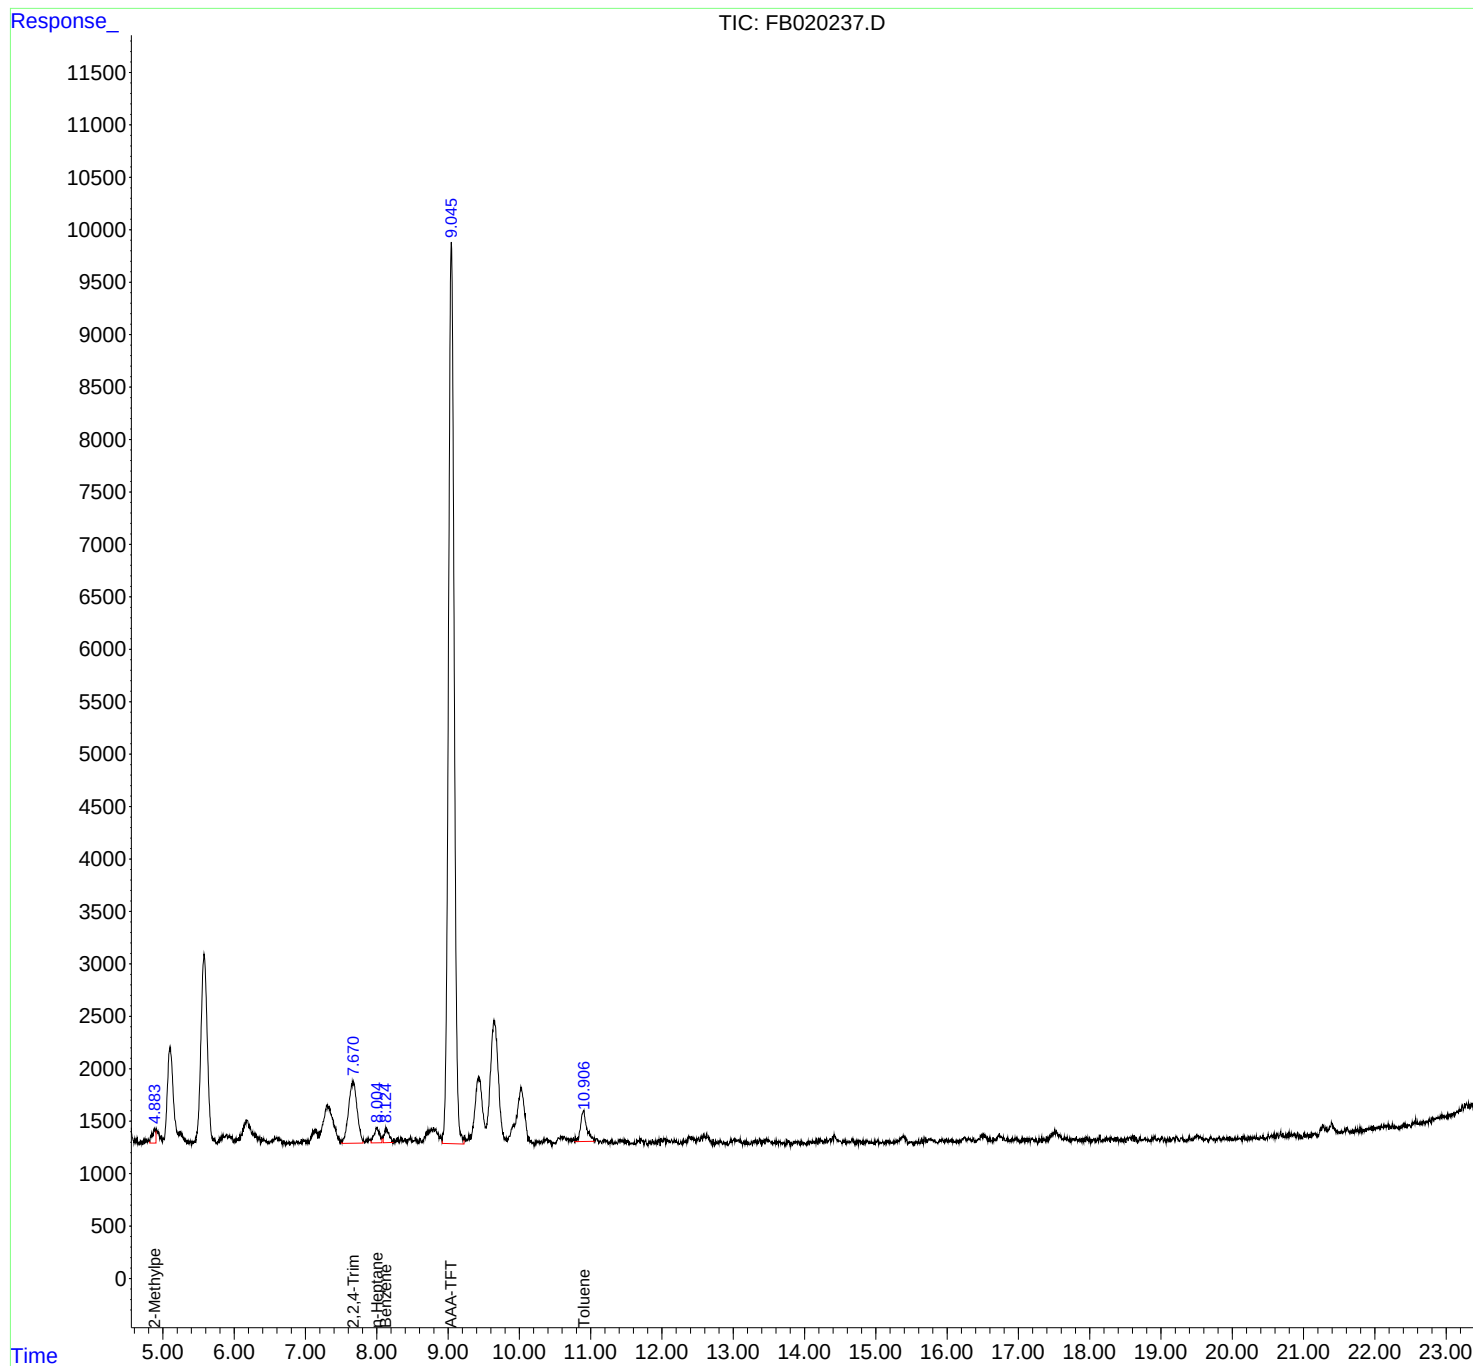


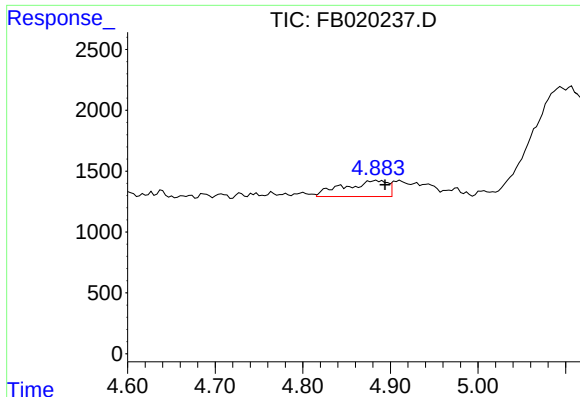

#1 2-Methylpentane


R.T.: 4.884 min
Delta R.T.: -0.010 min
Response: 4549
Conc: 0.13 ng/ml

Instrument :
FID_B
ClientSampleId :
TP-5-A

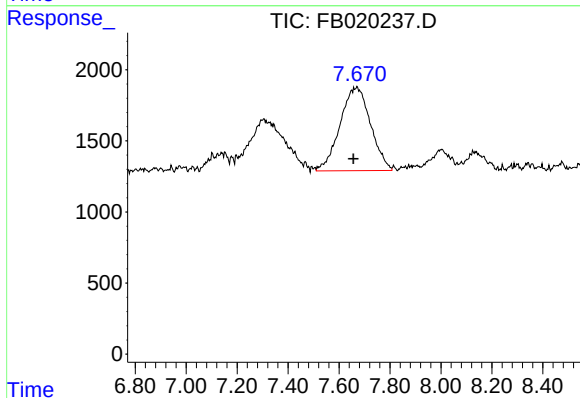


#2 2,2,4-Trimethylpentane

R.T.: 7.671 min
Delta R.T.: 0.014 min
Response: 48730
Conc: 1.49 ng/ml

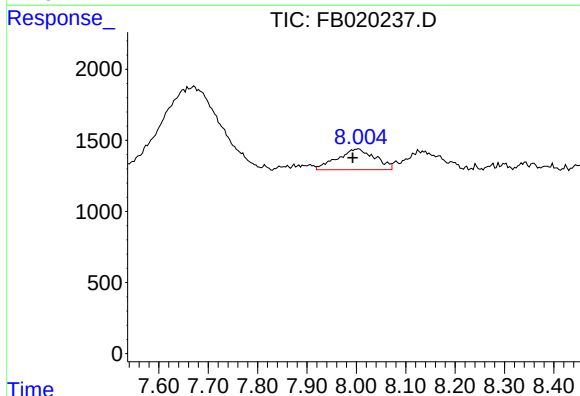


#3 n-Heptane

R.T.: 8.005 min
Delta R.T.: 0.012 min
Response: 7638
Conc: 0.18 ng/ml

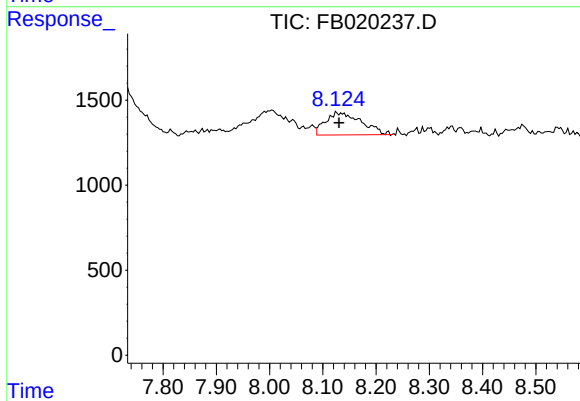

#4 Benzene


R.T.: 8.126 min
Delta R.T.: -0.004 min
Response: 6127
Conc: 0.13 ng/ml

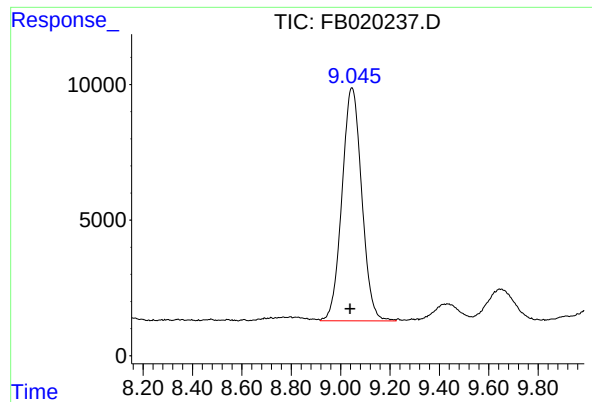

#5 AAA-TFT

R.T.: 9.046 min
Delta R.T.: 0.008 min
Response: 477872
Conc: 18.20 ng/ml

Instrument :
FID_B
ClientSampleId :
TP-5-A

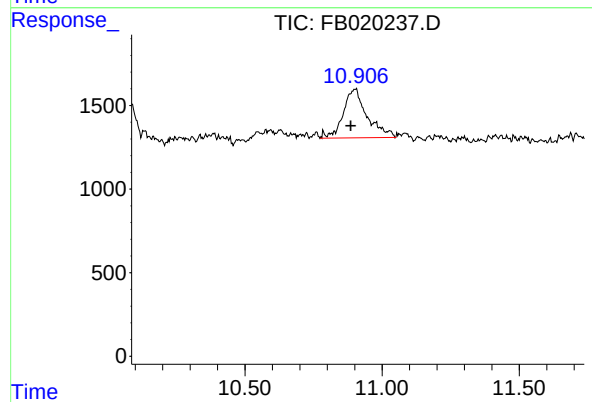

#6 Toluene

R.T.: 10.902 min
Delta R.T.: 0.017 min
Response: 17585
Conc: 0.48 ng/ml