

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB031522\
 Data File : FB026683.D
 Signal(s) : FID2B.CH
 Acq On : 15 Mar 2022 10:43
 Operator : AJ/MA
 Sample : BSF0315W1
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0315W1

Integration File: Calibration.e
 Quant Time: Mar 15 22:09:33 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030822.M
 Quant Title :
 QLast Update : Fri Mar 11 13:08:49 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.787	200637	19.120 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.707	532005	28.099 ng/ml
2) t 2,2,4-Trimethylpentane	7.430	575569	27.769 ng/ml
3) t n-Heptane	7.746	186320	9.413 ng/ml
4) t Benzene	7.883	217527	9.427 ng/ml
6) t Toluene	10.615	618095	28.233 ng/ml
7) t Ethylbenzene	13.052	188506	9.379 ng/ml
8) t m-Xylene	13.185	376797	18.697 ng/ml
9) t O-Xylene	13.912	370210	18.557 ng/ml
10) t 1,2,4-Trimethylbenzene	16.187	379732	19.059 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB031522\
Data File : FB026683.D
Signal(s) : FID2B.CH
Acq On : 15 Mar 2022 10:43
Operator : AJ/MA
Sample : BSF0315W1
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0315W1

Integration File: Calibration.e
Quant Time: Mar 15 22:09:33 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030822.M
Quant Title :
QLast Update : Fri Mar 11 13:08:49 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

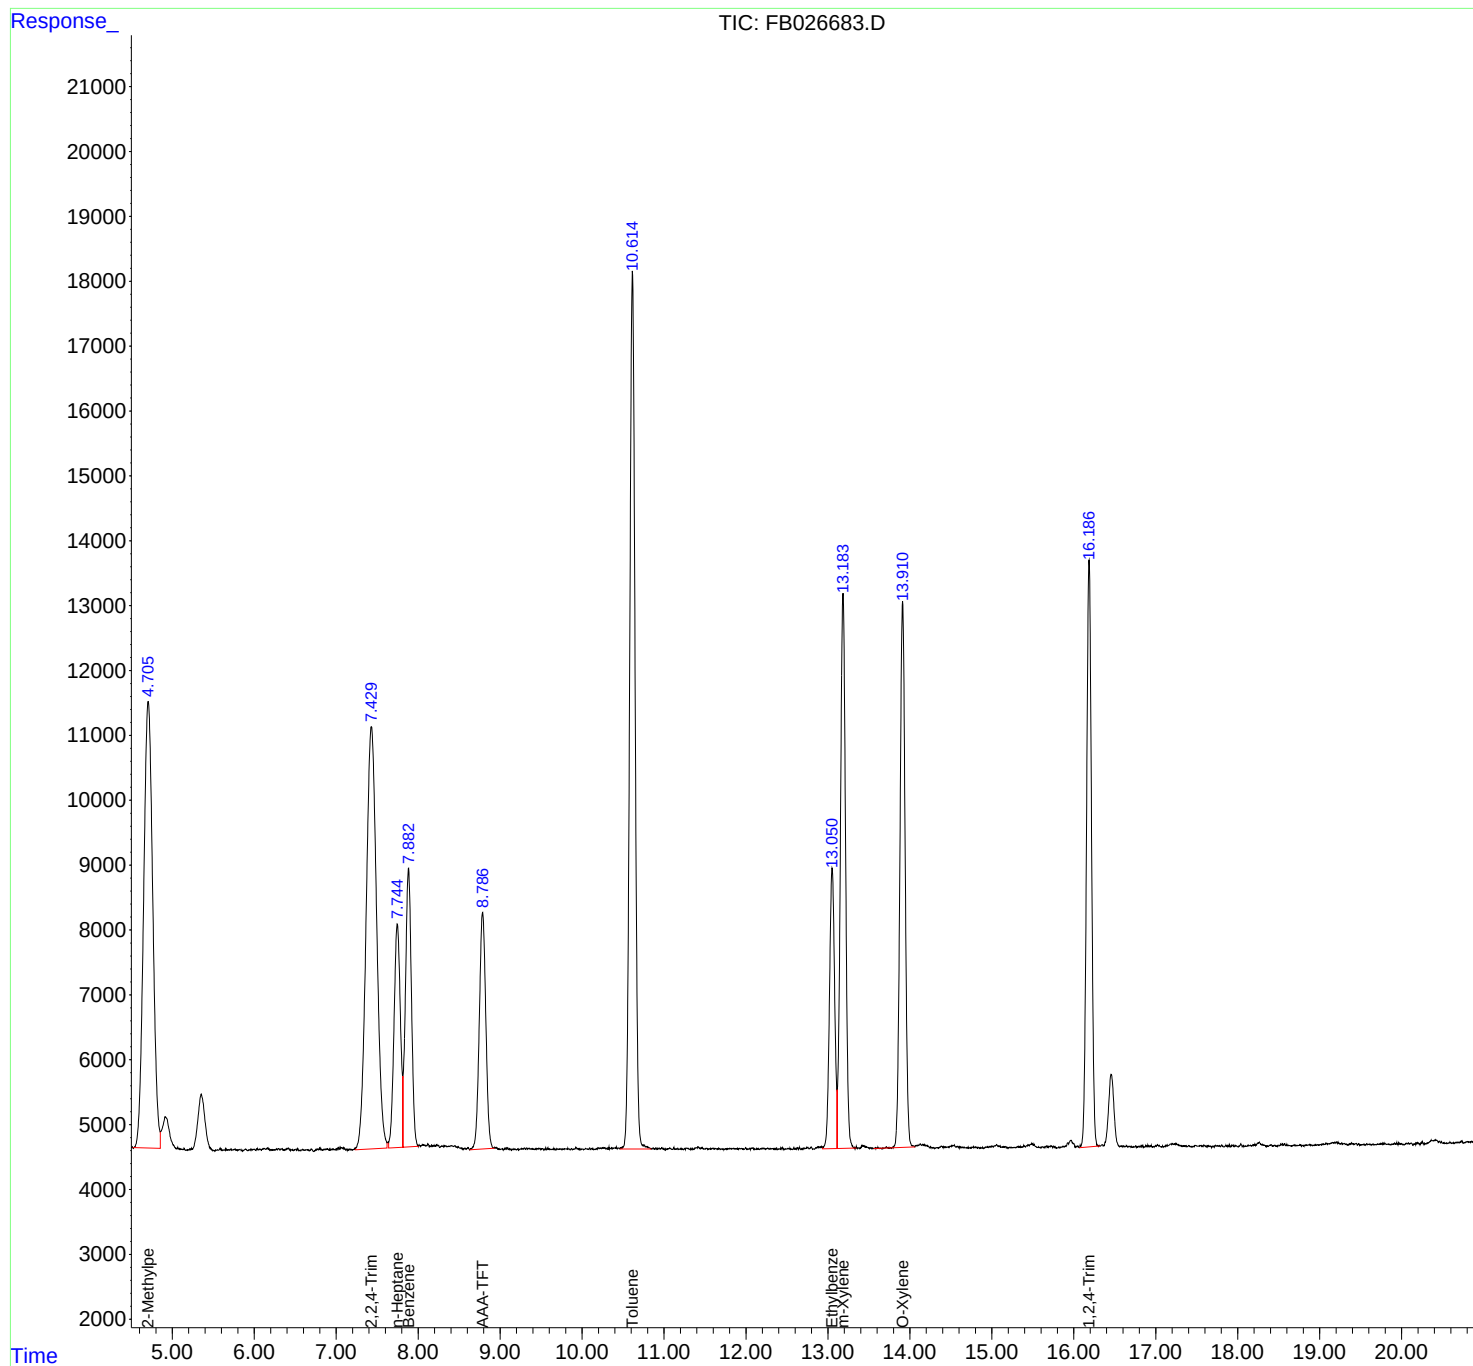


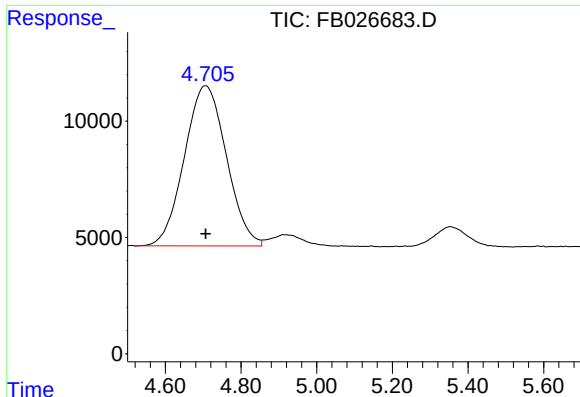

#1 2-Methylpentane


R.T.: 4.707 min
Delta R.T.: 0.000 min
Response: 532005
Conc: 28.10 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0315W1

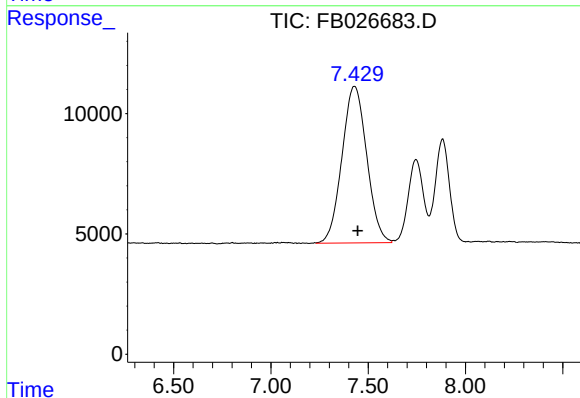


#2 2,2,4-Trimethylpentane

R.T.: 7.430 min
Delta R.T.: -0.017 min
Response: 575569
Conc: 27.77 ng/ml

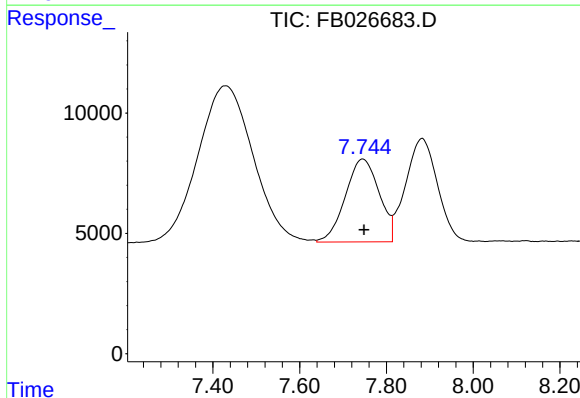


#3 n-Heptane

R.T.: 7.746 min
Delta R.T.: -0.003 min
Response: 186320
Conc: 9.41 ng/ml

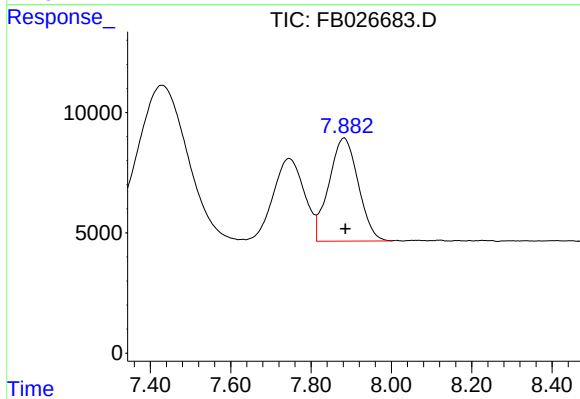

#4 Benzene


R.T.: 7.883 min
Delta R.T.: -0.003 min
Response: 217527
Conc: 9.43 ng/ml

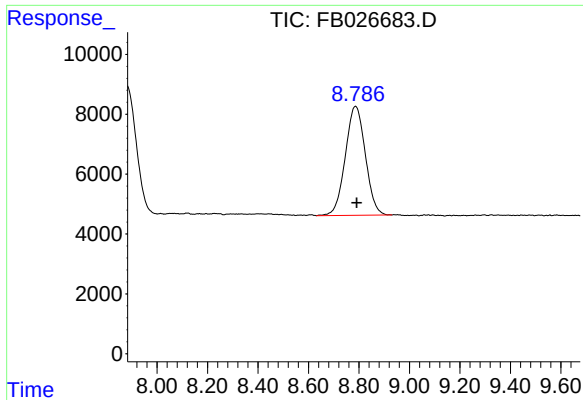

#5 AAA-TFT


R.T.: 8.787 min
Delta R.T.: -0.004 min
Response: 200637
Conc: 19.12 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0315W1

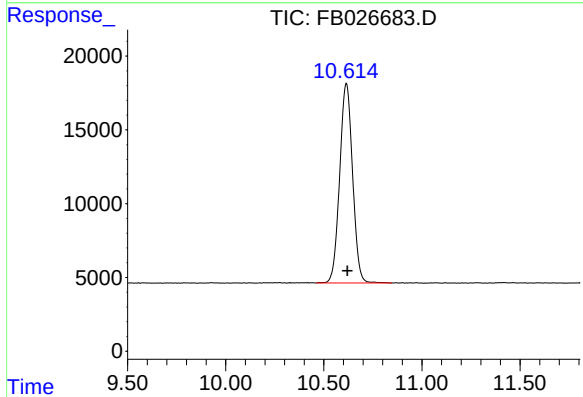


#6 Toluene

R.T.: 10.615 min
Delta R.T.: -0.006 min
Response: 618095
Conc: 28.23 ng/ml

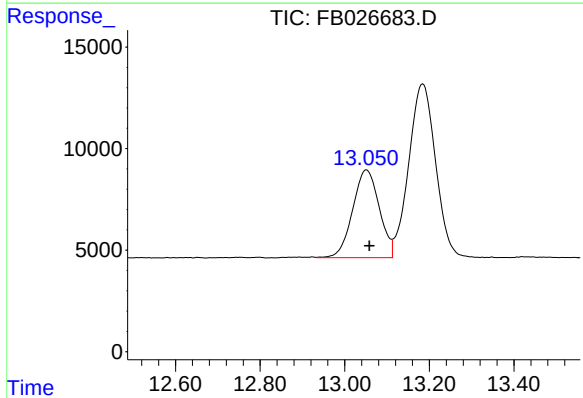


#7 Ethylbenzene

R.T.: 13.052 min
Delta R.T.: -0.007 min
Response: 188506
Conc: 9.38 ng/ml

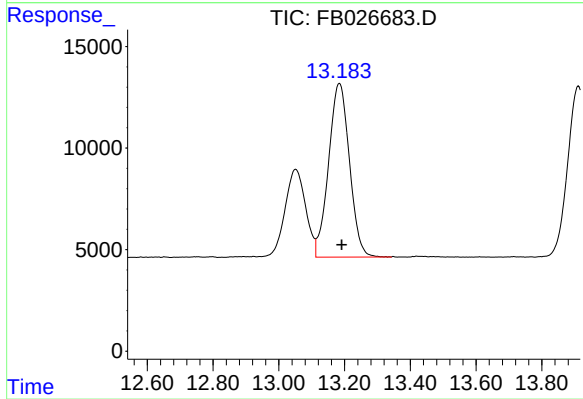

#8 m-Xylene


R.T.: 13.185 min
Delta R.T.: -0.007 min
Response: 376797
Conc: 18.70 ng/ml

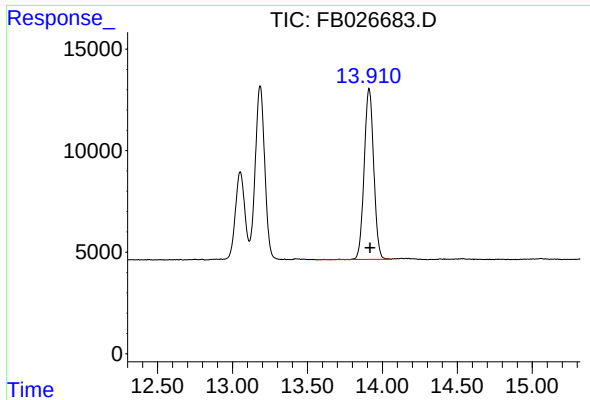

#9 O-Xylene

R.T.: 13.912 min
Delta R.T.: -0.007 min
Response: 370210
Conc: 18.56 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0315W1

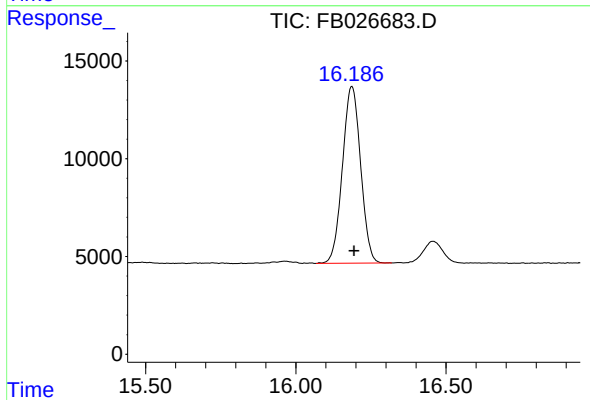

#10 1,2,4-Trimethylbenzene

R.T.: 16.187 min
Delta R.T.: -0.007 min
Response: 379732
Conc: 19.06 ng/ml