

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB031523\
 Data File : FB029489.D
 Signal(s) : FID2B.CH
 Acq On : 15 Mar 2023 8:25
 Operator : YP/AJ
 Sample : BSF0315W1
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Mar 16 02:26:46 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030123.M
 Quant Title :
 QLast Update : Wed Mar 01 12:30:24 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.792	264907	21.865 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.709	448614	29.237 ng/ml
2) t 2,2,4-Trimethylpentane	7.421	510968	30.334 ng/ml
3) t n-Heptane	7.750	172326	9.963 ng/ml
4) t Benzene	7.887	205943	10.146 ng/ml
6) t Toluene	10.621	606611	30.732 ng/ml
7) t Ethylbenzene	13.058	187286	10.060 ng/ml
8) t m-Xylene	13.191	372685	20.033 ng/ml
9) t O-Xylene	13.917	358352	19.462 ng/ml
10) t 1,2,4-Trimethylbenzene	16.193	354252	19.019 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB031523\
Data File : FB029489.D
Signal(s) : FID2B.CH
Acq On : 15 Mar 2023 8:25
Operator : YP/AJ
Sample : BSF0315W1
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Mar 16 02:26:46 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030123.M
Quant Title :
QLast Update : Wed Mar 01 12:30:24 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

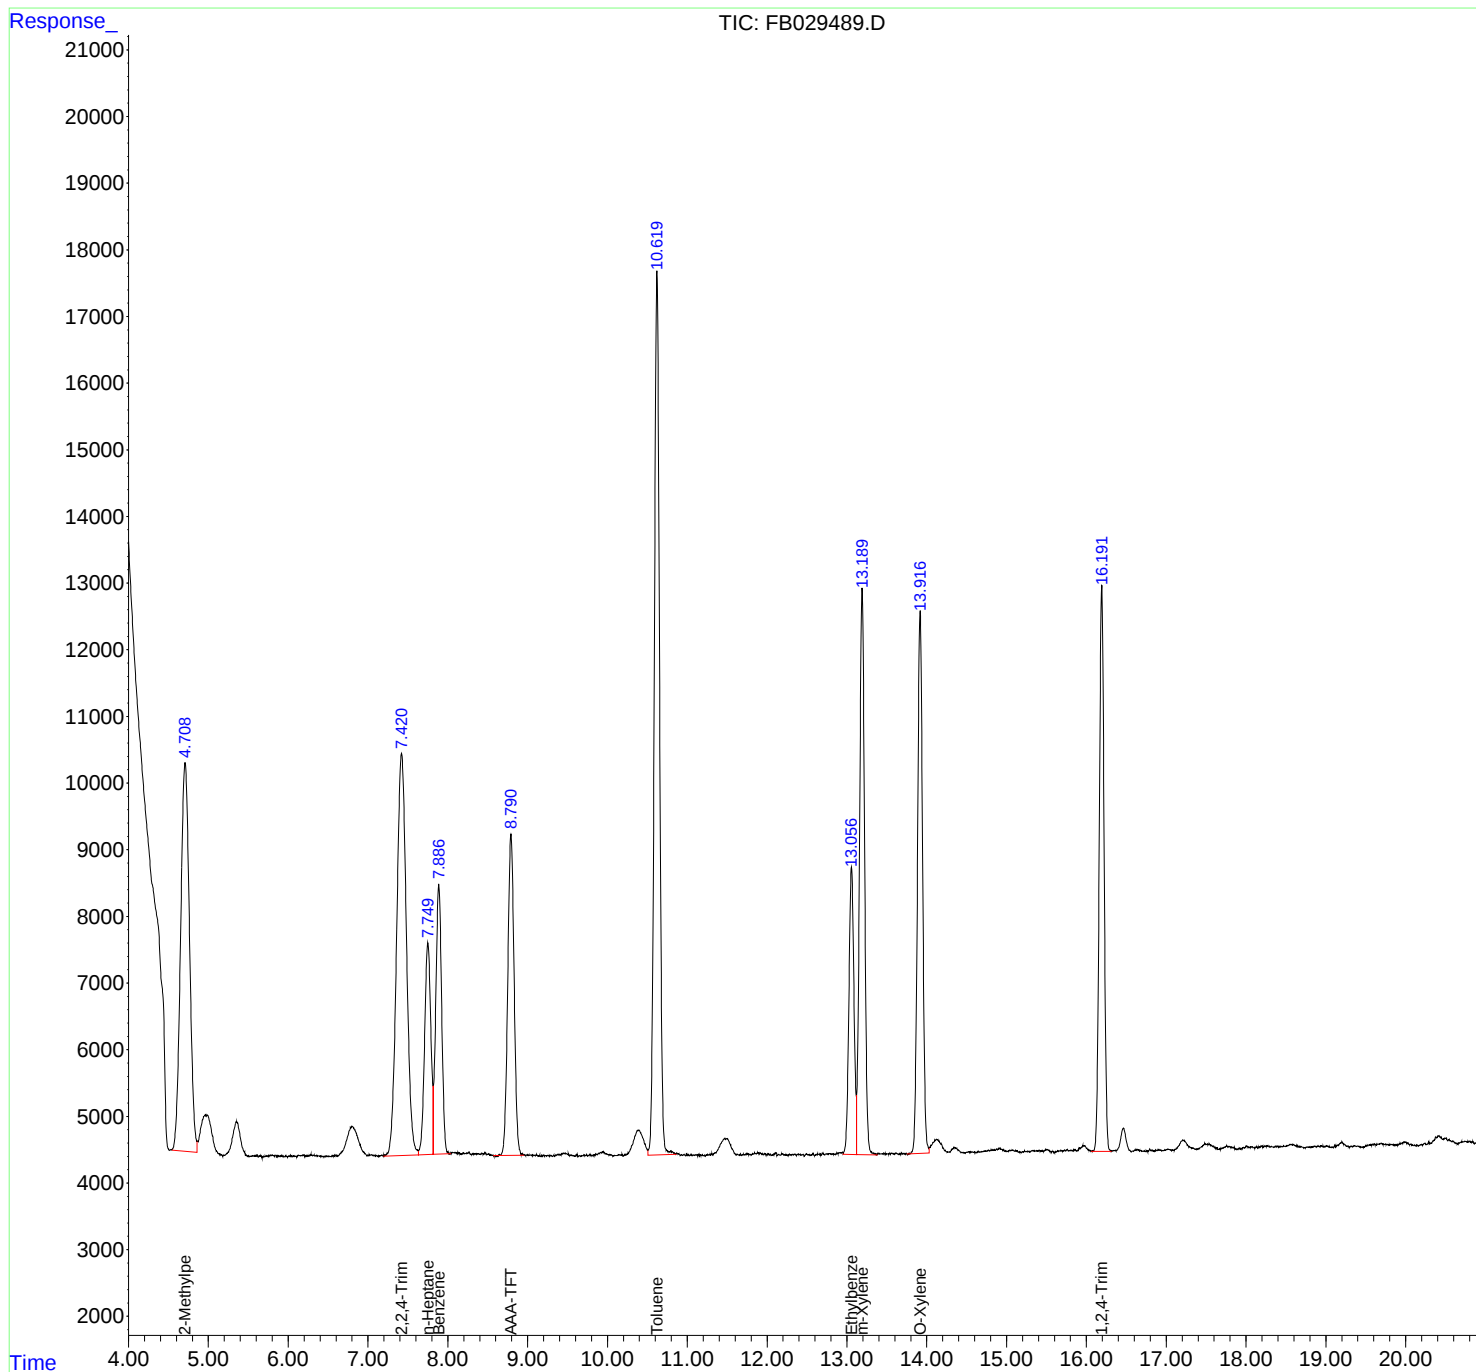


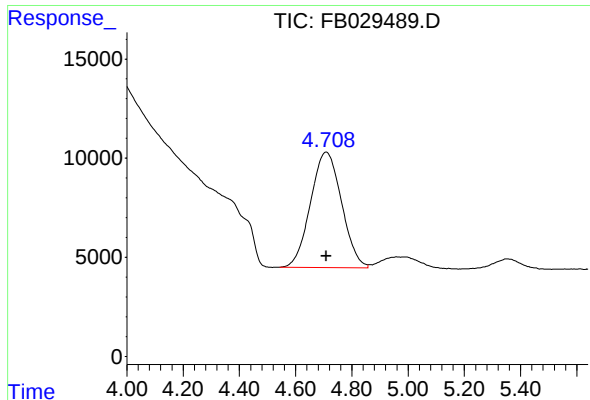

#1 2-Methylpentane


R.T.: 4.709 min
Delta R.T.: 0.000 min
Response: 448614
Conc: 29.24 ng/ml

Instrument :
FID_B
ClientSampleId :

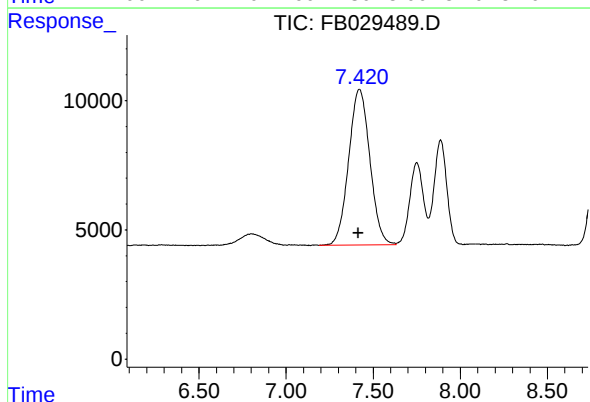


#2 2,2,4-Trimethylpentane

R.T.: 7.421 min
Delta R.T.: 0.005 min
Response: 510968
Conc: 30.33 ng/ml

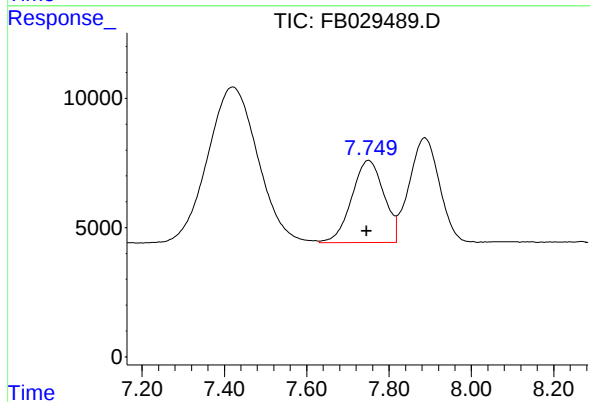


#3 n-Heptane

R.T.: 7.750 min
Delta R.T.: 0.005 min
Response: 172326
Conc: 9.96 ng/ml

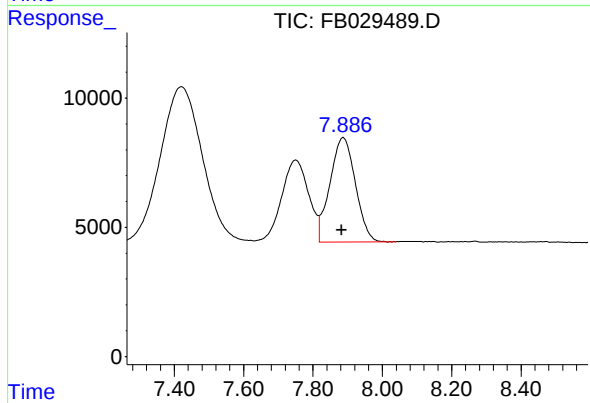

#4 Benzene


R.T.: 7.887 min
Delta R.T.: 0.004 min
Response: 205943
Conc: 10.15 ng/ml

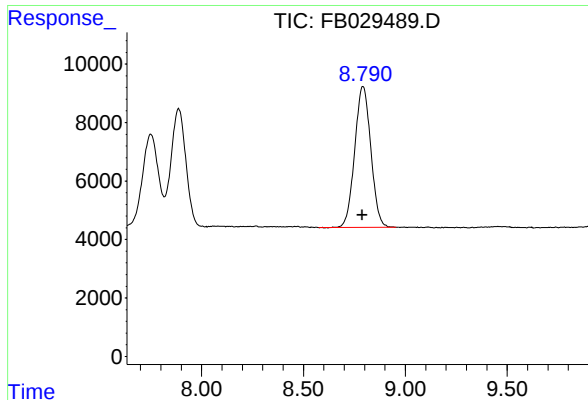

#5 AAA-TFT


R.T.: 8.792 min
Delta R.T.: 0.004 min
Response: 264907
Conc: 21.86 ng/ml

Instrument : FID_B
ClientSampleId :

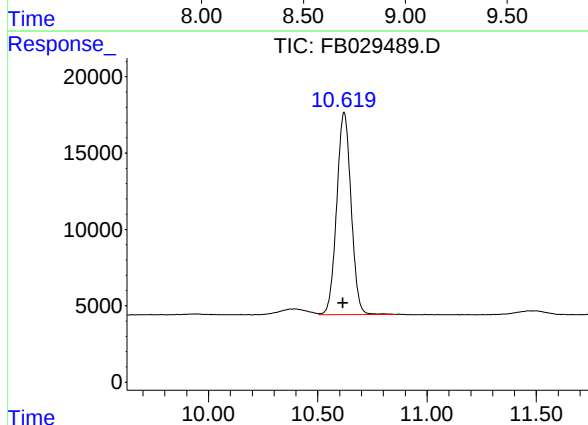


#6 Toluene

R.T.: 10.621 min
Delta R.T.: 0.005 min
Response: 606611
Conc: 30.73 ng/ml

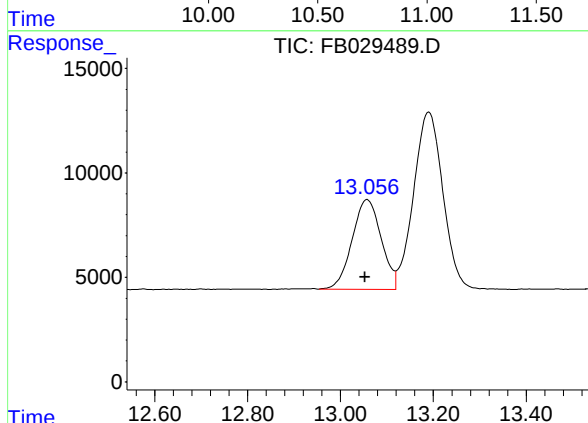


#7 Ethylbenzene

R.T.: 13.058 min
Delta R.T.: 0.005 min
Response: 187286
Conc: 10.06 ng/ml

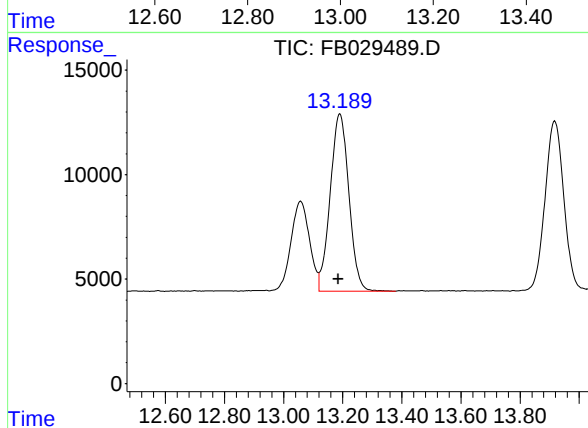

#8 m-Xylene


R.T.: 13.191 min
Delta R.T.: 0.006 min
Response: 372685
Conc: 20.03 ng/ml

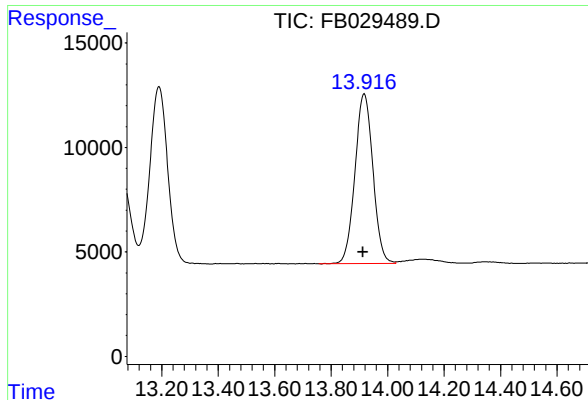

#9 O-Xylene

R.T.: 13.917 min
Delta R.T.: 0.005 min
Response: 358352
Conc: 19.46 ng/ml

Instrument :
FID_B
ClientSampleId :

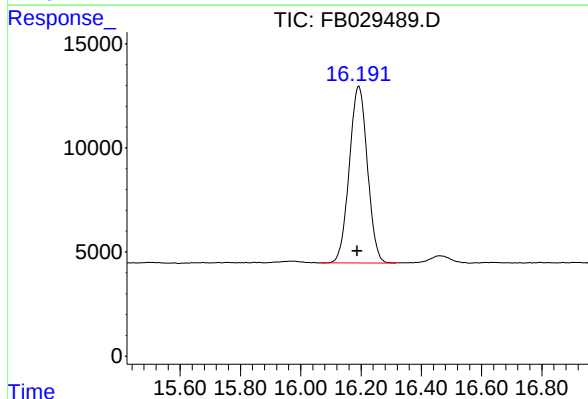

#10 1,2,4-Trimethylbenzene

R.T.: 16.193 min
Delta R.T.: 0.006 min
Response: 354252
Conc: 19.02 ng/ml