

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB031523\
 Data File : FB029490.D
 Signal(s) : FID2B.CH
 Acq On : 15 Mar 2023 9:03
 Operator : YP/AJ
 Sample : BSF0315W2
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0315W2

Integration File: Calibration.e
 Quant Time: Mar 16 02:26:52 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030123.M
 Quant Title :
 QLast Update : Wed Mar 01 12:30:24 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.794	234223	19.332 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.711	438879	28.602 ng/ml
2) t 2,2,4-Trimethylpentane	7.421	526775	31.272 ng/ml
3) t n-Heptane	7.752	164221	9.495 ng/ml
4) t Benzene	7.889	200421	9.874 ng/ml
6) t Toluene	10.622	587783	29.778 ng/ml
7) t Ethylbenzene	13.059	187044	10.047 ng/ml
8) t m-Xylene	13.191	370825	19.933 ng/ml
9) t O-Xylene	13.918	363665	19.750 ng/ml
10) t 1,2,4-Trimethylbenzene	16.193	375230	20.146 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB031523\
Data File : FB029490.D
Signal(s) : FID2B.CH
Acq On : 15 Mar 2023 9:03
Operator : YP/AJ
Sample : BSF0315W2
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0315W2

Integration File: Calibration.e
Quant Time: Mar 16 02:26:52 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030123.M
Quant Title :
QLast Update : Wed Mar 01 12:30:24 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

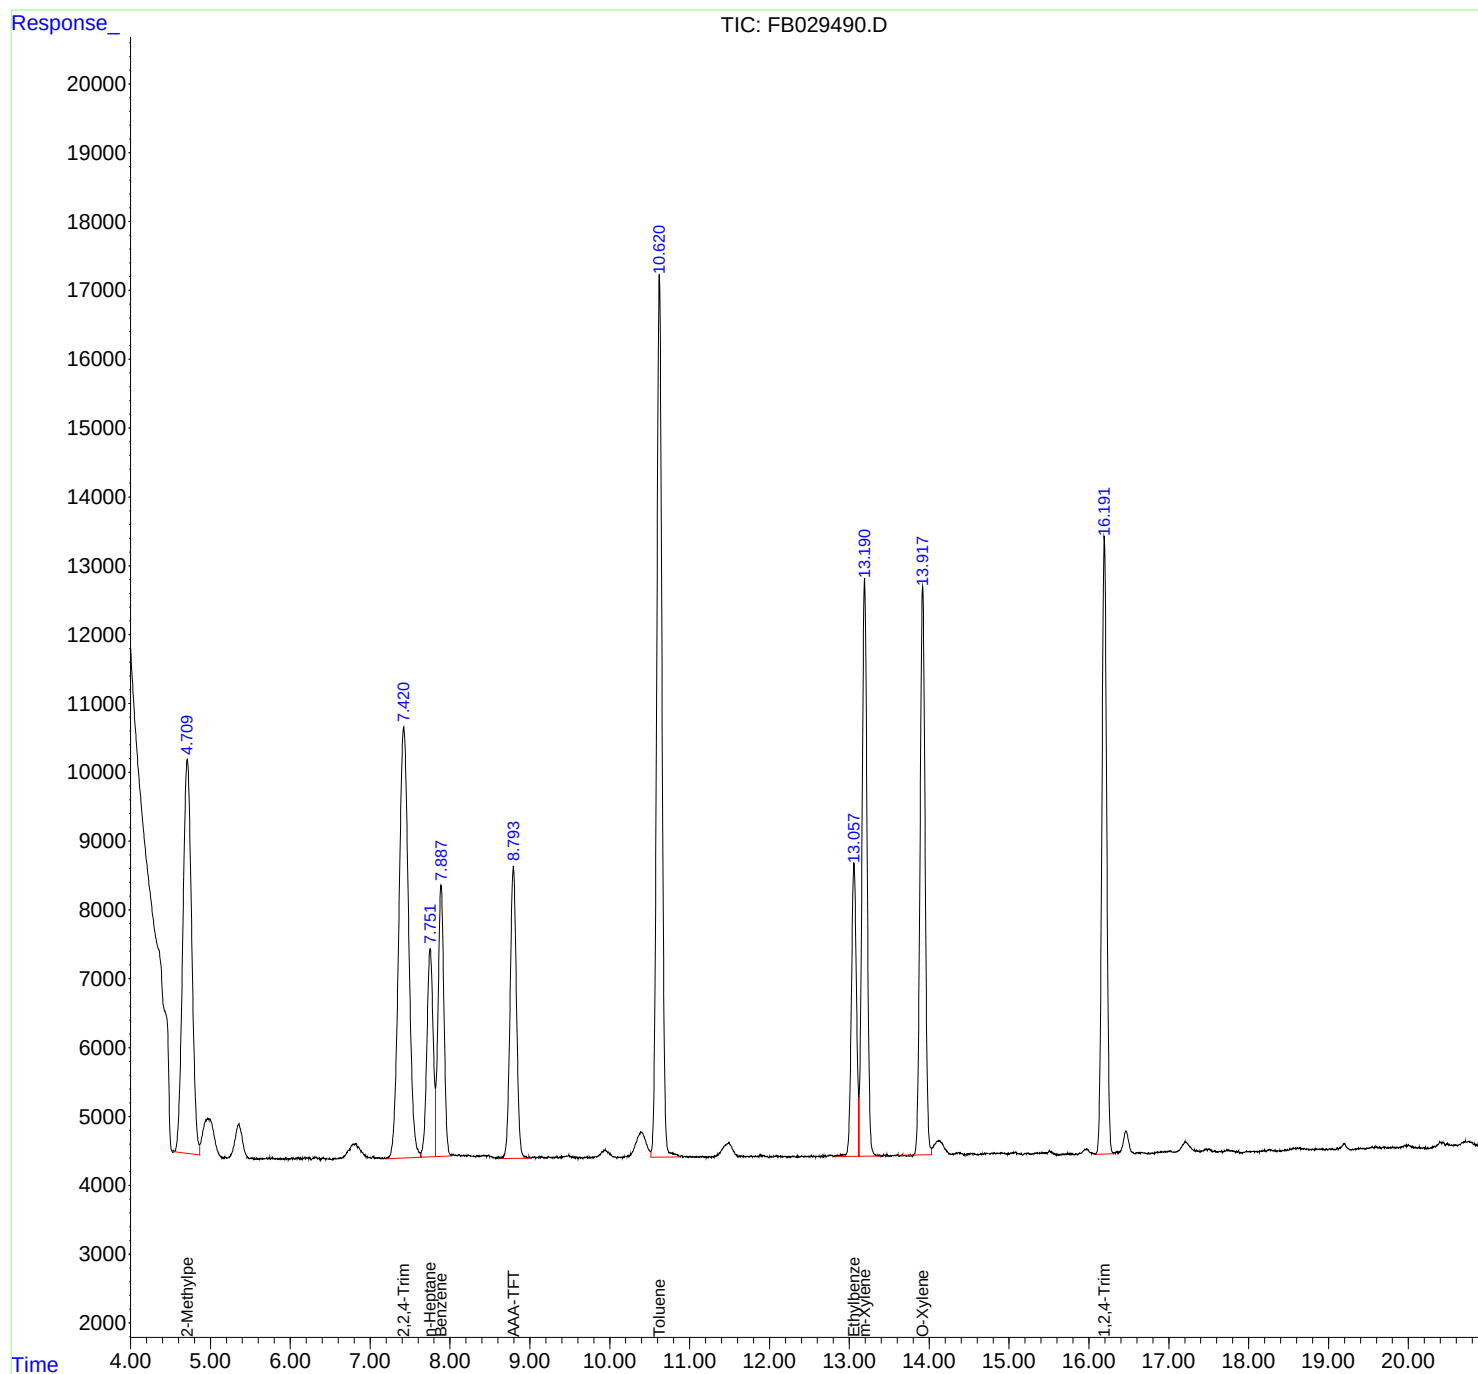


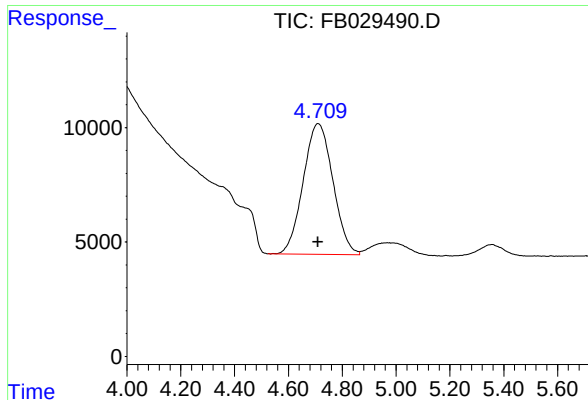

#1 2-Methylpentane


R.T.: 4.711 min
Delta R.T.: 0.000 min
Response: 438879
Conc: 28.60 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0315W2

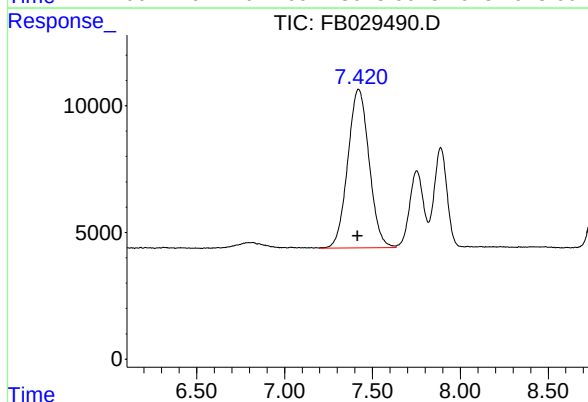


#2 2,2,4-Trimethylpentane

R.T.: 7.421 min
Delta R.T.: 0.006 min
Response: 526775
Conc: 31.27 ng/ml

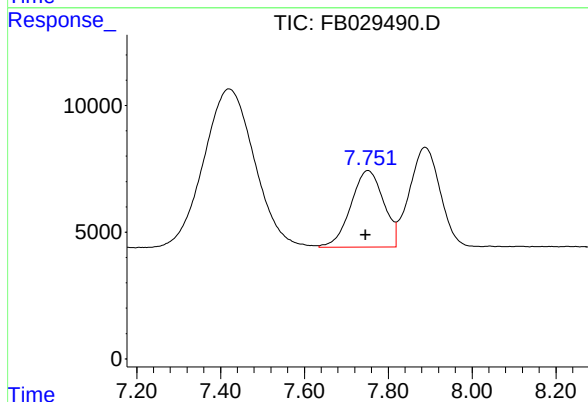


#3 n-Heptane

R.T.: 7.752 min
Delta R.T.: 0.007 min
Response: 164221
Conc: 9.49 ng/ml

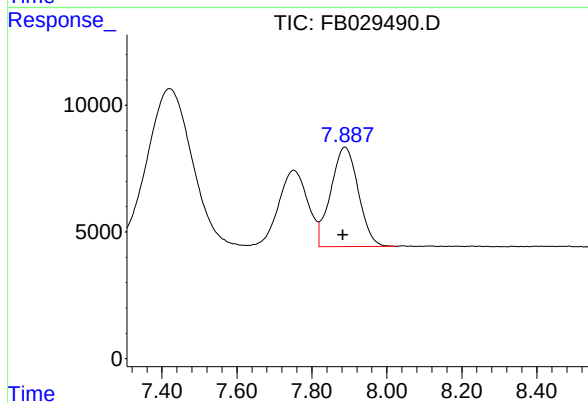

#4 Benzene


R.T.: 7.889 min
Delta R.T.: 0.005 min
Response: 200421
Conc: 9.87 ng/ml

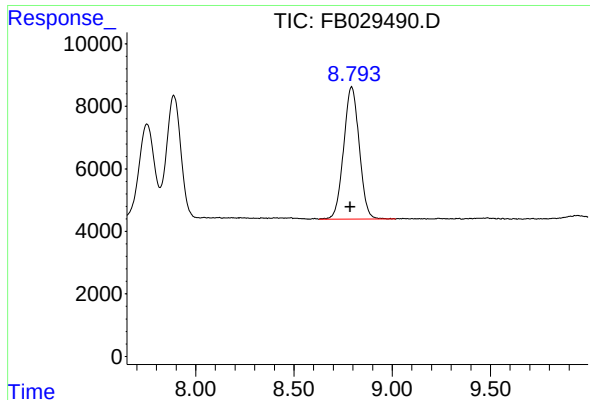

#5 AAA-TFT


R.T.: 8.794 min
Delta R.T.: 0.006 min
Response: 234223
Conc: 19.33 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0315W2

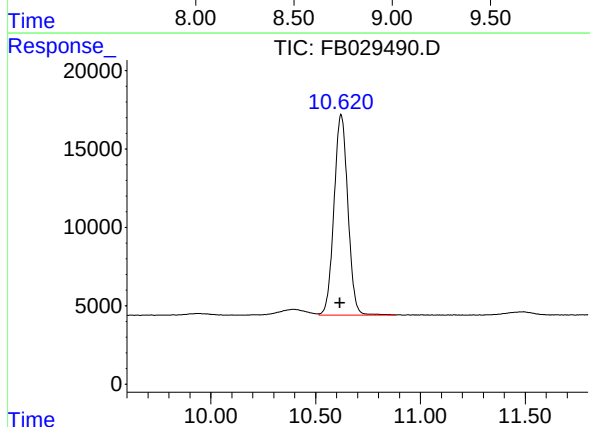


#6 Toluene

R.T.: 10.622 min
Delta R.T.: 0.006 min
Response: 587783
Conc: 29.78 ng/ml

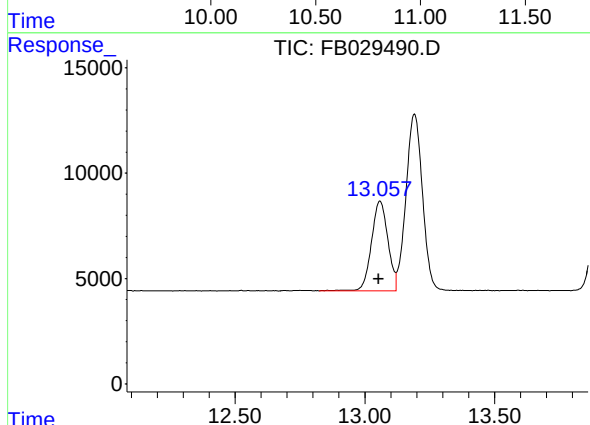


#7 Ethylbenzene

R.T.: 13.059 min
Delta R.T.: 0.006 min
Response: 187044
Conc: 10.05 ng/ml

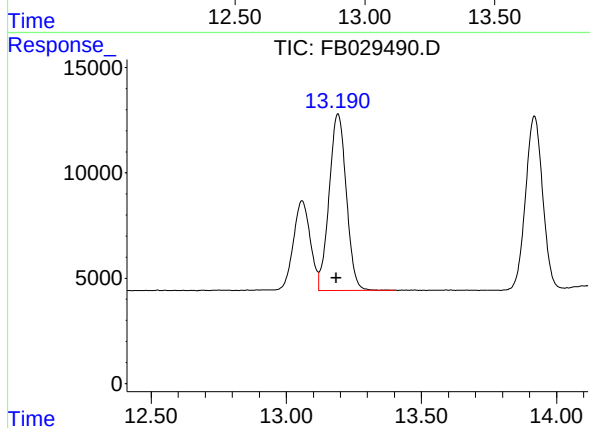

#8 m-Xylene


R.T.: 13.191 min
Delta R.T.: 0.007 min
Response: 370825
Conc: 19.93 ng/ml

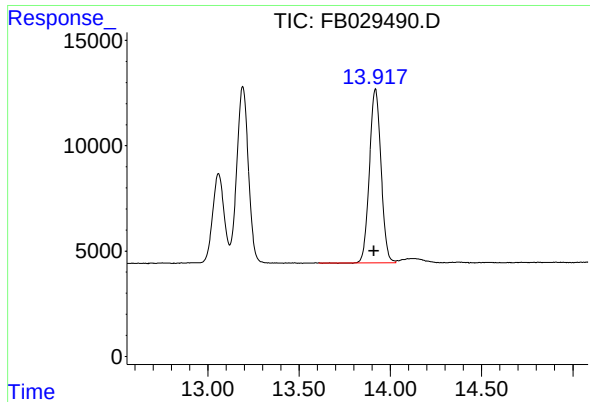

#9 O-Xylene

R.T.: 13.918 min
Delta R.T.: 0.006 min
Response: 363665
Conc: 19.75 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0315W2

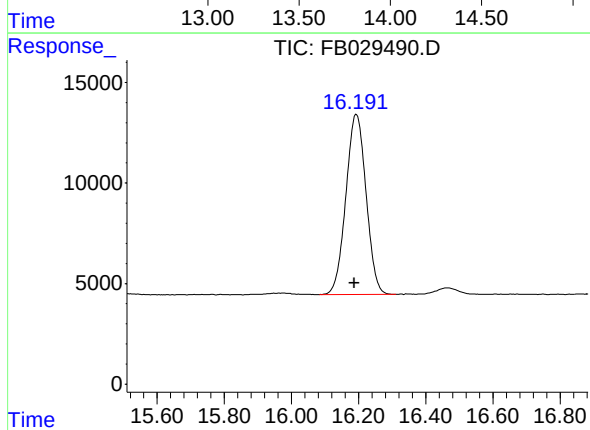

#10 1,2,4-Trimethylbenzene

R.T.: 16.193 min
Delta R.T.: 0.006 min
Response: 375230
Conc: 20.15 ng/ml