

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB031620\
 Data File : FB023959.D
 Signal(s) : FID2B.CH
 Acq On : 16 Mar 2020 11:23
 Operator : DD/AJ
 Sample : VBF0316S1
 Misc : 5.01g/5.00ml DI WATER
 ALS Vial : 2 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Mar 17 00:51:51 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030520.M
 Quant Title :
 QLast Update : Thu Mar 05 11:03:12 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	8.792	453886	21.562 ng/ml
Target Compounds				
1) t	2-Methylpentane	4.691	3306	0.107 ng/ml
2) t	2,2,4-Trimethylpentane	7.378	989	0.029 ng/ml
3) t	n-Heptane	7.756	1953	0.059 ng/ml
4) t	Benzene	7.869	438	0.010 ng/ml
6) t	Toluene	10.622	2512	0.062 ng/ml
7) t	Ethylbenzene	13.068	1530	0.040 ng/ml
8) t	m-Xylene	13.195	3052	0.083 ng/ml
9) t	O-Xylene	13.921	1445	0.041 ng/ml
10) t	1,2,4-Trimethylbenzene	16.204	6726	0.222 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB031620\
Data File : FB023959.D
Signal(s) : FID2B.CH
Acq On : 16 Mar 2020 11:23
Operator : DD/AJ
Sample : VBF0316S1
Misc : 5.01g/5.00ml DI WATER
ALS Vial : 2 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Mar 17 00:51:51 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030520.M
Quant Title :
QLast Update : Thu Mar 05 11:03:12 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

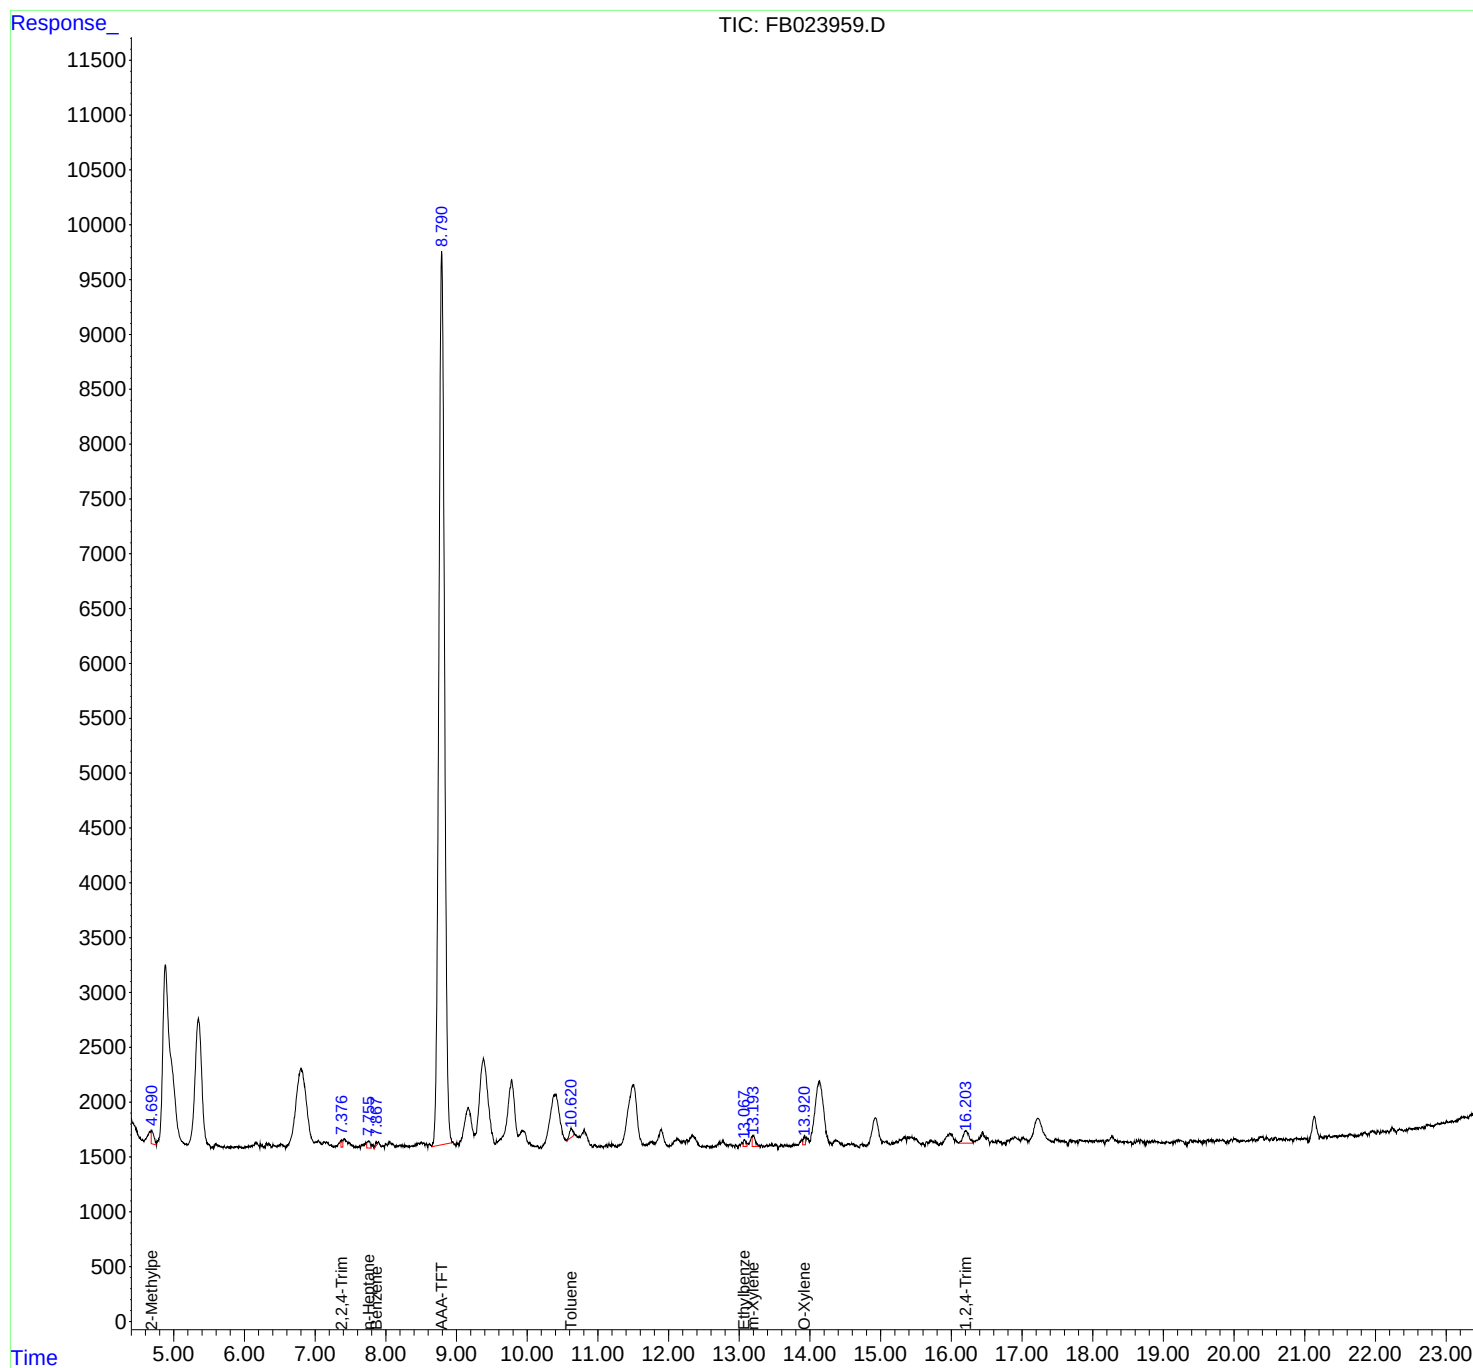

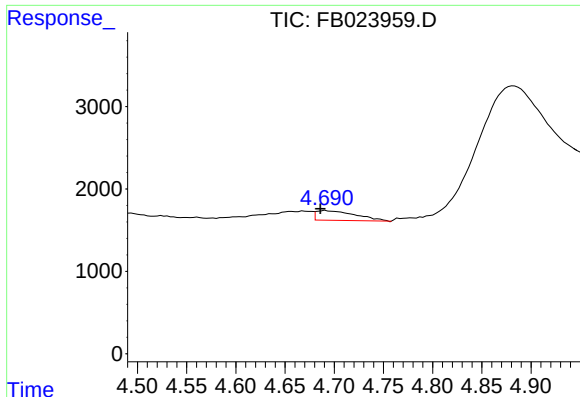


#1 2-Methylpentane

R.T.: 4.691 min
Delta R.T.: 0.005 min
Response: 3306
Conc: 0.11 ng/ml

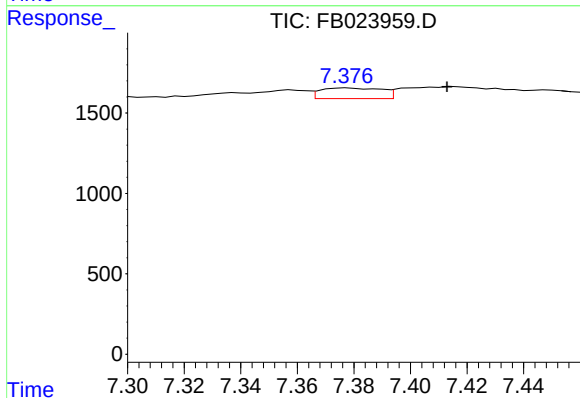


#2 2,2,4-Trimethylpentane

R.T.: 7.378 min
Delta R.T.: -0.035 min
Response: 989
Conc: 0.03 ng/ml

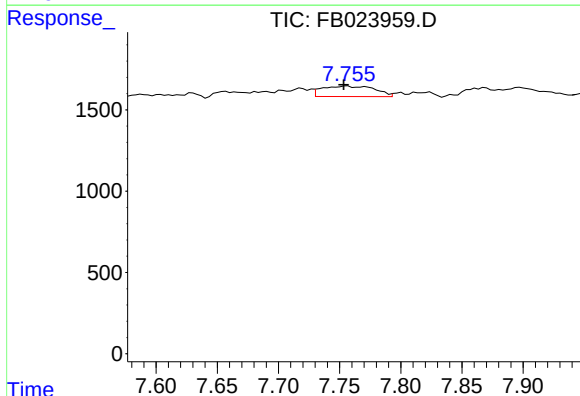


#3 n-Heptane

R.T.: 7.756 min
Delta R.T.: 0.003 min
Response: 1953
Conc: 0.06 ng/ml

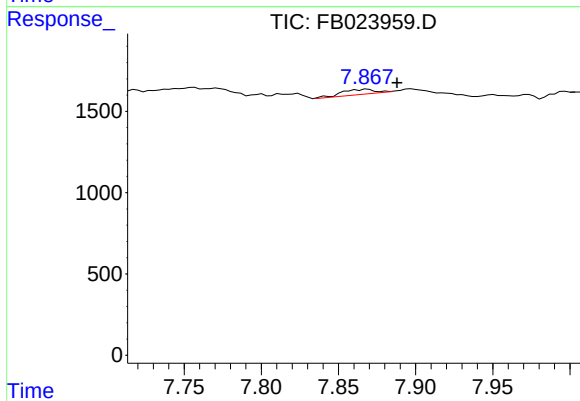


#4 Benzene

R.T.: 7.869 min
Delta R.T.: -0.019 min
Response: 438
Conc: 0.01 ng/ml

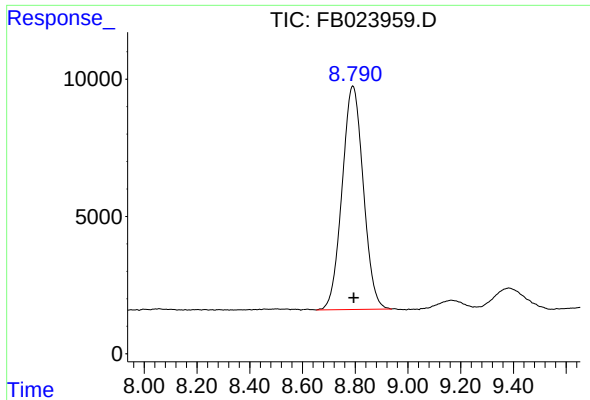


#5 AAA-TFT

R.T.: 8.792 min
Delta R.T.: -0.003 min
Response: 453886
Conc: 21.56 ng/ml

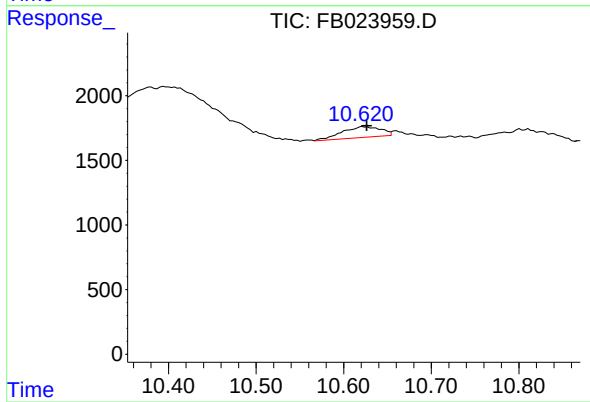


#6 Toluene

R.T.: 10.622 min
Delta R.T.: -0.005 min
Response: 2512
Conc: 0.06 ng/ml

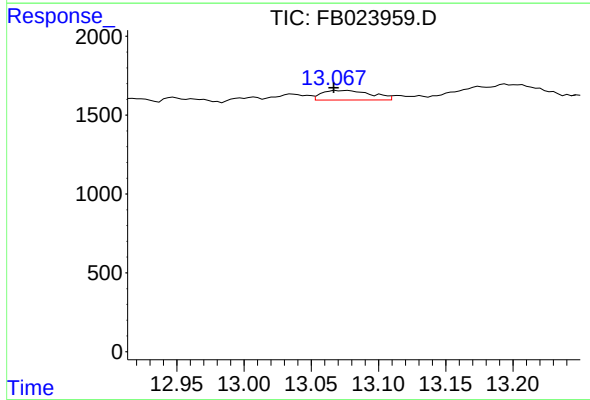


#7 Ethylbenzene

R.T.: 13.068 min
Delta R.T.: 0.002 min
Response: 1530
Conc: 0.04 ng/ml

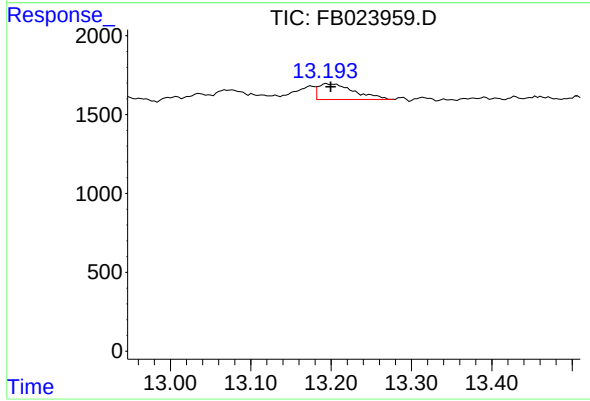


#8 m-Xylene

R.T.: 13.195 min
Delta R.T.: -0.005 min
Response: 3052
Conc: 0.08 ng/ml

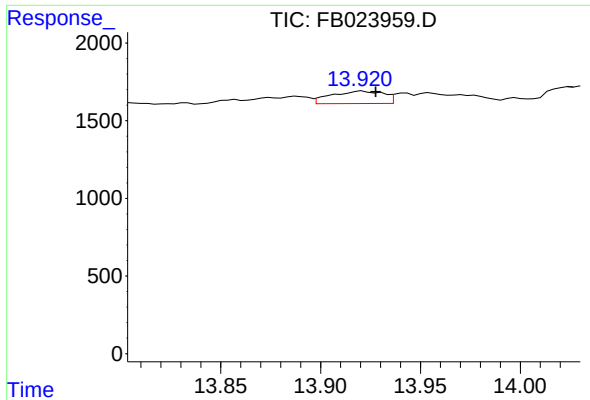

#9 O-Xylene

R.T.: 13.921 min
Delta R.T.: -0.006 min
Response: 1445
Conc: 0.04 ng/ml

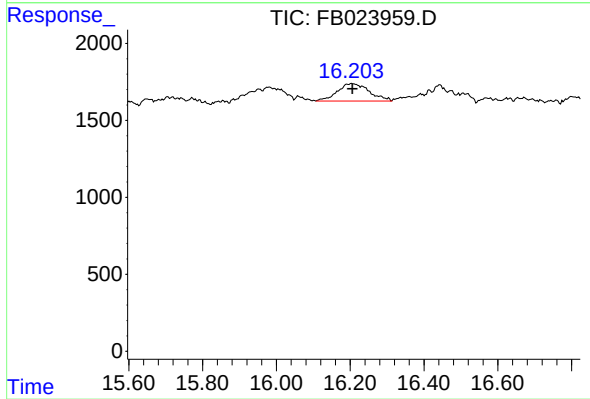

#10 1,2,4-Trimethylbenzene

R.T.: 16.204 min
Delta R.T.: -0.001 min
Response: 6726
Conc: 0.22 ng/ml