

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB031620\
 Data File : FB023960.D
 Signal(s) : FID2B.CH
 Acq On : 16 Mar 2020 11:53
 Operator : DD/AJ
 Sample : BSF0316S1
 Misc : 5.02g/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Mar 17 00:51:56 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030520.M
 Quant Title :
 QLast Update : Thu Mar 05 11:03:12 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	8.793	466394	22.156 ng/ml
Target Compounds				
1) t	2-Methylpentane	4.686	984014	31.840 ng/ml
2) t	2,2,4-Trimethylpentane	7.411	1132712	33.591 ng/ml
3) t	n-Heptane	7.752	362970	10.956 ng/ml
4) t	Benzene	7.886	442268	10.562 ng/ml
6) t	Toluene	10.624	1313245	32.208 ng/ml
7) t	Ethylbenzene	13.064	410597	10.747 ng/ml
8) t	m-Xylene	13.197	794031	21.567 ng/ml
9) t	O-Xylene	13.924	758192	21.318 ng/ml
10) t	1,2,4-Trimethylbenzene	16.202	654916	21.618 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB031620\
Data File : FB023960.D
Signal(s) : FID2B.CH
Acq On : 16 Mar 2020 11:53
Operator : DD/AJ
Sample : BSF0316S1
Misc : 5.02g/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Mar 17 00:51:56 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030520.M
Quant Title :
QLast Update : Thu Mar 05 11:03:12 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

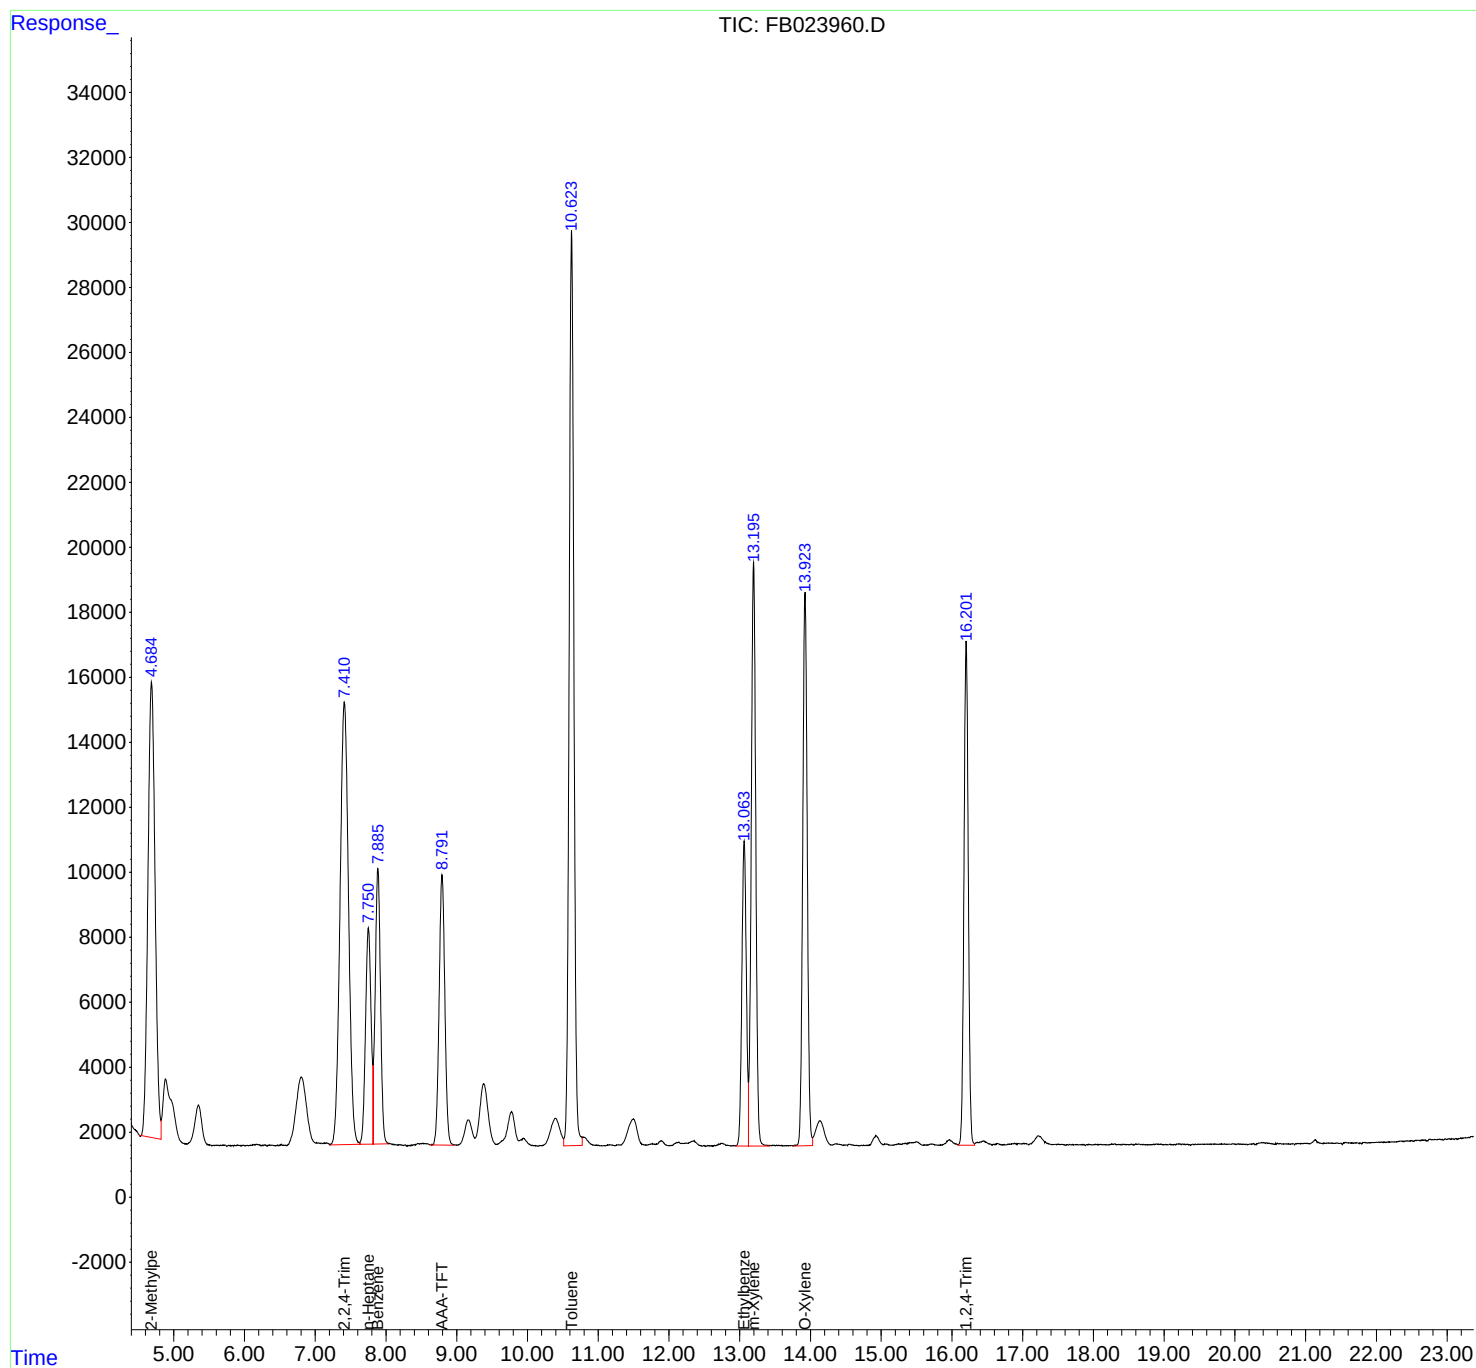

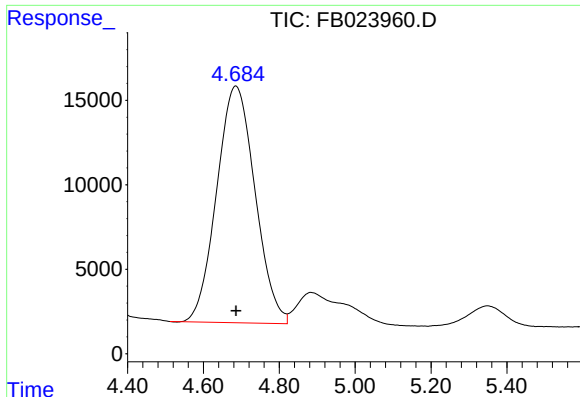


#1 2-Methylpentane

R.T.: 4.686 min
Delta R.T.: 0.000 min
Response: 984014
Conc: 31.84 ng/ml

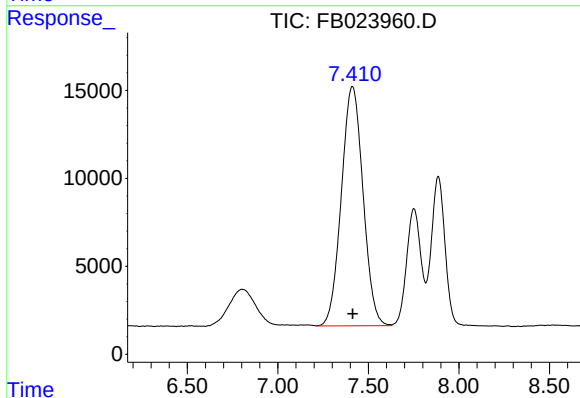


#2 2,2,4-Trimethylpentane

R.T.: 7.411 min
Delta R.T.: -0.002 min
Response: 1132712
Conc: 33.59 ng/ml

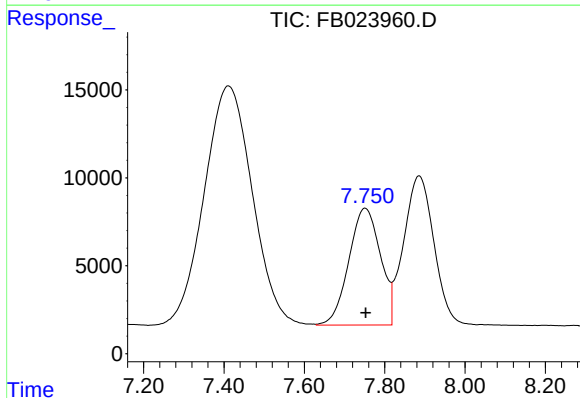


#3 n-Heptane

R.T.: 7.752 min
Delta R.T.: -0.002 min
Response: 362970
Conc: 10.96 ng/ml

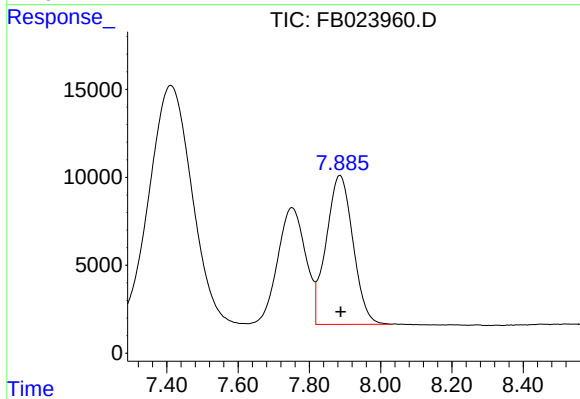


#4 Benzene

R.T.: 7.886 min
Delta R.T.: -0.002 min
Response: 442268
Conc: 10.56 ng/ml

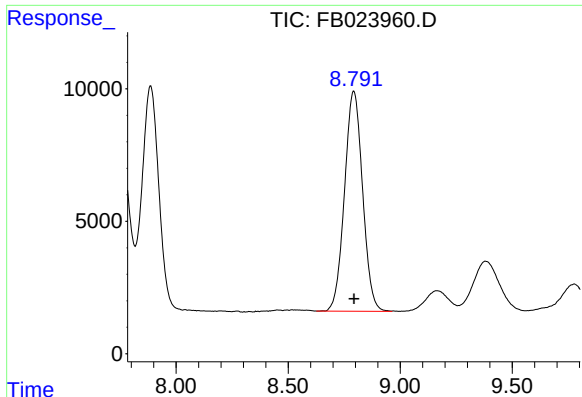


#5 AAA-TFT

R.T.: 8.793 min
Delta R.T.: -0.002 min
Response: 466394
Conc: 22.16 ng/ml

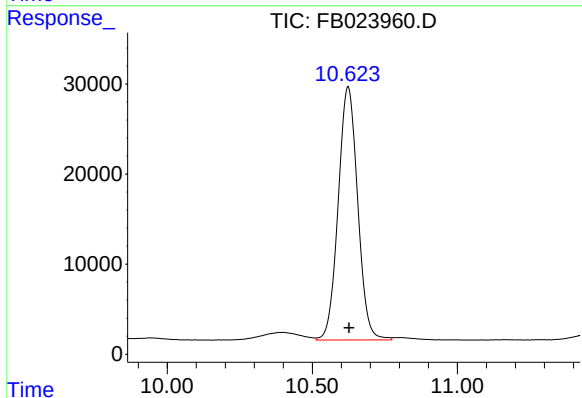


#6 Toluene

R.T.: 10.624 min
Delta R.T.: -0.002 min
Response: 1313245
Conc: 32.21 ng/ml

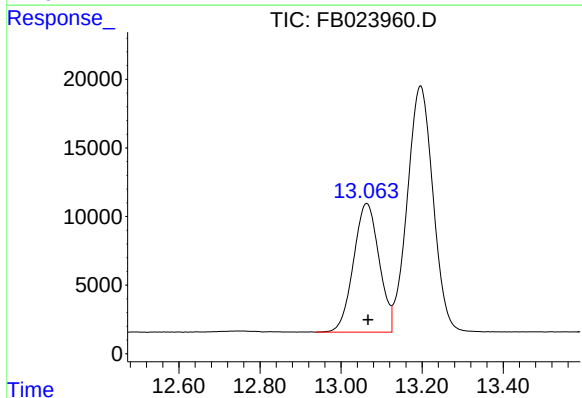


#7 Ethylbenzene

R.T.: 13.064 min
Delta R.T.: -0.003 min
Response: 410597
Conc: 10.75 ng/ml

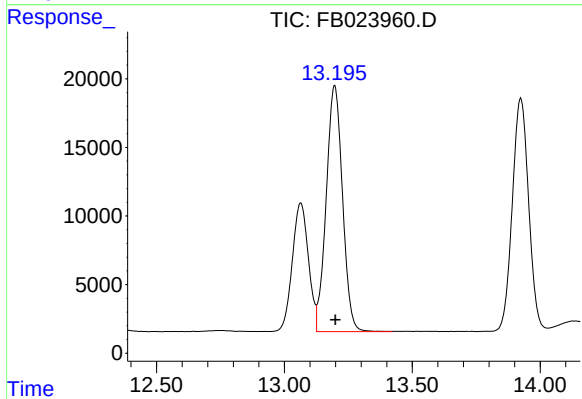


#8 m-Xylene

R.T.: 13.197 min
Delta R.T.: -0.003 min
Response: 794031
Conc: 21.57 ng/ml

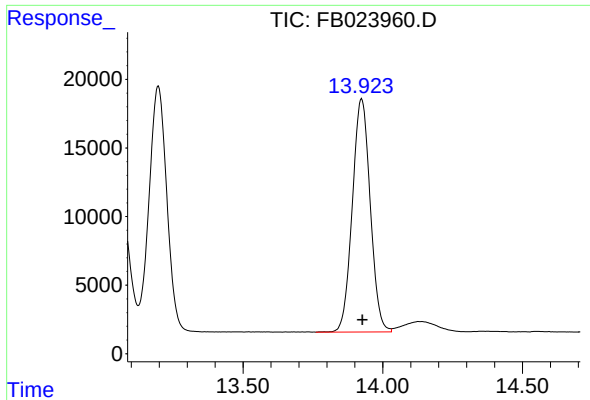

#9 O-Xylene

R.T.: 13.924 min
Delta R.T.: -0.003 min
Response: 758192
Conc: 21.32 ng/ml

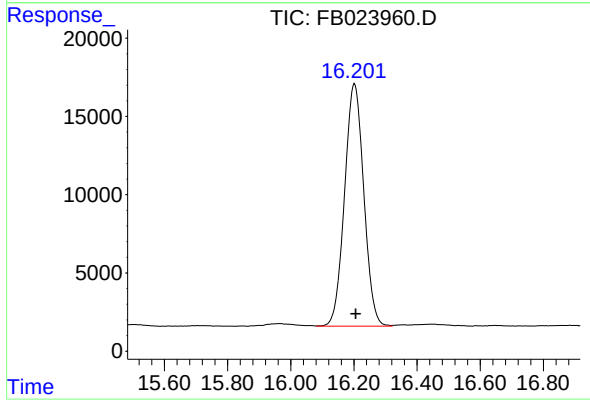

#10 1,2,4-Trimethylbenzene

R.T.: 16.202 min
Delta R.T.: -0.004 min
Response: 654916
Conc: 21.62 ng/ml