

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB031620\
Data File : FB023961.D
Signal(s) : FID2B.CH
Acq On : 16 Mar 2020 13:32
Operator : DD/AJ
Sample : L1943-03
Misc : 5.04g/5.00ml DI WATER
ALS Vial : 4 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Mar 17 00:52:01 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030520.M
Quant Title :
QLast Update : Thu Mar 05 11:03:12 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.789	468126	22.238 ng/ml
Target Compounds			
6) t Toluene	10.620	3775	0.093 ng/ml
9) t O-Xylene	13.898	3697	0.104 ng/ml
10) t 1,2,4-Trimethylbenzene	16.206	5178	0.171 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB031620\
Data File : FB023961.D
Signal(s) : FID2B.CH
Acq On : 16 Mar 2020 13:32
Operator : DD/AJ
Sample : L1943-03
Misc : 5.04g/5.00ml DI WATER
ALS Vial : 4 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Mar 17 00:52:01 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030520.M
Quant Title :
QLast Update : Thu Mar 05 11:03:12 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

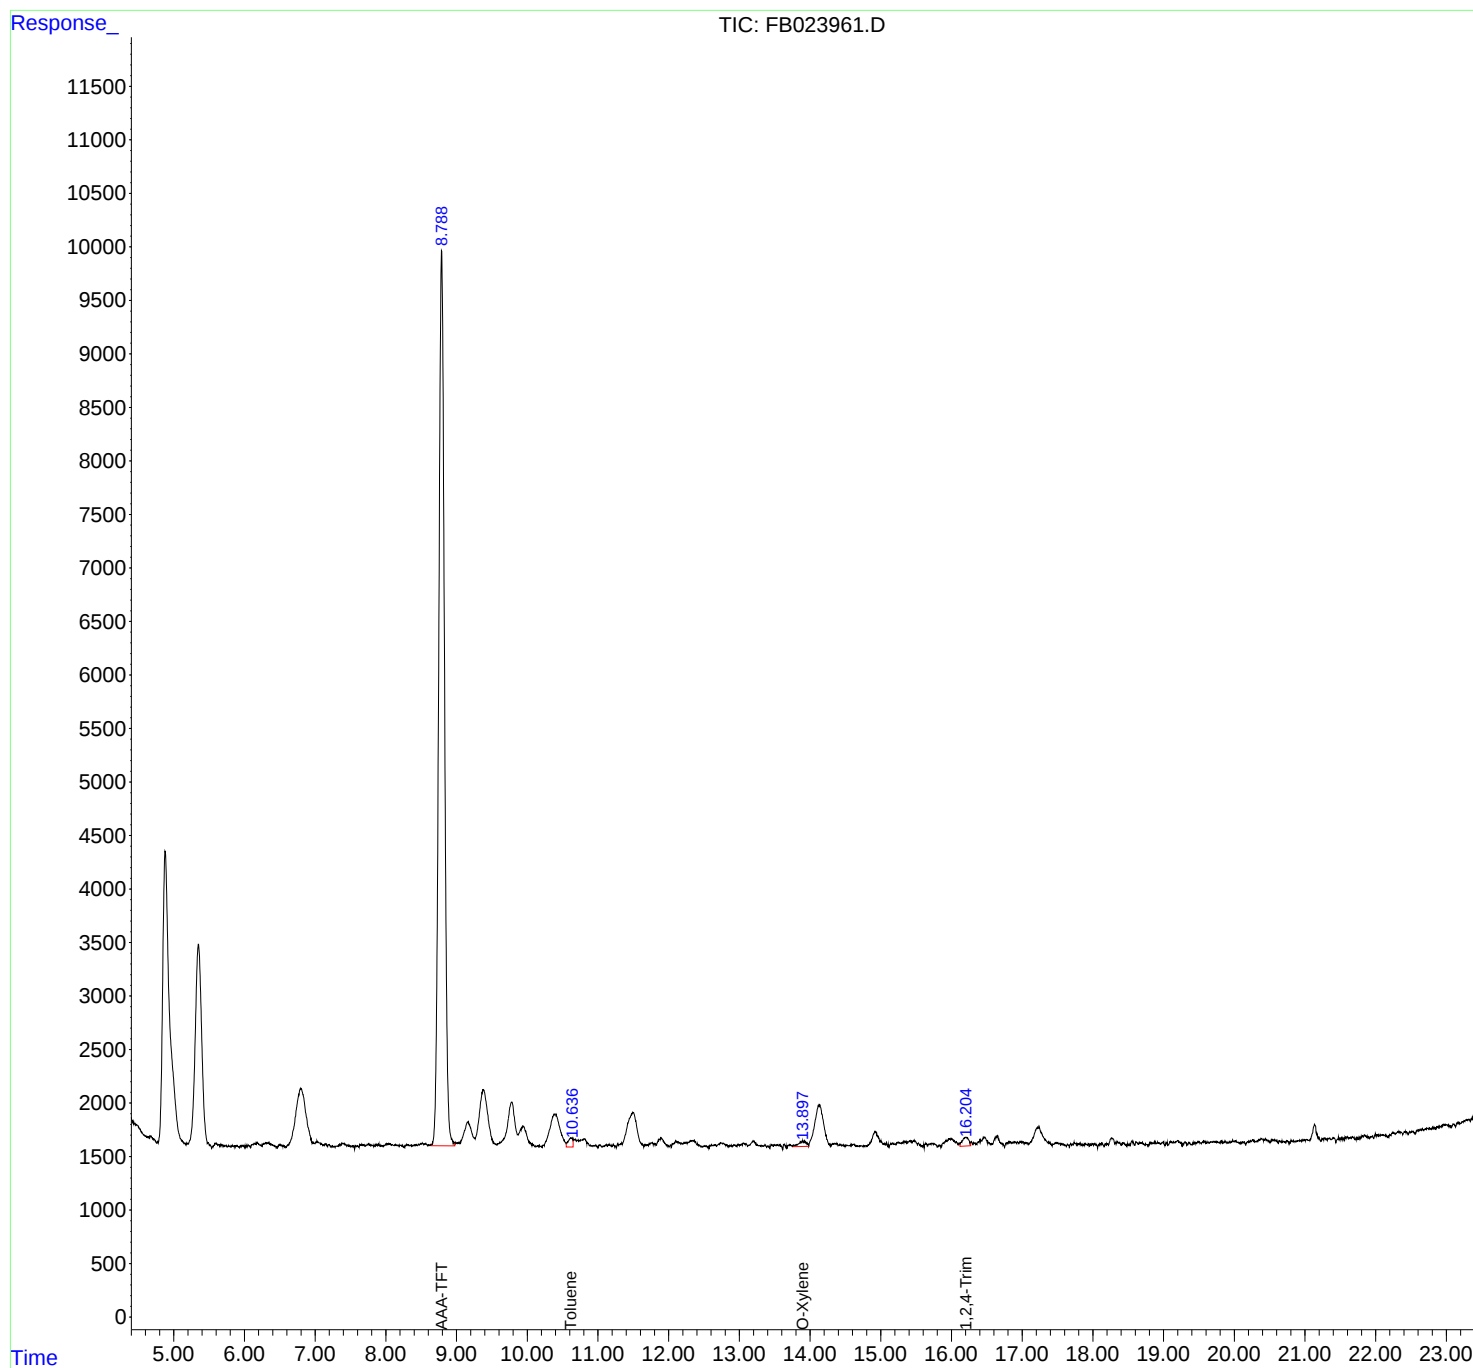

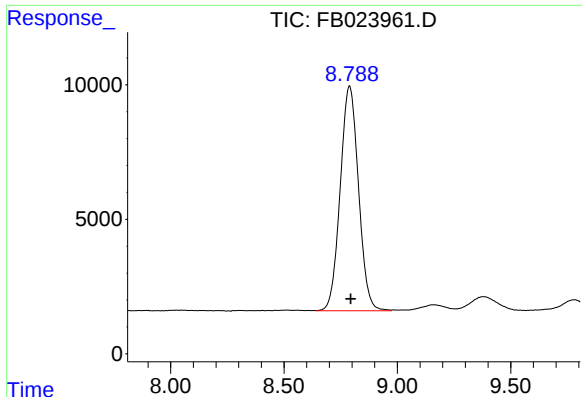


#5 AAA-TFT

R.T.: 8.789 min
Delta R.T.: -0.005 min
Response: 468126
Conc: 22.24 ng/ml

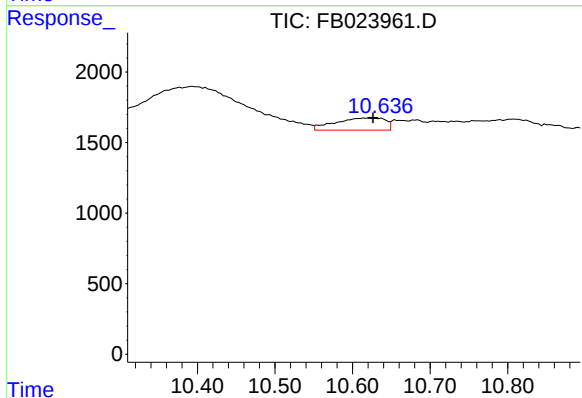


#6 Toluene

R.T.: 10.620 min
Delta R.T.: -0.006 min
Response: 3775
Conc: 0.09 ng/ml

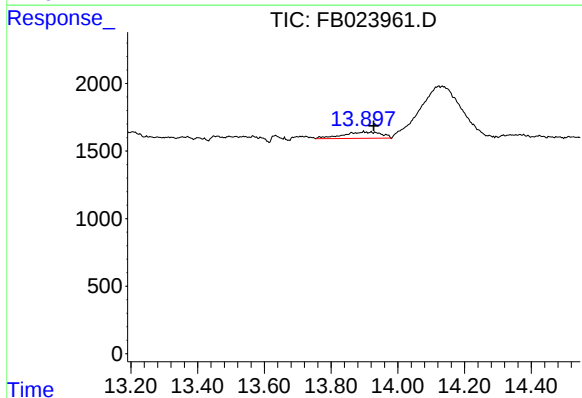

#9 O-Xylene

R.T.: 13.898 min
Delta R.T.: -0.030 min
Response: 3697
Conc: 0.10 ng/ml

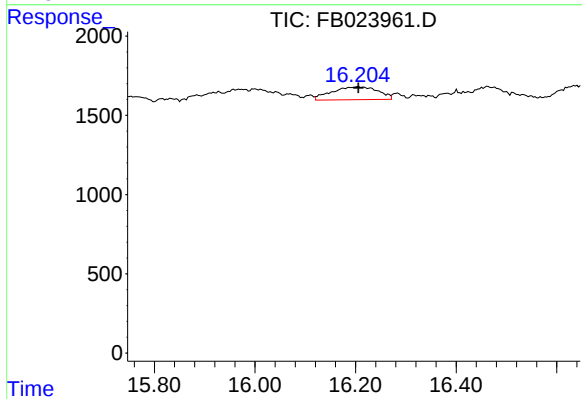

#10 1,2,4-Trimethylbenzene

R.T.: 16.206 min
Delta R.T.: 0.000 min
Response: 5178
Conc: 0.17 ng/ml