

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB031620\
 Data File : FB023962.D
 Signal(s) : FID2B.CH
 Acq On : 16 Mar 2020 14:02
 Operator : DD/AJ
 Sample : L1943-03MS
 Misc : 5.01g/5.00ml DI WATER
 ALS Vial : 5 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Mar 17 00:52:05 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030520.M
 Quant Title :
 QLast Update : Thu Mar 05 11:03:12 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.793	438028	20.808 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.685	936442	30.301 ng/ml
2) t 2,2,4-Trimethylpentane	7.412	1046307	31.029 ng/ml
3) t n-Heptane	7.752	328654	9.920 ng/ml
4) t Benzene	7.886	428238	10.227 ng/ml
6) t Toluene	10.624	1248790	30.627 ng/ml
7) t Ethylbenzene	13.064	384055	10.052 ng/ml
8) t m-Xylene	13.197	744458	20.220 ng/ml
9) t O-Xylene	13.924	714828	20.099 ng/ml
10) t 1,2,4-Trimethylbenzene	16.202	594026	19.608 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB031620\
Data File : FB023962.D
Signal(s) : FID2B.CH
Acq On : 16 Mar 2020 14:02
Operator : DD/AJ
Sample : L1943-03MS
Misc : 5.01g/5.00ml DI WATER
ALS Vial : 5 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Mar 17 00:52:05 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030520.M
Quant Title :
QLast Update : Thu Mar 05 11:03:12 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

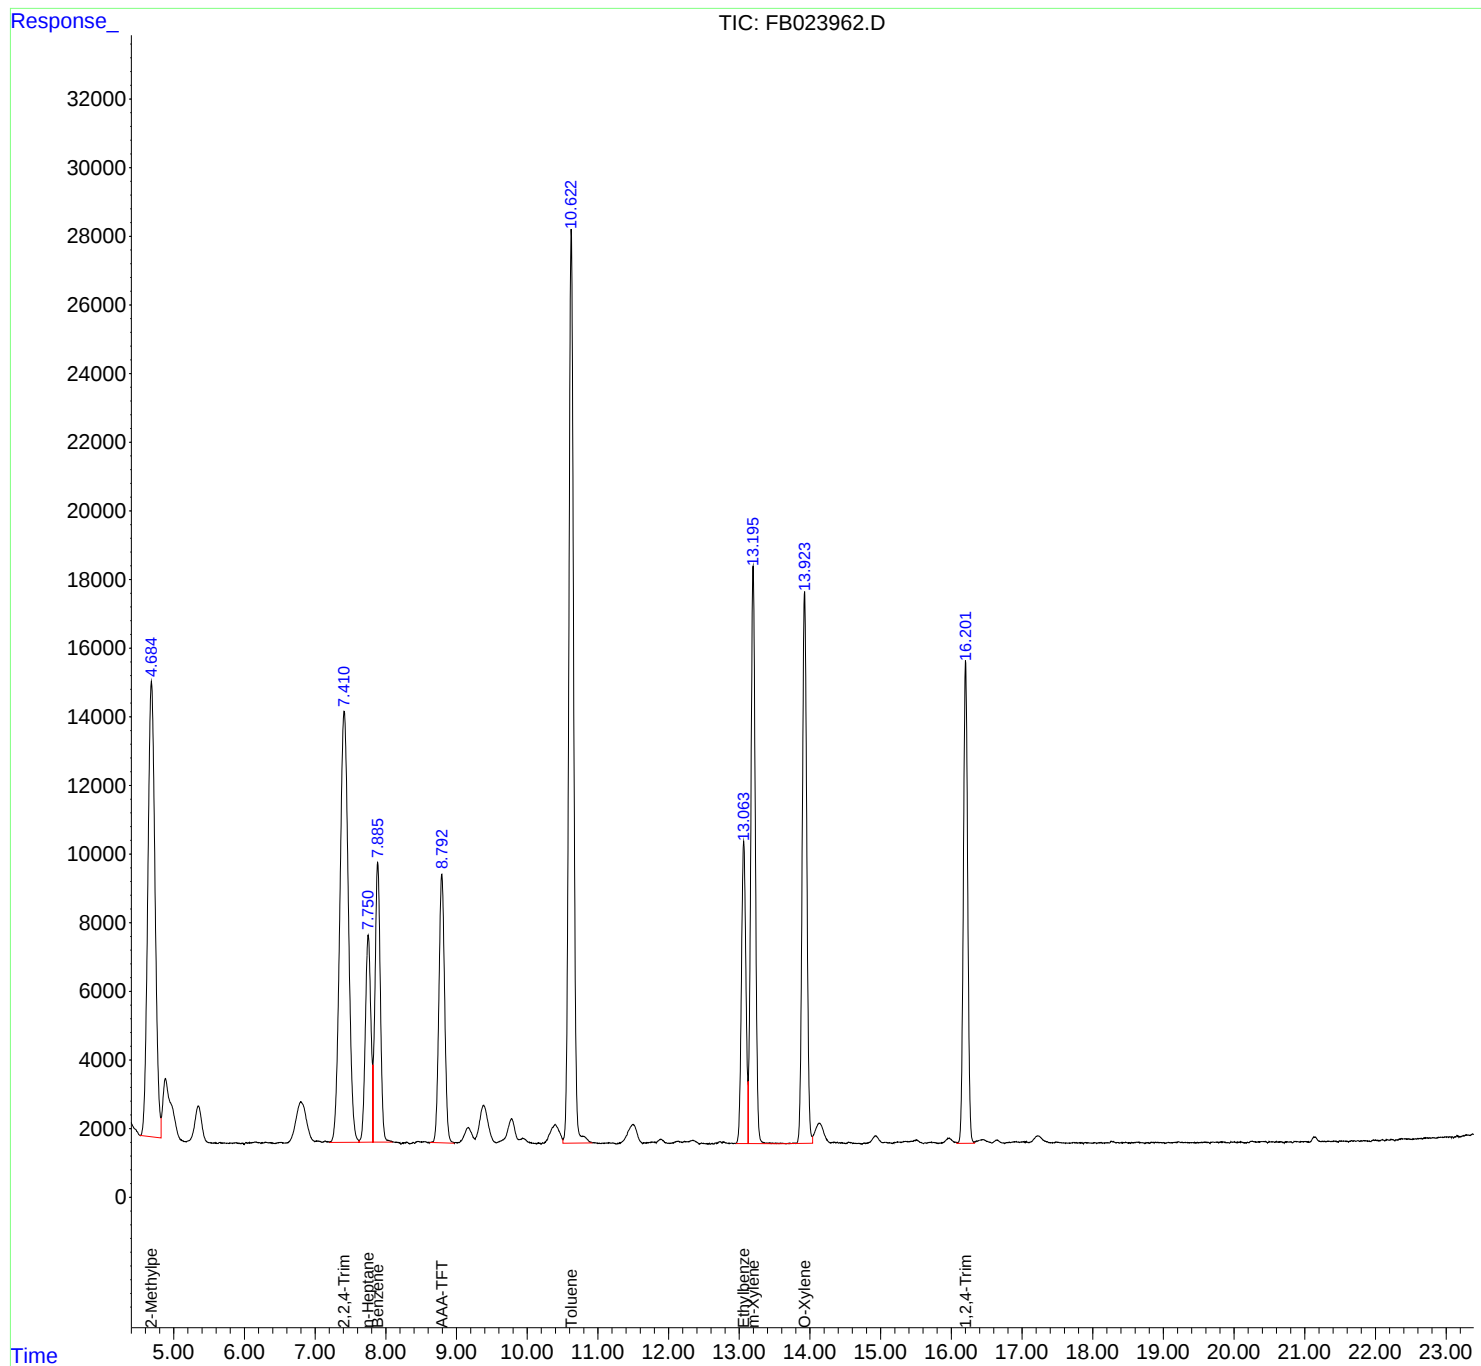

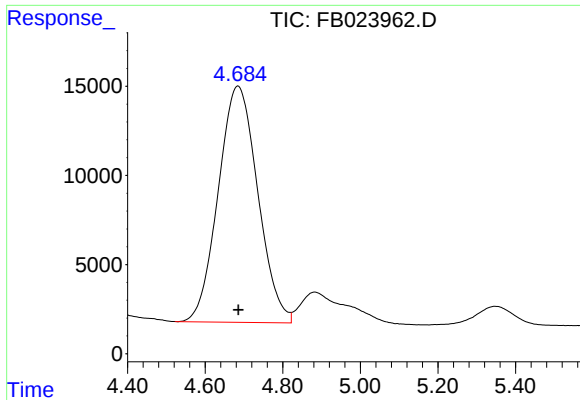


#1 2-Methylpentane

R.T.: 4.685 min
Delta R.T.: -0.001 min
Response: 936442
Conc: 30.30 ng/ml

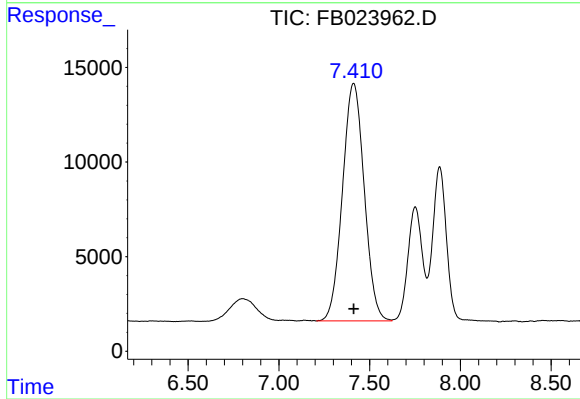


#2 2,2,4-Trimethylpentane

R.T.: 7.412 min
Delta R.T.: -0.001 min
Response: 1046307
Conc: 31.03 ng/ml

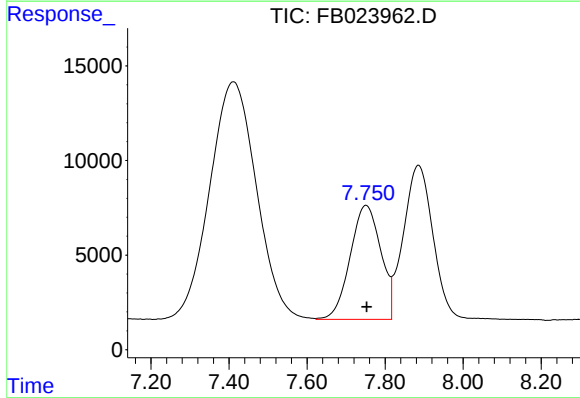


#3 n-Heptane

R.T.: 7.752 min
Delta R.T.: -0.002 min
Response: 328654
Conc: 9.92 ng/ml

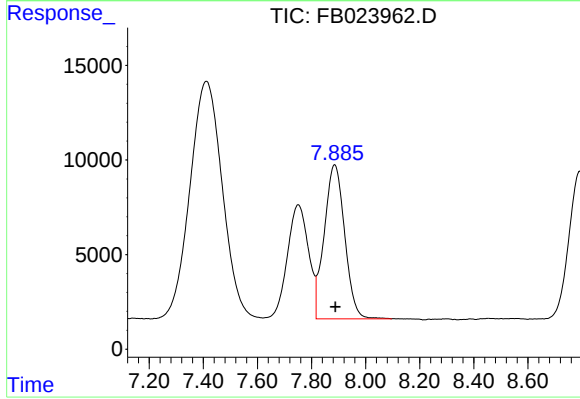


#4 Benzene

R.T.: 7.886 min
Delta R.T.: -0.002 min
Response: 428238
Conc: 10.23 ng/ml

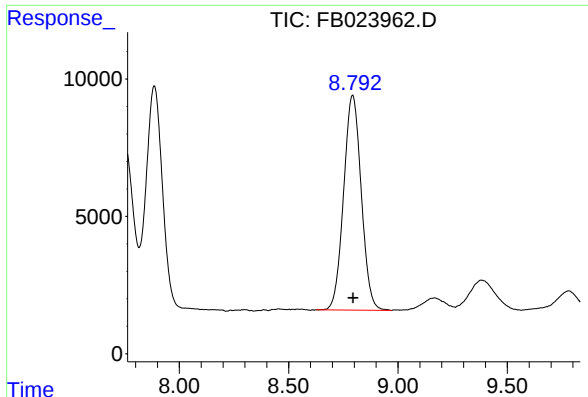


#5 AAA-TFT

R.T.: 8.793 min
Delta R.T.: -0.002 min
Response: 438028
Conc: 20.81 ng/ml

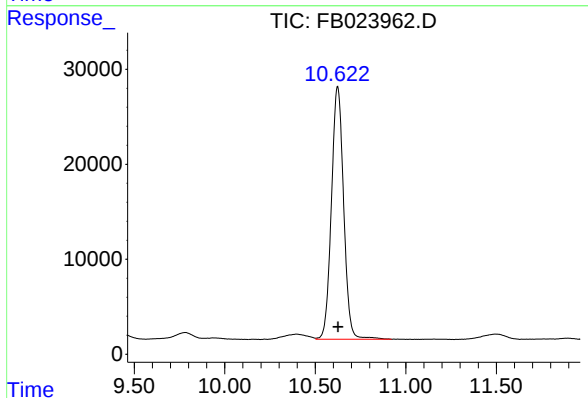


#6 Toluene

R.T.: 10.624 min
Delta R.T.: -0.003 min
Response: 1248790
Conc: 30.63 ng/ml

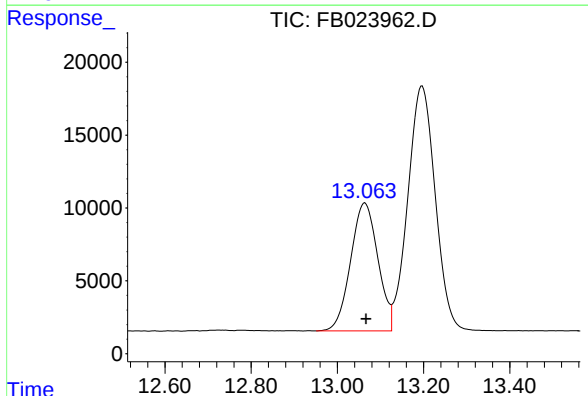


#7 Ethylbenzene

R.T.: 13.064 min
Delta R.T.: -0.003 min
Response: 384055
Conc: 10.05 ng/ml

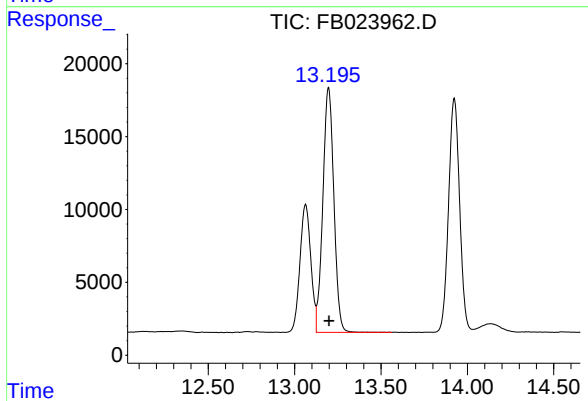


#8 m-Xylene

R.T.: 13.197 min
Delta R.T.: -0.003 min
Response: 744458
Conc: 20.22 ng/ml

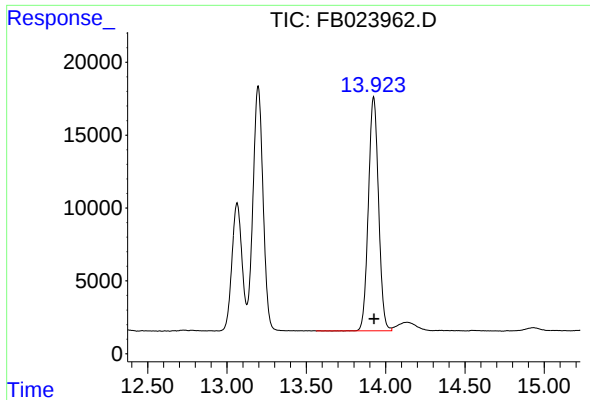

#9 O-Xylene

R.T.: 13.924 min
Delta R.T.: -0.003 min
Response: 714828
Conc: 20.10 ng/ml

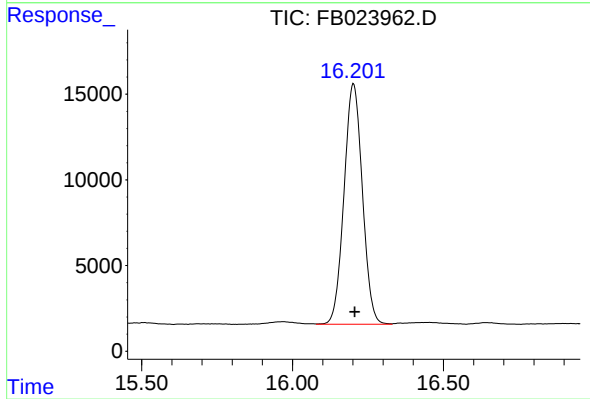

#10 1,2,4-Trimethylbenzene

R.T.: 16.202 min
Delta R.T.: -0.004 min
Response: 594026
Conc: 19.61 ng/ml