

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB031620\
 Data File : FB023963.D
 Signal(s) : FID2B.CH
 Acq On : 16 Mar 2020 14:32
 Operator : DD/AJ
 Sample : L1943-03MSD
 Misc : 5.03g/5.00ml DI WATER
 ALS Vial : 6 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Mar 17 00:52:10 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030520.M
 Quant Title :
 QLast Update : Thu Mar 05 11:03:12 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	8.793	404438	19.213 ng/ml
Target Compounds				
1) t	2-Methylpentane	4.685	764444	24.735 ng/ml
2) t	2,2,4-Trimethylpentane	7.412	861163	25.538 ng/ml
3) t	n-Heptane	7.752	268293	8.098 ng/ml
4) t	Benzene	7.886	386201	9.223 ng/ml
6) t	Toluene	10.624	1113095	27.299 ng/ml
7) t	Ethylbenzene	13.064	343743	8.997 ng/ml
8) t	m-Xylene	13.197	668968	18.170 ng/ml
9) t	O-Xylene	13.925	652879	18.357 ng/ml
10) t	1,2,4-Trimethylbenzene	16.203	551046	18.189 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB031620\
Data File : FB023963.D
Signal(s) : FID2B.CH
Acq On : 16 Mar 2020 14:32
Operator : DD/AJ
Sample : L1943-03MSD
Misc : 5.03g/5.00ml DI WATER
ALS Vial : 6 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Mar 17 00:52:10 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030520.M
Quant Title :
QLast Update : Thu Mar 05 11:03:12 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

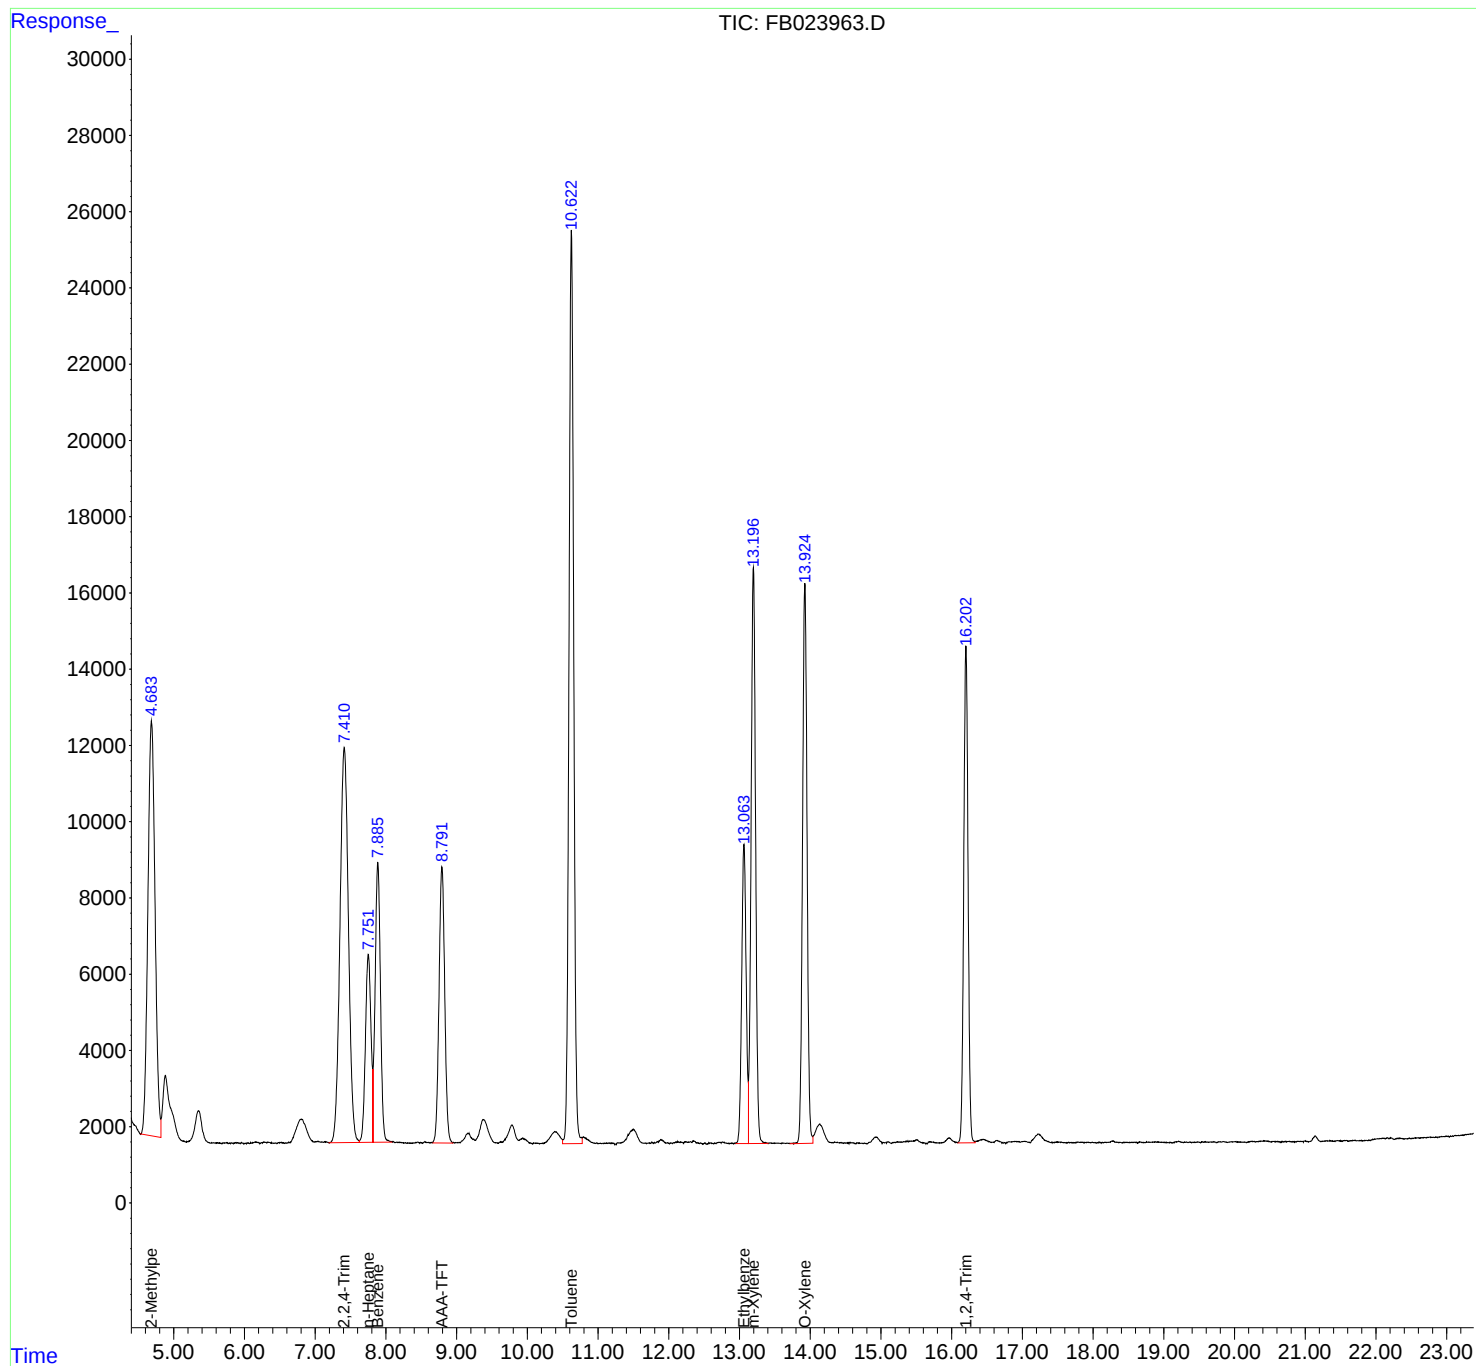

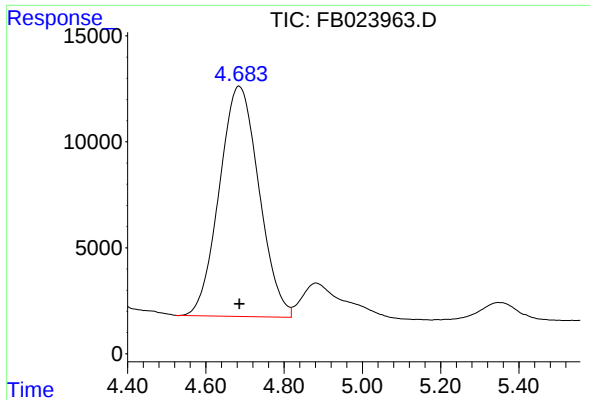


#1 2-Methylpentane

R.T.: 4.685 min
Delta R.T.: -0.001 min
Response: 764444
Conc: 24.74 ng/ml

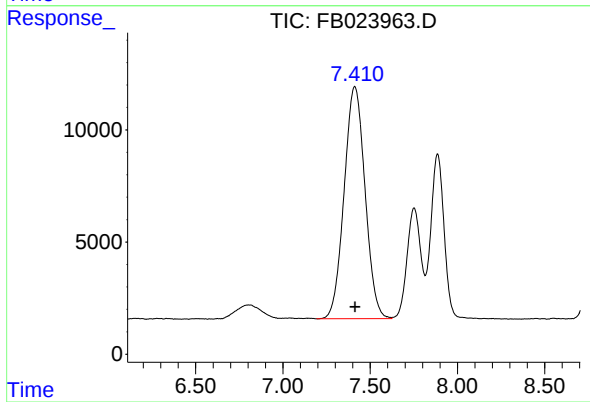


#2 2,2,4-Trimethylpentane

R.T.: 7.412 min
Delta R.T.: -0.001 min
Response: 861163
Conc: 25.54 ng/ml

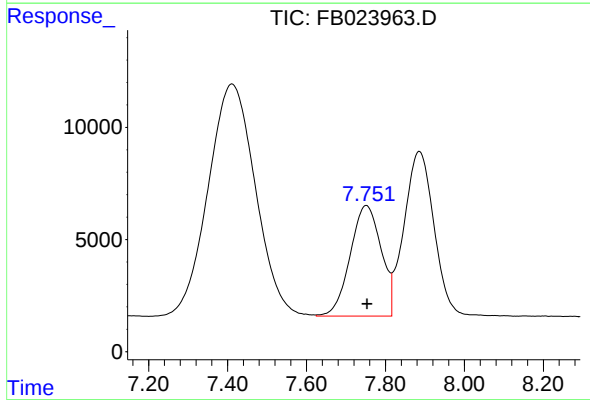


#3 n-Heptane

R.T.: 7.752 min
Delta R.T.: -0.002 min
Response: 268293
Conc: 8.10 ng/ml

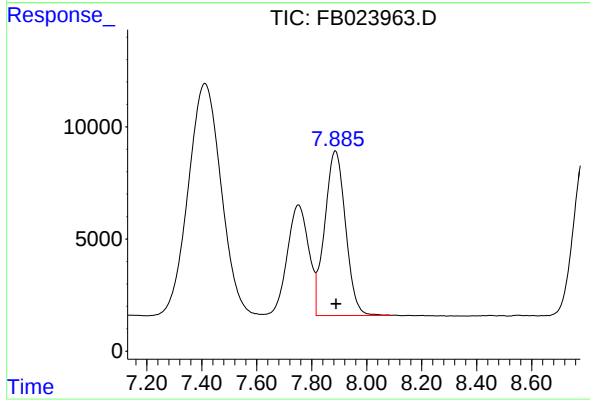


#4 Benzene

R.T.: 7.886 min
Delta R.T.: -0.002 min
Response: 386201
Conc: 9.22 ng/ml

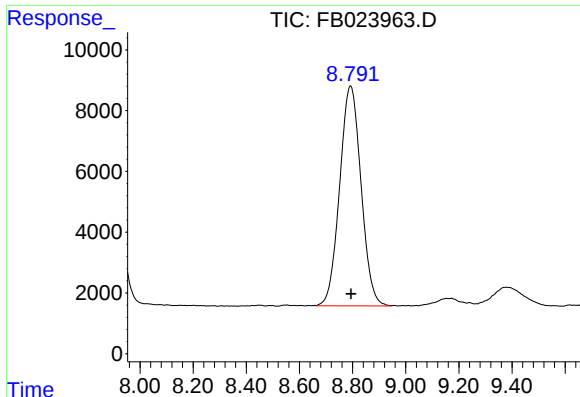


#5 AAA-TFT

R.T.: 8.793 min
Delta R.T.: -0.002 min
Response: 404438
Conc: 19.21 ng/ml

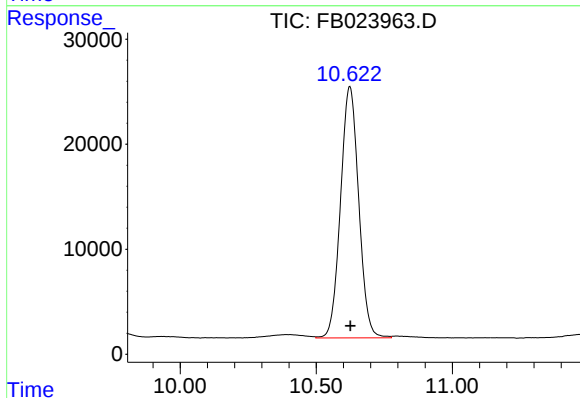


#6 Toluene

R.T.: 10.624 min
Delta R.T.: -0.003 min
Response: 1113095
Conc: 27.30 ng/ml

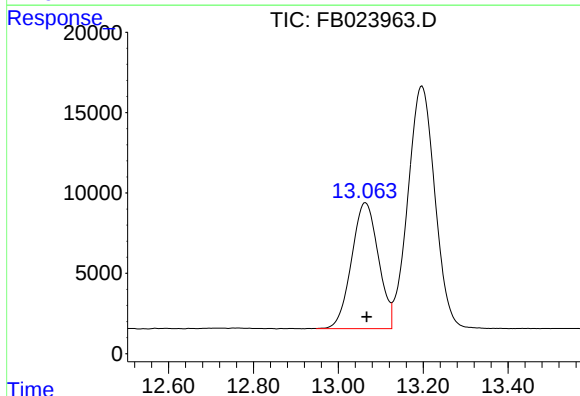


#7 Ethylbenzene

R.T.: 13.064 min
Delta R.T.: -0.003 min
Response: 343743
Conc: 9.00 ng/ml

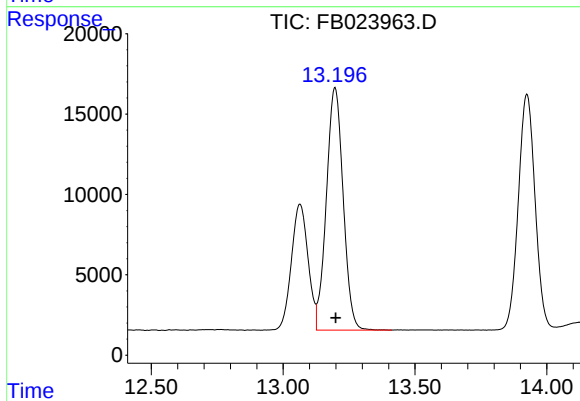


#8 m-Xylene

R.T.: 13.197 min
Delta R.T.: -0.003 min
Response: 668968
Conc: 18.17 ng/ml

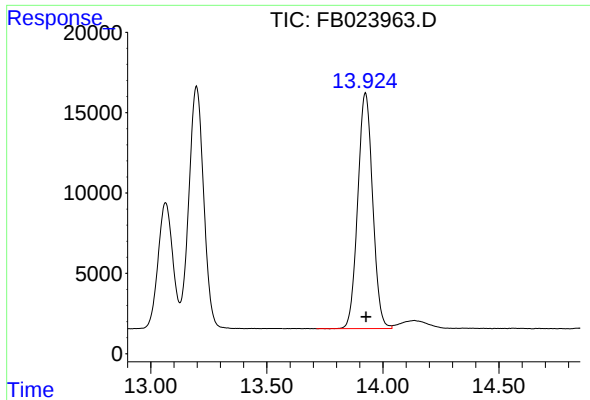

#9 O-Xylene

R.T.: 13.925 min
Delta R.T.: -0.003 min
Response: 652879
Conc: 18.36 ng/ml

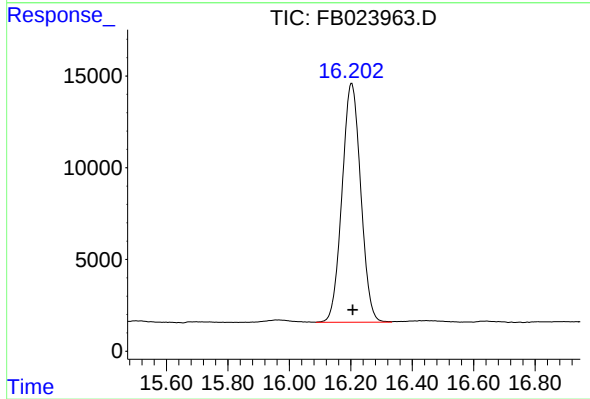

#10 1,2,4-Trimethylbenzene

R.T.: 16.203 min
Delta R.T.: -0.003 min
Response: 551046
Conc: 18.19 ng/ml