

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB031621\
 Data File : FB025523.D
 Signal(s) : FID2B.CH
 Acq On : 16 Mar 2021 13:02
 Operator : DD/AJ
 Sample : 10 GRO STD
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Mar 17 08:38:32 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB031621.M
 Quant Title :
 QLast Update : Wed Mar 17 08:34:43 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.801	188937	8.854 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.691	436441	14.422 ng/ml
2) t 2,2,4-Trimethylpentane	7.420	468573	14.602 ng/ml
3) t n-Heptane	7.759	150258	4.762 ng/ml
4) t Benzene	7.895	184109	4.618 ng/ml
6) t Toluene	10.632	542075	14.054 ng/ml
7) t Ethylbenzene	13.072	167864	4.781 ng/ml
8) t m-Xylene	13.205	340521	9.656 ng/ml
9) t O-Xylene	13.933	325350	9.509 ng/ml
10) t 1,2,4-Trimethylbenzene	16.211	276950	9.261 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB031621\
Data File : FB025523.D
Signal(s) : FID2B.CH
Acq On : 16 Mar 2021 13:02
Operator : DD/AJ
Sample : 10 GRO STD
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Mar 17 08:38:32 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB031621.M
Quant Title :
QLast Update : Wed Mar 17 08:34:43 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

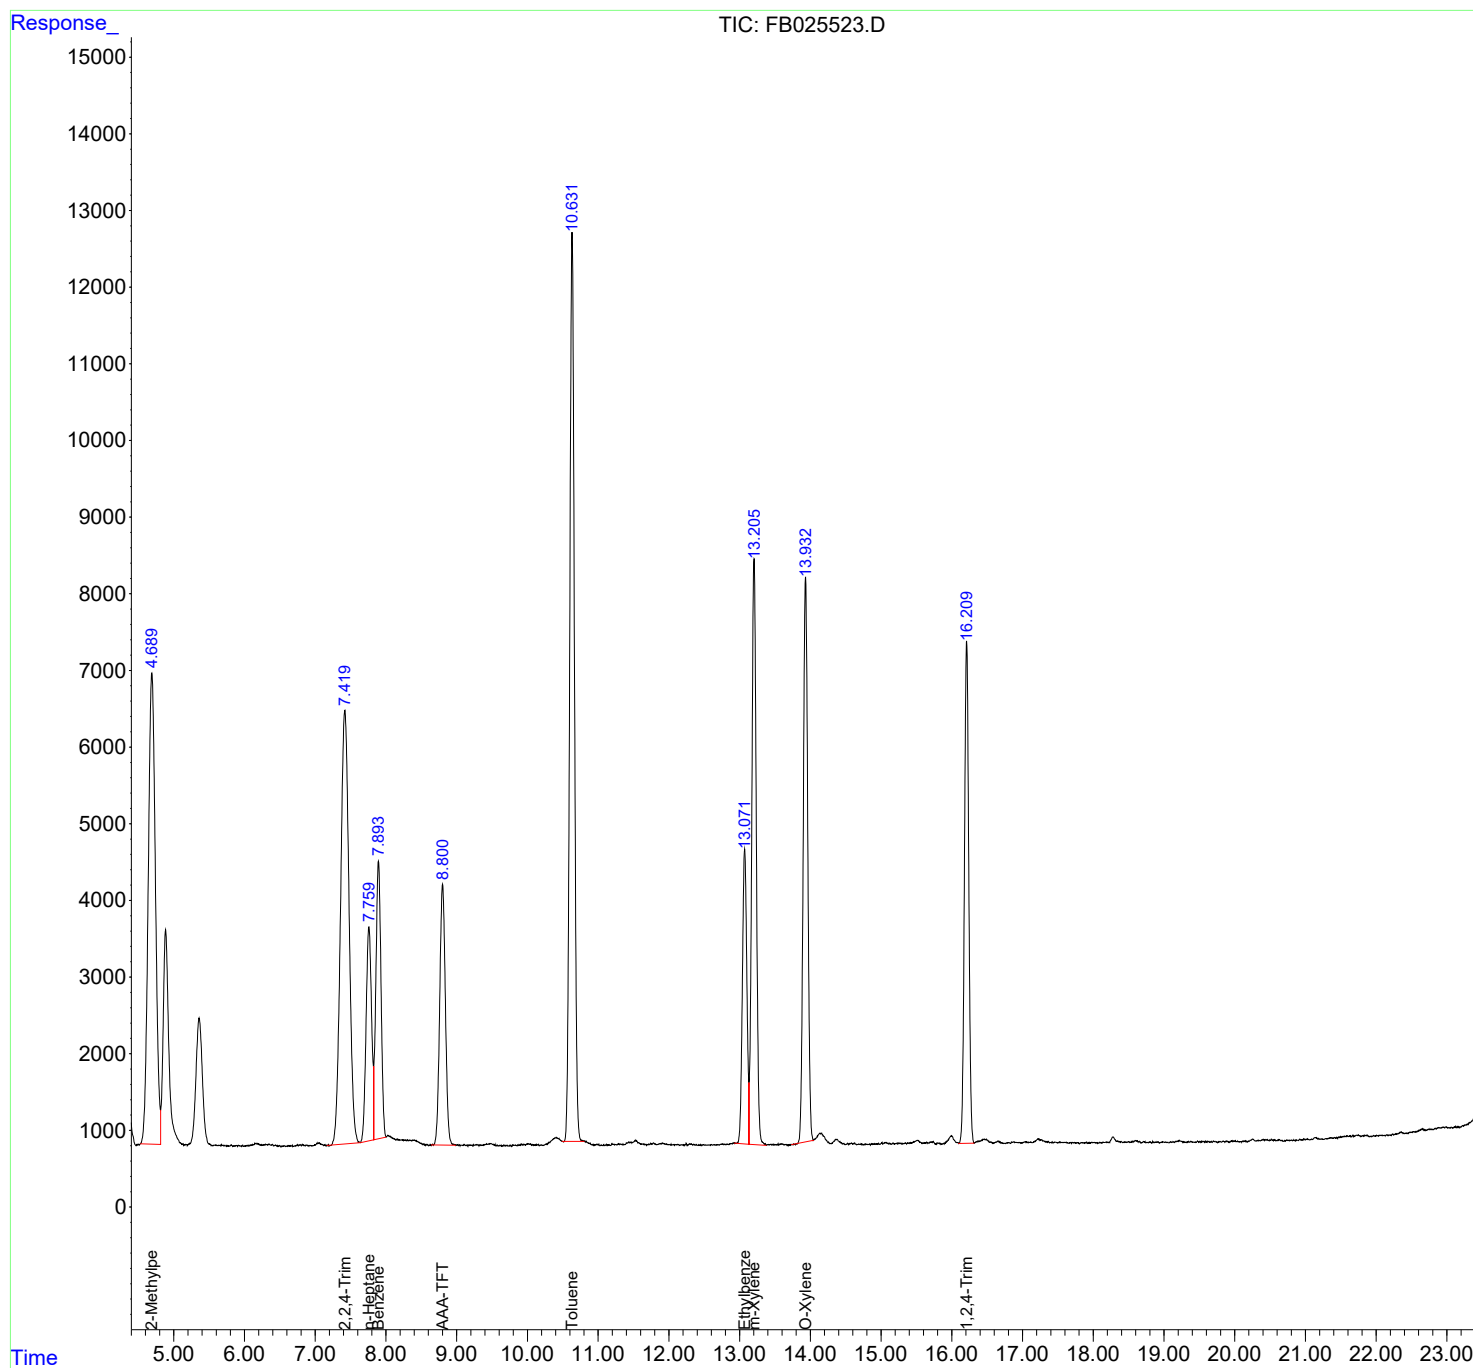


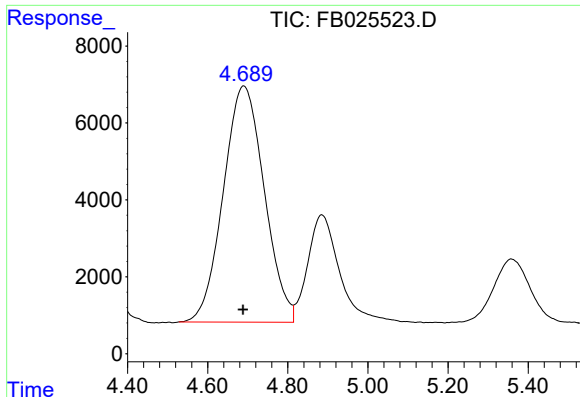

#1 2-Methylpentane


R.T.: 4.691 min
Delta R.T.: 0.003 min
Response: 436441
Conc: 14.42 ng/ml

Instrument :
FID_B
ClientSampleId :

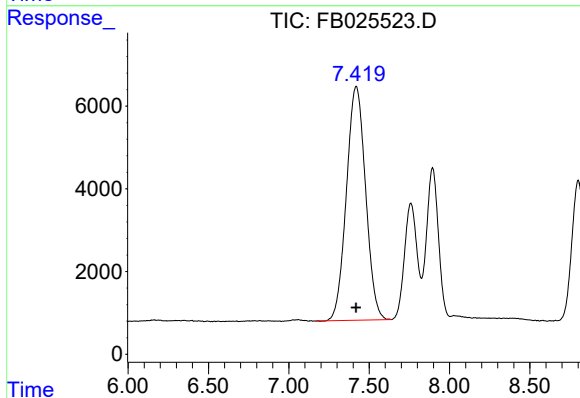


#2 2,2,4-Trimethylpentane

R.T.: 7.420 min
Delta R.T.: 0.002 min
Response: 468573
Conc: 14.60 ng/ml

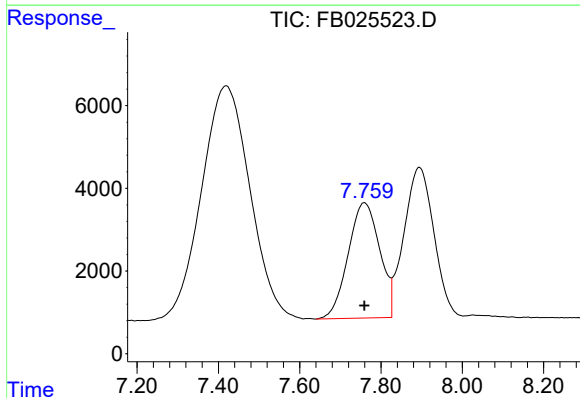


#3 n-Heptane

R.T.: 7.759 min
Delta R.T.: 0.000 min
Response: 150258
Conc: 4.76 ng/ml

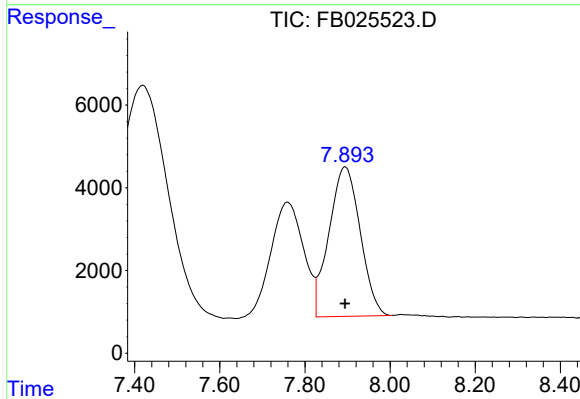

#4 Benzene


R.T.: 7.895 min
Delta R.T.: 0.000 min
Response: 184109
Conc: 4.62 ng/ml

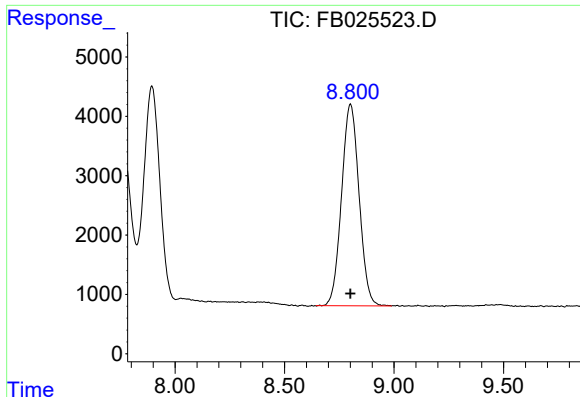

#5 AAA-TFT


R.T.: 8.801 min
Delta R.T.: 0.000 min
Response: 188937
Conc: 8.85 ng/ml

Instrument :
FID_B
ClientSampleId :

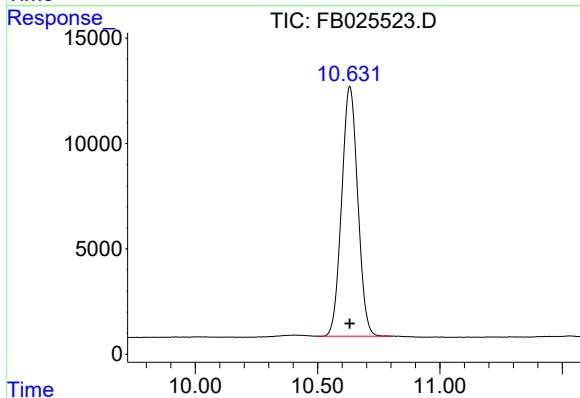


#6 Toluene

R.T.: 10.632 min
Delta R.T.: 0.000 min
Response: 542075
Conc: 14.05 ng/ml

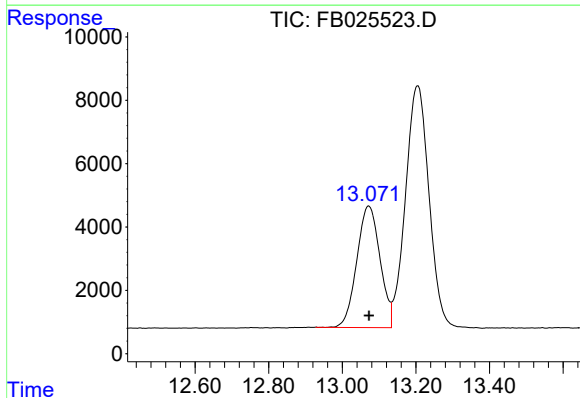


#7 Ethylbenzene

R.T.: 13.072 min
Delta R.T.: 0.000 min
Response: 167864
Conc: 4.78 ng/ml

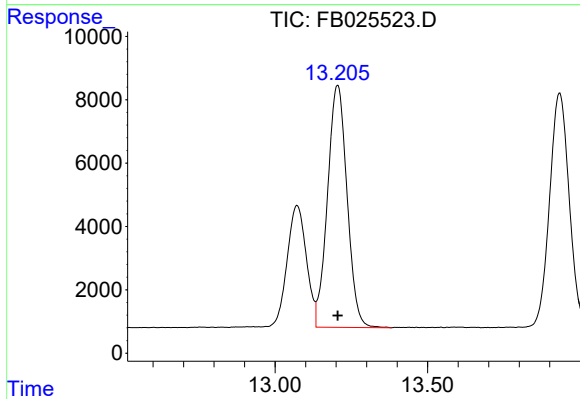

#8 m-Xylene


R.T.: 13.205 min
Delta R.T.: 0.000 min
Response: 340521
Conc: 9.66 ng/ml

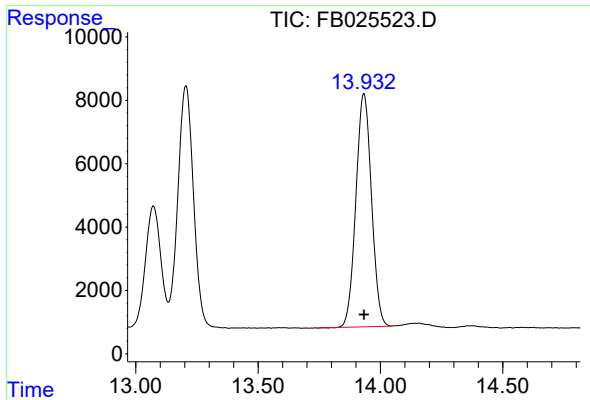

#9 O-Xylene

R.T.: 13.933 min
Delta R.T.: 0.000 min
Response: 325350
Conc: 9.51 ng/ml

Instrument :
FID_B
ClientSampleId :

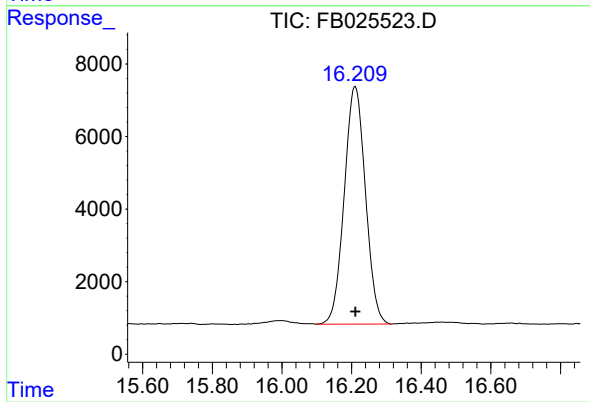

#10 1,2,4-Trimethylbenzene

R.T.: 16.211 min
Delta R.T.: 0.000 min
Response: 276950
Conc: 9.26 ng/ml