

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB031622\
 Data File : FB026696.D
 Signal(s) : FID2B.CH
 Acq On : 16 Mar 2022 20:52
 Operator : AJ/MA
 Sample : N1966-15
 Misc : 5.01G/5.00 ML DI WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Mar 17 01:01:32 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030822.M
 Quant Title :
 QLast Update : Fri Mar 11 13:08:49 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.791	170800	16.277 ng/ml
Target Compounds			
3) t n-Heptane	7.734	3081	0.156 ng/ml
4) t Benzene	7.885	668364	28.965 ng/ml
6) t Toluene	10.616	81802	3.736 ng/ml
7) t Ethylbenzene	13.055	1199815	59.699 ng/ml
8) t m-Xylene	13.185	1405981	69.767 ng/ml
9) t O-Xylene	13.915	355805	17.835 ng/ml
10) t 1,2,4-Trimethylbenzene	16.190	411770	20.666 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB031622\
Data File : FB026696.D
Signal(s) : FID2B.CH
Acq On : 16 Mar 2022 20:52
Operator : AJ/MA
Sample : N1966-15
Misc : 5.01G/5.00 ML DI WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Mar 17 01:01:32 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030822.M
Quant Title :
QLast Update : Fri Mar 11 13:08:49 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

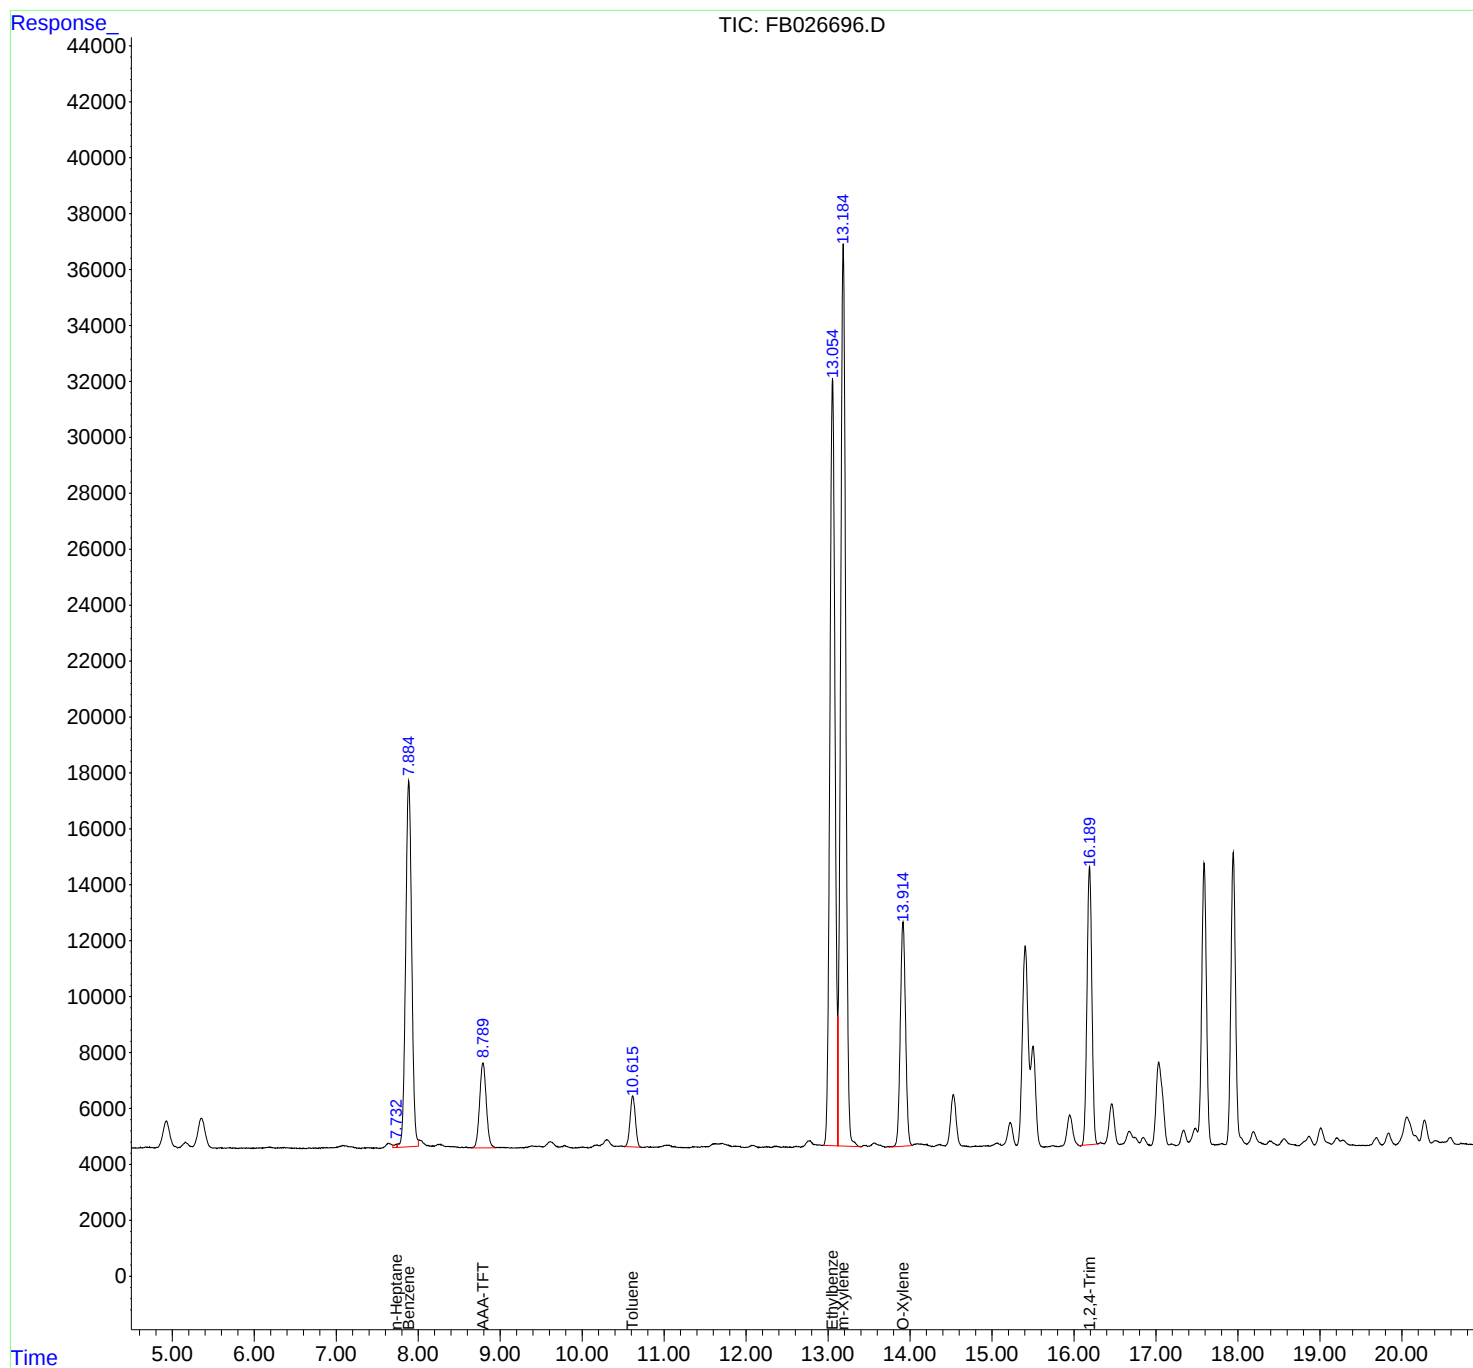


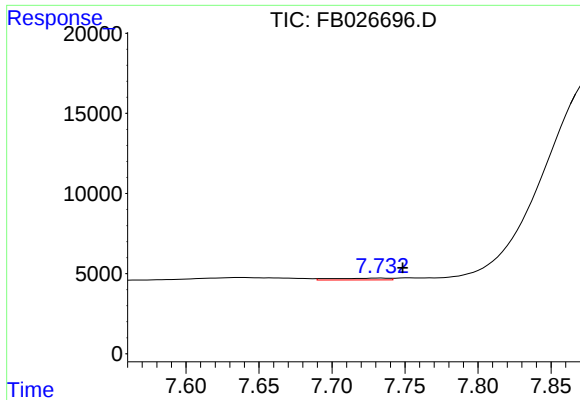

#3 n-Heptane


R.T.: 7.734 min
Delta R.T.: -0.015 min
Response: 3081
Conc: 0.16 ng/ml

Instrument :
FID_B
ClientSampleId :

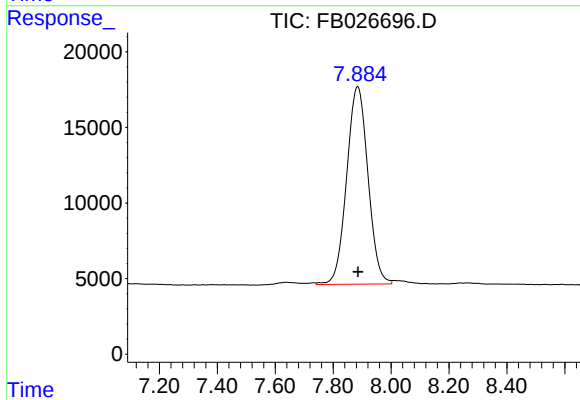


#4 Benzene

R.T.: 7.885 min
Delta R.T.: 0.000 min
Response: 668364
Conc: 28.97 ng/ml

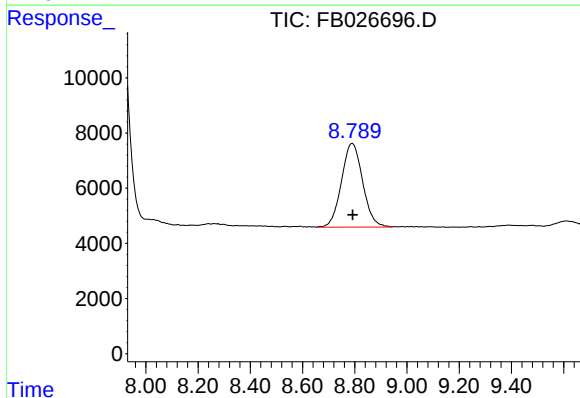


#5 AAA-TFT

R.T.: 8.791 min
Delta R.T.: 0.000 min
Response: 170800
Conc: 16.28 ng/ml

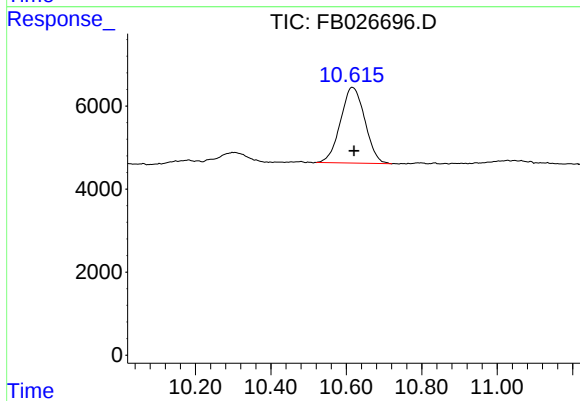

#6 Toluene


R.T.: 10.616 min
Delta R.T.: -0.005 min
Response: 81802
Conc: 3.74 ng/ml

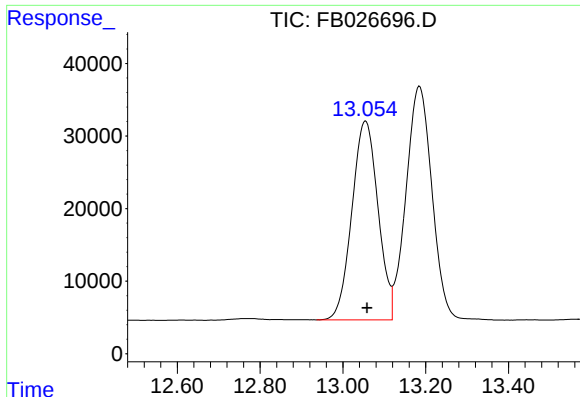

#7 Ethylbenzene


R.T.: 13.055 min
Delta R.T.: -0.004 min
Response: 1199815
Conc: 59.70 ng/ml

Instrument :
FID_B
ClientSampleId :

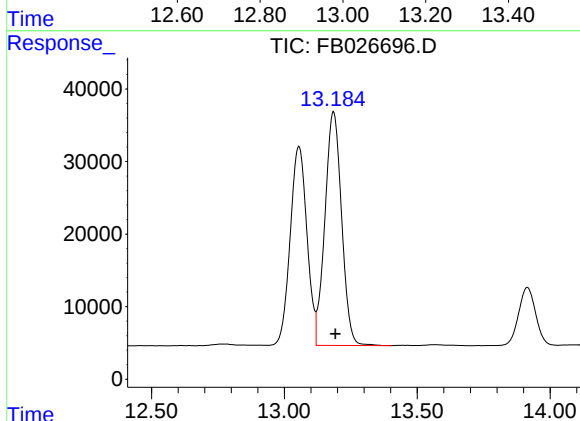


#8 m-Xylene

R.T.: 13.185 min
Delta R.T.: -0.006 min
Response: 1405981
Conc: 69.77 ng/ml

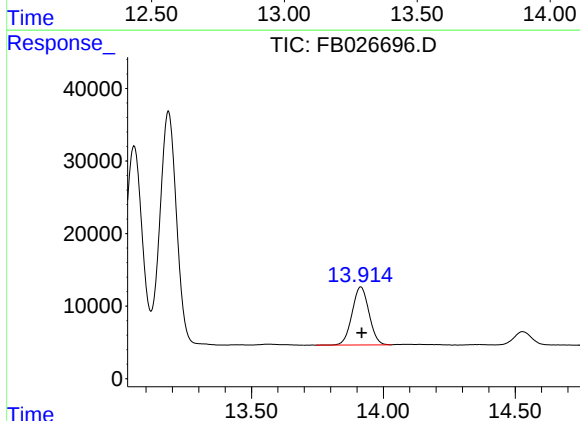

#9 o-Xylene

R.T.: 13.915 min
Delta R.T.: -0.004 min
Response: 355805
Conc: 17.83 ng/ml

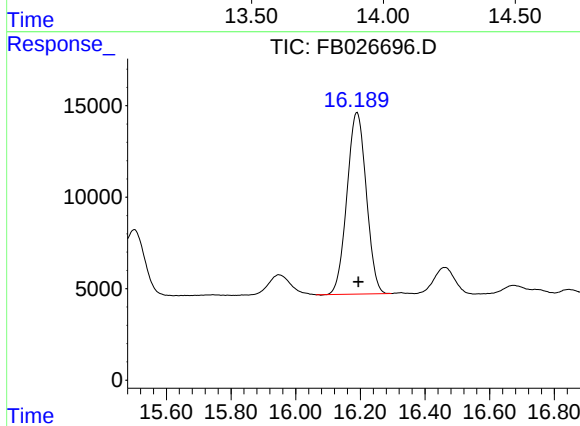

#10 1,2,4-Trimethylbenzene

R.T.: 16.190 min
Delta R.T.: -0.004 min
Response: 411770
Conc: 20.67 ng/ml