

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB031622\
 Data File : FB026700.D
 Signal(s) : FID2B.CH
 Acq On : 17 Mar 2022 23:25
 Operator : AJ/MA
 Sample : N1970-03
 Misc : 5.02G/5.00 ML DI WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Mar 17 01:02:04 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030822.M
 Quant Title :
 QLast Update : Fri Mar 11 13:08:49 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.790	138511	13.200 ng/ml
Target Compounds			
4) t Benzene	7.889	47333	2.051 ng/ml
6) t Toluene	10.618	18343	0.838 ng/ml
7) t Ethylbenzene	13.053	150301	7.478 ng/ml
8) t m-Xylene	13.184	200720	9.960 ng/ml
9) t O-Xylene	13.913	81230	4.072 ng/ml
10) t 1,2,4-Trimethylbenzene	16.190	91234	4.579 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB031622\
Data File : FB026700.D
Signal(s) : FID2B.CH
Acq On : 17 Mar 2022 23:25
Operator : AJ/MA
Sample : N1970-03
Misc : 5.02G/5.00 ML DI WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Mar 17 01:02:04 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030822.M
Quant Title :
QLast Update : Fri Mar 11 13:08:49 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

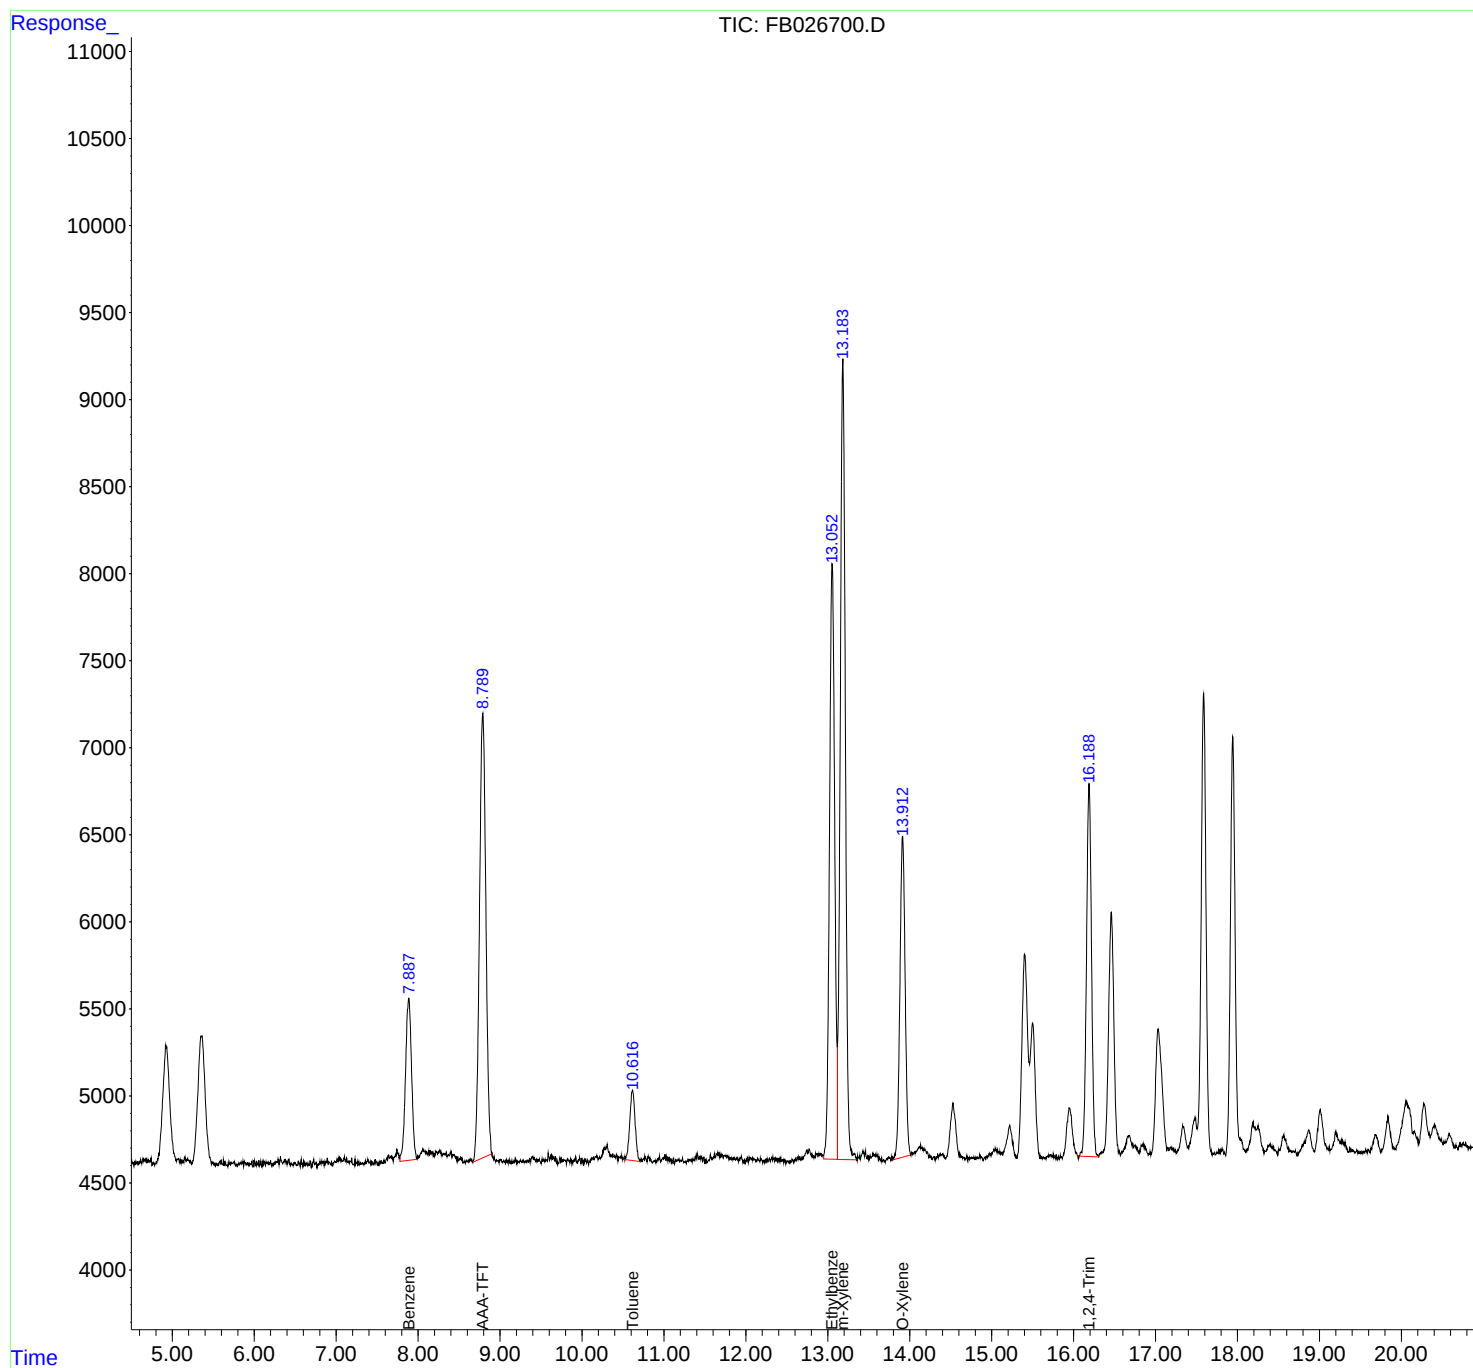


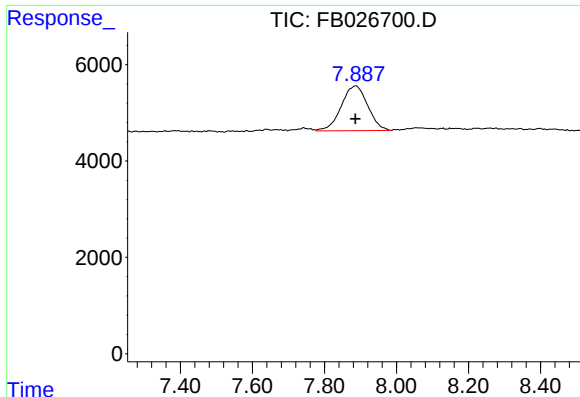

#4 Benzene


R.T.: 7.889 min
Delta R.T.: 0.003 min
Response: 47333
Conc: 2.05 ng/ml

Instrument :
FID_B
ClientSampleId :

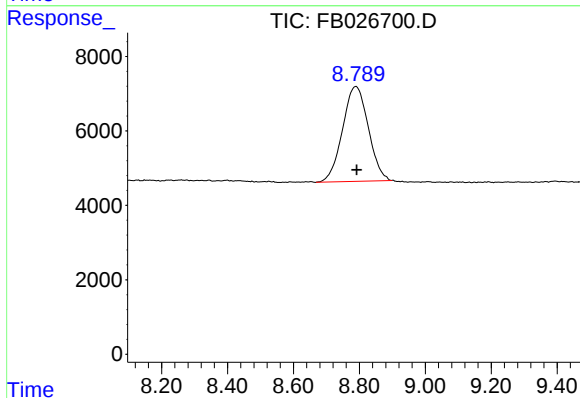


#5 AAA-TFT

R.T.: 8.790 min
Delta R.T.: -0.001 min
Response: 138511
Conc: 13.20 ng/ml

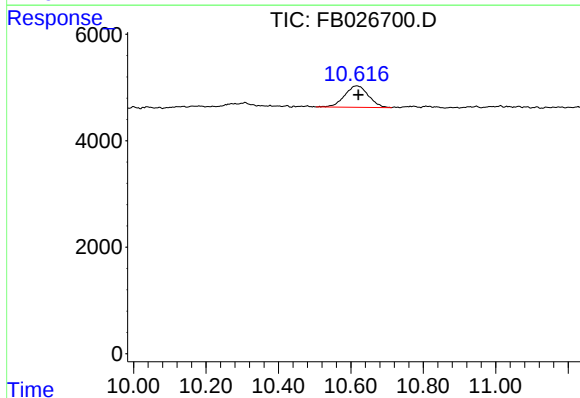


#6 Toluene

R.T.: 10.618 min
Delta R.T.: -0.003 min
Response: 18343
Conc: 0.84 ng/ml

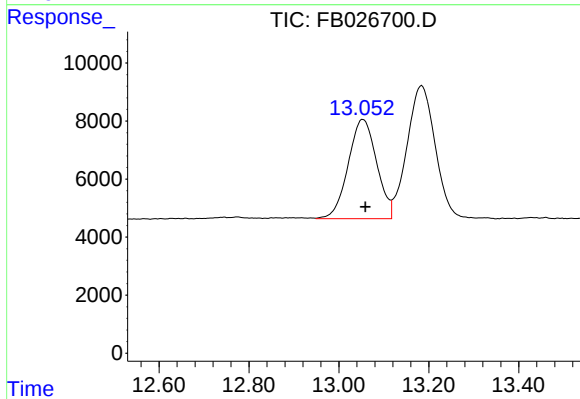

#7 Ethylbenzene


R.T.: 13.053 min
Delta R.T.: -0.005 min
Response: 150301
Conc: 7.48 ng/ml

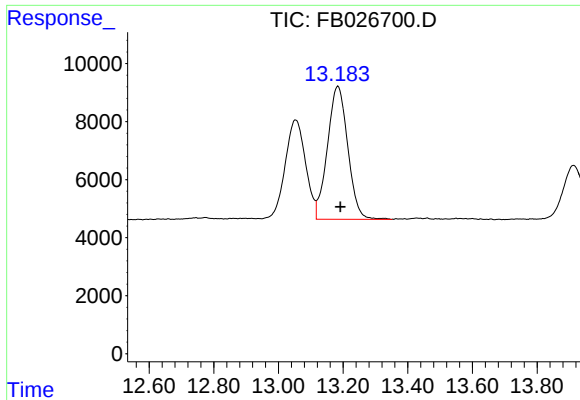

#8 m-Xylene


R.T.: 13.184 min
Delta R.T.: -0.007 min
Response: 200720
Conc: 9.96 ng/ml

Instrument :
FID_B
ClientSampleId :

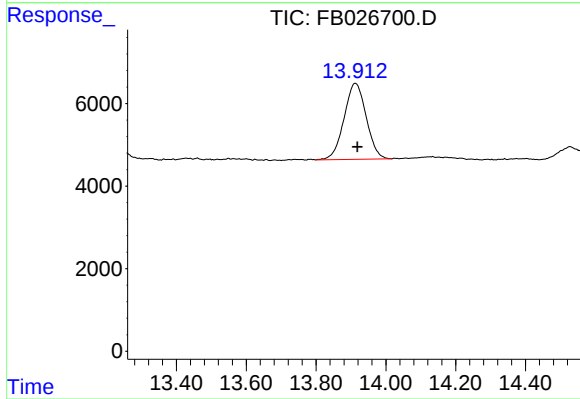

#9 O-Xylene

R.T.: 13.913 min
Delta R.T.: -0.006 min
Response: 81230
Conc: 4.07 ng/ml

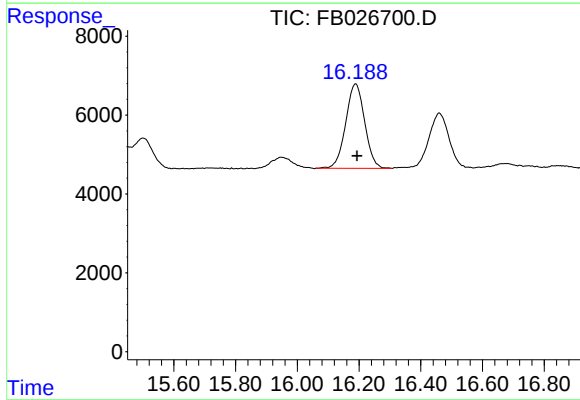

#10 1,2,4-Trimethylbenzene

R.T.: 16.190 min
Delta R.T.: -0.005 min
Response: 91234
Conc: 4.58 ng/ml