

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB031622\
Data File : FB026704.D
Signal(s) : FID2B.CH
Acq On : 17 Mar 2022 2:36
Operator : AJ/MA
Sample : N1970-11
Misc : 5.02G/5.00 ML DI WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Mar 17 04:25:39 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030822.M
Quant Title :
QLast Update : Fri Mar 11 13:08:49 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.791	150327	14.326 ng/ml
Target Compounds			
4) t Benzene	7.890	6472	0.280 ng/ml
7) t Ethylbenzene	13.067	6528	0.325 ng/ml
8) t m-Xylene	13.185	7056	0.350 ng/ml
10) t 1,2,4-Trimethylbenzene	16.185	1745	0.088 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB031622\
Data File : FB026704.D
Signal(s) : FID2B.CH
Acq On : 17 Mar 2022 2:36
Operator : AJ/MA
Sample : N1970-11
Misc : 5.02G/5.00 ML DI WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Mar 17 04:25:39 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030822.M
Quant Title :
QLast Update : Fri Mar 11 13:08:49 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

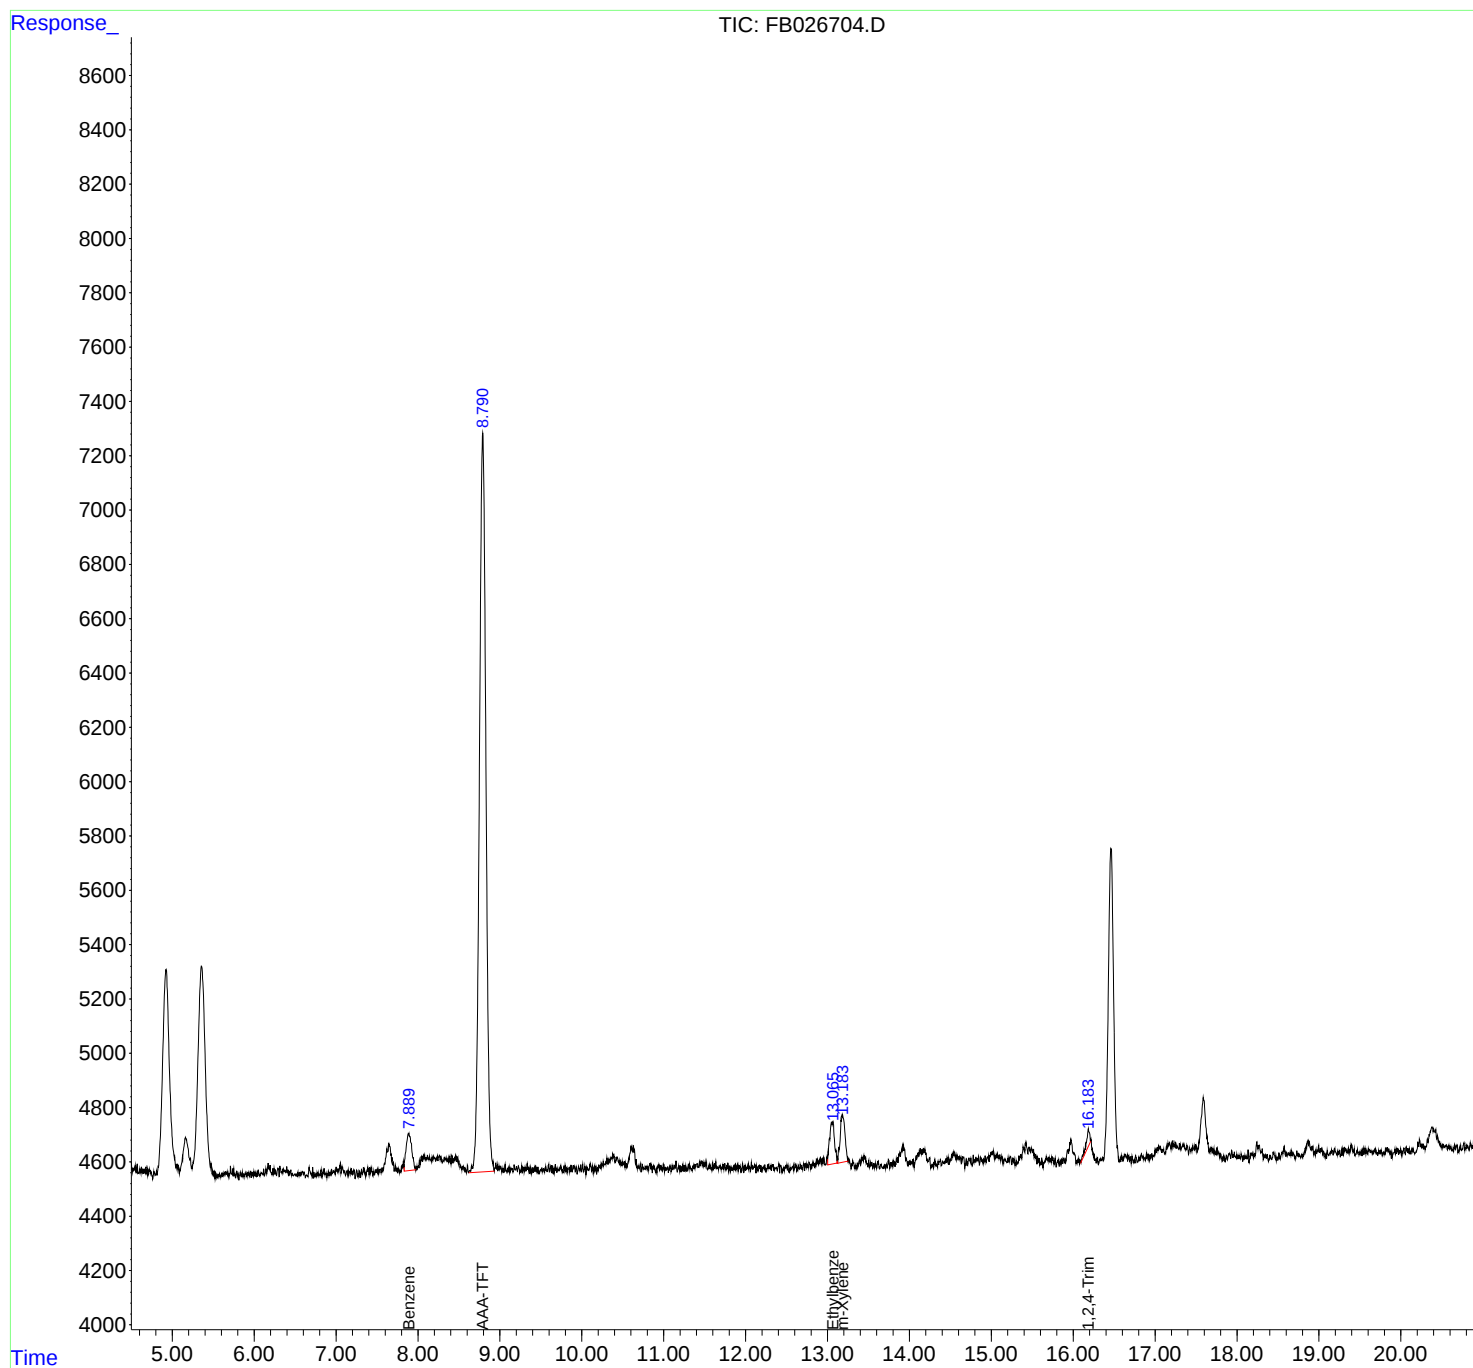


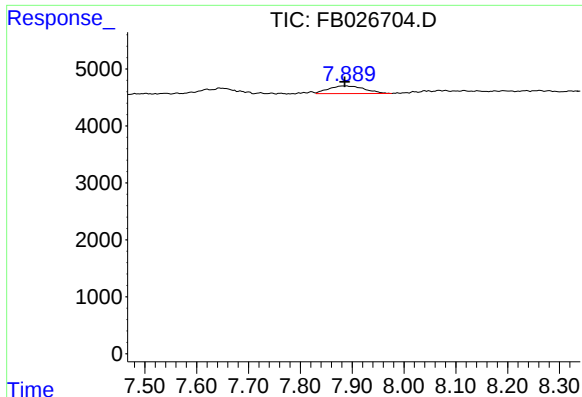

#4 Benzene


R.T.: 7.890 min
Delta R.T.: 0.004 min
Response: 6472
Conc: 0.28 ng/ml

Instrument :
FID_B
ClientSampleId :

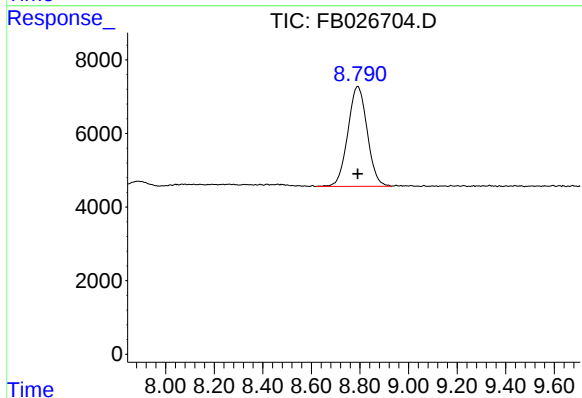


#5 AAA-TFT

R.T.: 8.791 min
Delta R.T.: 0.000 min
Response: 150327
Conc: 14.33 ng/ml

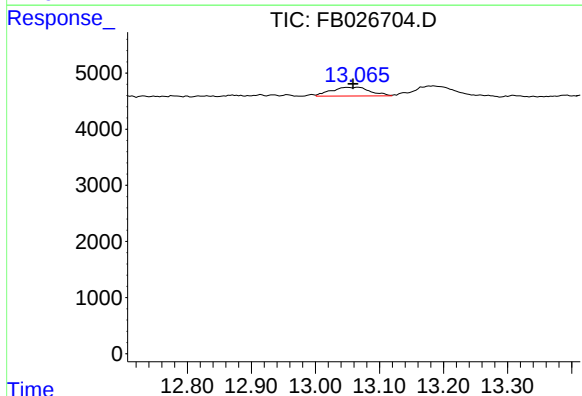


#7 Ethylbenzene

R.T.: 13.067 min
Delta R.T.: 0.008 min
Response: 6528
Conc: 0.32 ng/ml

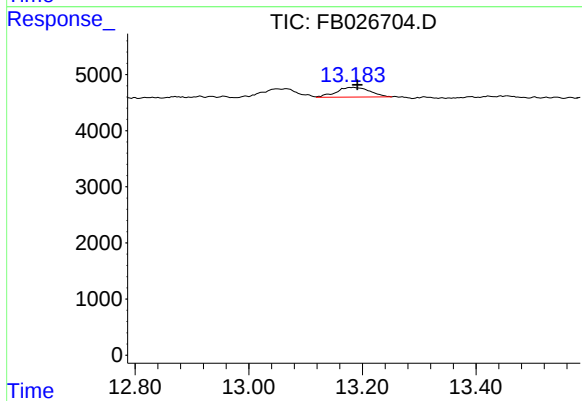

#8 m-Xylene

R.T.: 13.185 min
Delta R.T.: -0.007 min
Response: 7056
Conc: 0.35 ng/ml

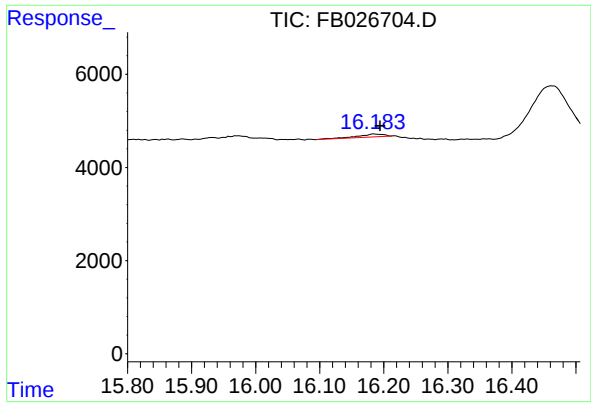

#10 1,2,4-Trimethylbenzene

R.T.: 16.185 min
Delta R.T.: -0.009 min
Response: 1745
Conc: 0.09 ng/ml

Instrument :
FID_B
ClientSampleId :