

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB031622\
 Data File : FB026705.D
 Signal(s) : FID2B.CH
 Acq On : 17 Mar 2022 3:14
 Operator : AJ/MA
 Sample : N1970-13
 Misc : 5.04G/5.00 ML DI WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Mar 17 07:44:16 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030822.M
 Quant Title :
 QLast Update : Fri Mar 11 13:08:49 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.791	89629	8.541 ng/ml
Target Compounds			
4) t Benzene	7.885	19746	0.856 ng/ml
6) t Toluene	10.622	4775	0.218 ng/ml
7) t Ethylbenzene	13.054	15807	0.787 ng/ml
8) t m-Xylene	13.189	17702	0.878 ng/ml
9) t O-Xylene	13.916	3887	0.195 ng/ml
10) t 1,2,4-Trimethylbenzene	16.188	11739	0.589 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB031622\
Data File : FB026705.D
Signal(s) : FID2B.CH
Acq On : 17 Mar 2022 3:14
Operator : AJ/MA
Sample : N1970-13
Misc : 5.04G/5.00 ML DI WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Mar 17 07:44:16 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030822.M
Quant Title :
QLast Update : Fri Mar 11 13:08:49 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

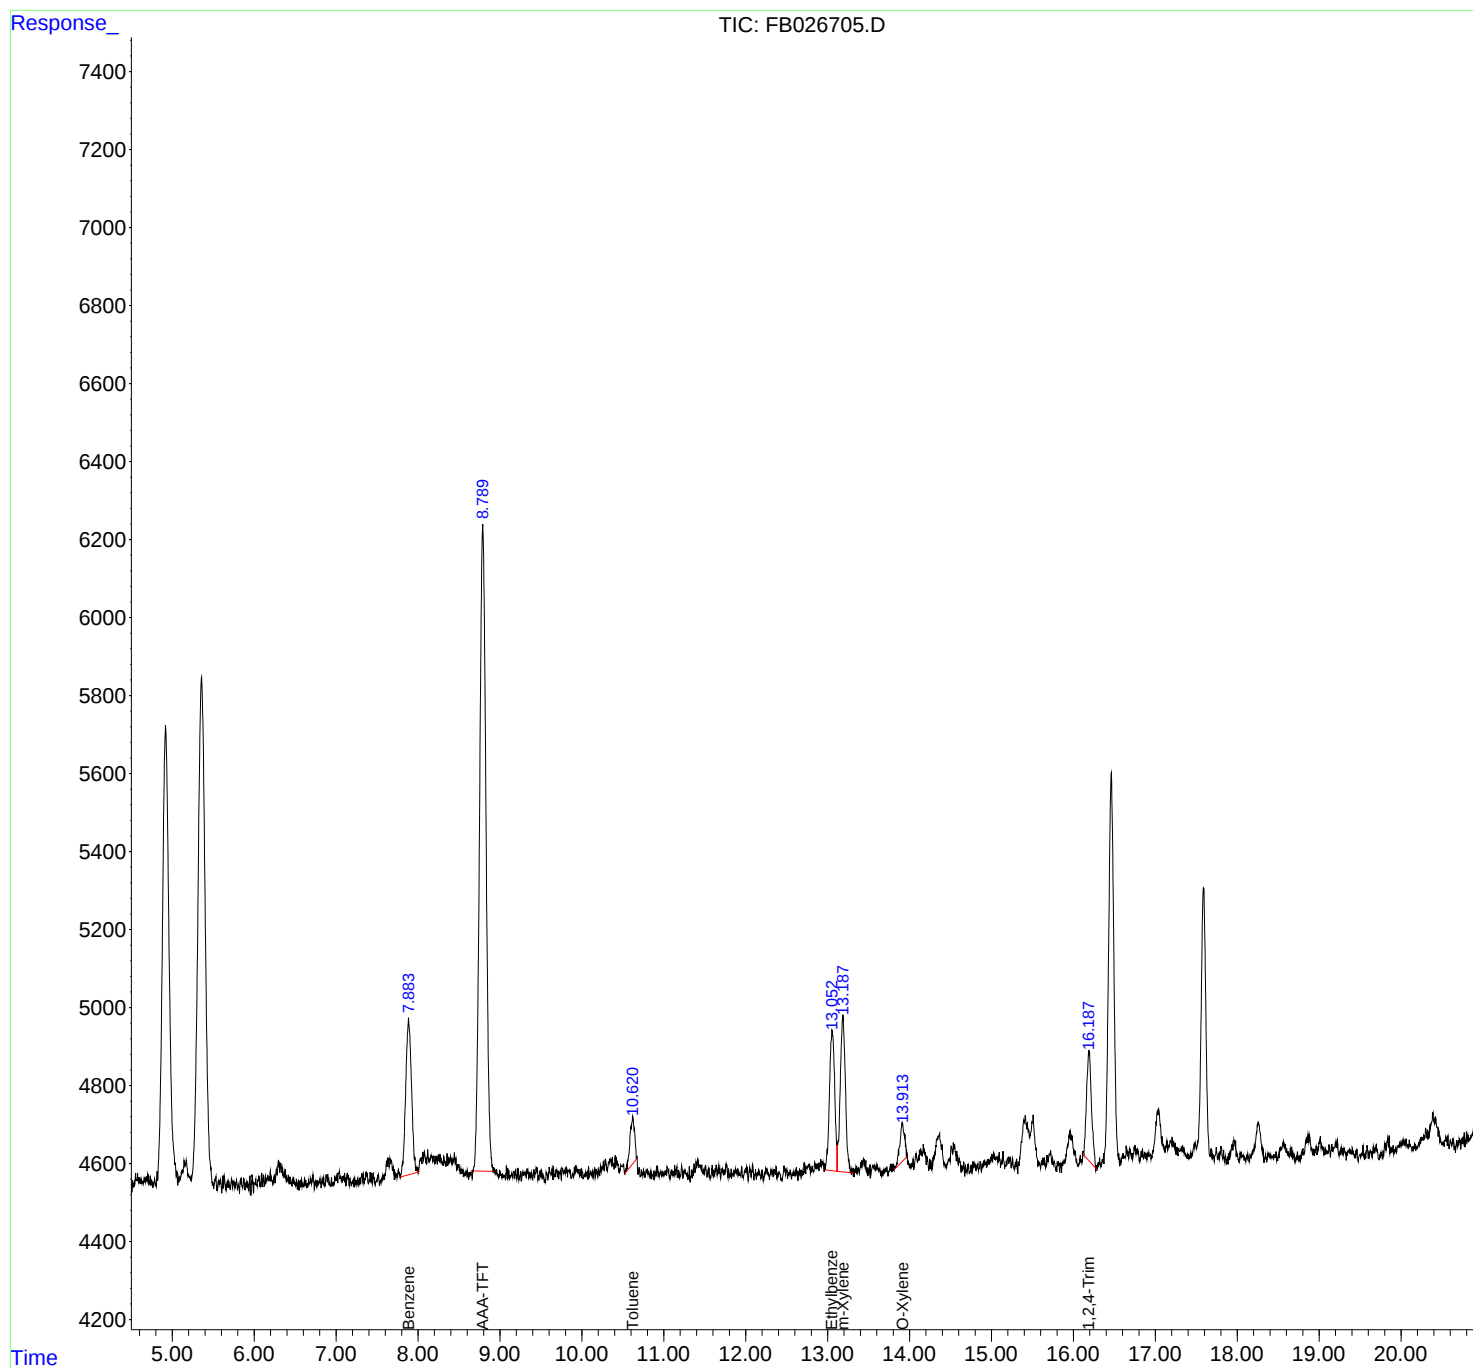


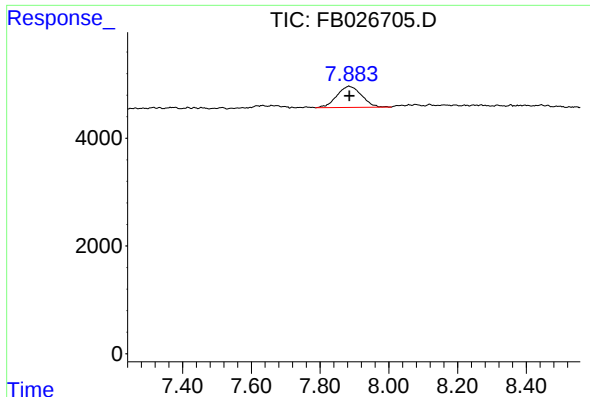

#4 Benzene


R.T.: 7.885 min
Delta R.T.: -0.001 min
Response: 19746
Conc: 0.86 ng/ml

Instrument :
FID_B
ClientSampleId :

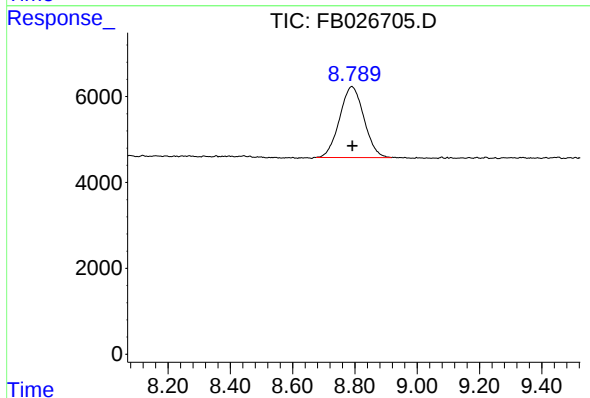


#5 AAA-TFT

R.T.: 8.791 min
Delta R.T.: 0.000 min
Response: 89629
Conc: 8.54 ng/ml

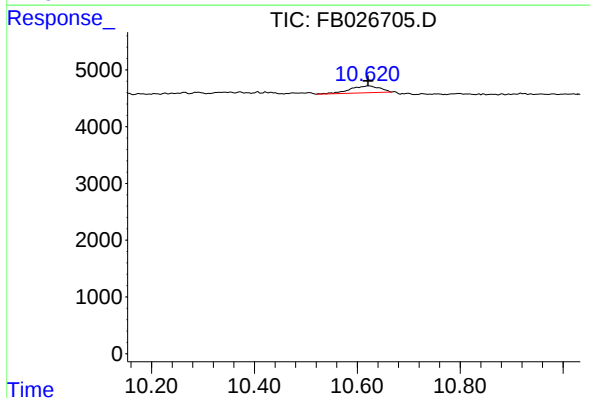


#6 Toluene

R.T.: 10.622 min
Delta R.T.: 0.001 min
Response: 4775
Conc: 0.22 ng/ml

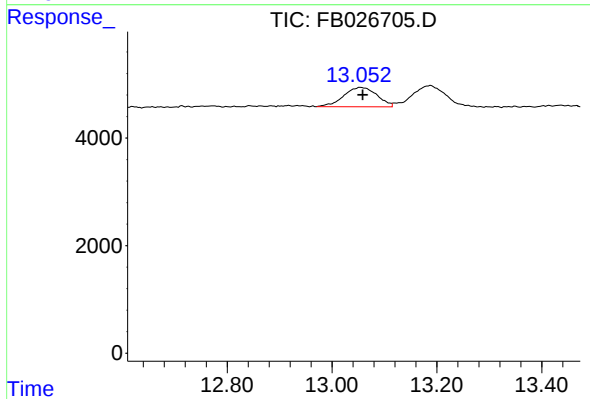

#7 Ethylbenzene


R.T.: 13.054 min
Delta R.T.: -0.005 min
Response: 15807
Conc: 0.79 ng/ml

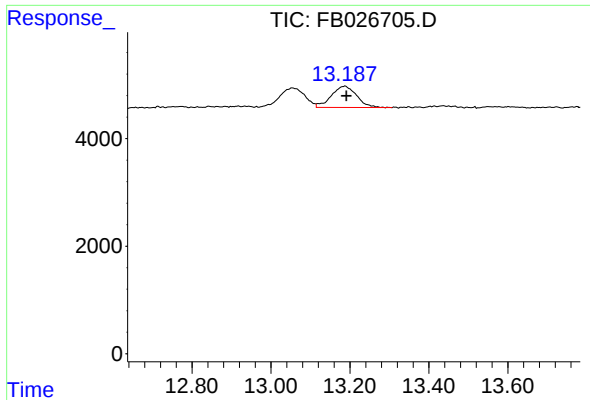

#8 m-Xylene


R.T.: 13.189 min
Delta R.T.: -0.003 min
Response: 17702
Conc: 0.88 ng/ml

Instrument :
FID_B
ClientSampleId :

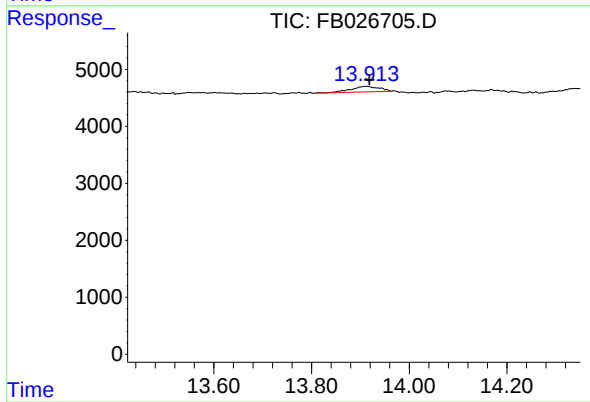

#9 O-Xylene

R.T.: 13.916 min
Delta R.T.: -0.003 min
Response: 3887
Conc: 0.19 ng/ml

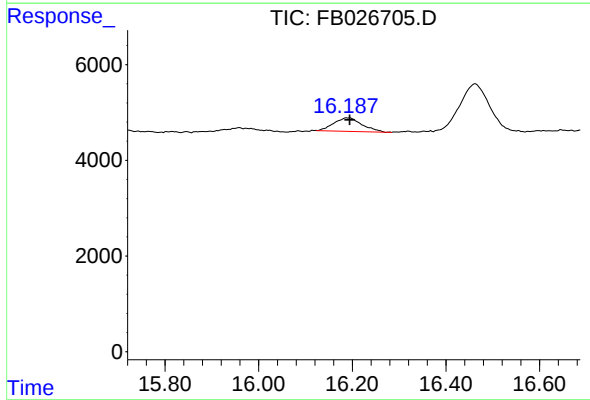

#10 1,2,4-Trimethylbenzene

R.T.: 16.188 min
Delta R.T.: -0.007 min
Response: 11739
Conc: 0.59 ng/ml