

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB031622\
 Data File : FB026719.D
 Signal(s) : FID2B.CH
 Acq On : 17 Mar 2022 13:37
 Operator : AJ/MA
 Sample : N1970-02
 Misc : 5.01G/5.00 ML DI WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Mar 17 15:10:23 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030822.M
 Quant Title :
 QLast Update : Fri Mar 11 13:08:49 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.794	5651	0.539 ng/ml
Target Compounds			
4) t Benzene	7.891	4378	0.190 ng/ml
7) t Ethylbenzene	13.064	12182	0.606 ng/ml
8) t m-Xylene	13.190	13857	0.688 ng/ml
9) t O-Xylene	13.912	4599	0.231 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB031622\
Data File : FB026719.D
Signal(s) : FID2B.CH
Acq On : 17 Mar 2022 13:37
Operator : AJ/MA
Sample : N1970-02
Misc : 5.01G/5.00 ML DI WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Mar 17 15:10:23 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030822.M
Quant Title :
QLast Update : Fri Mar 11 13:08:49 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

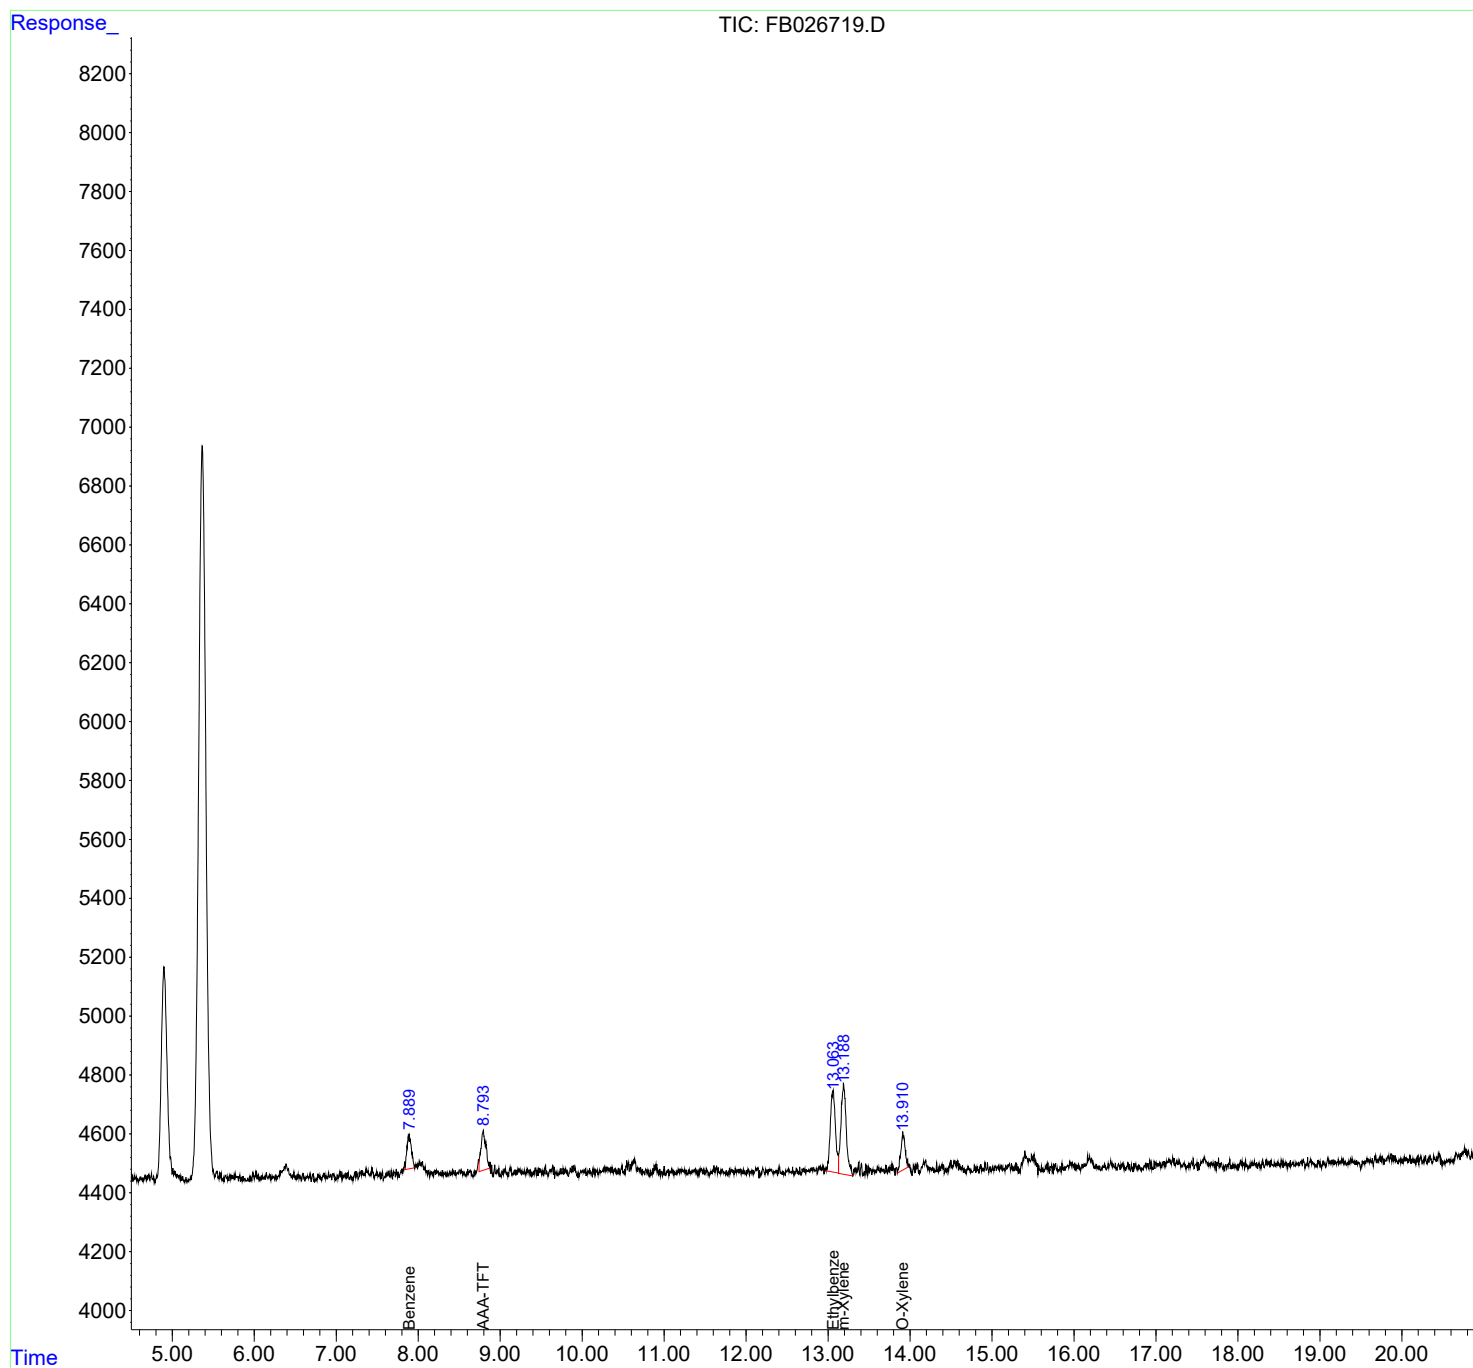


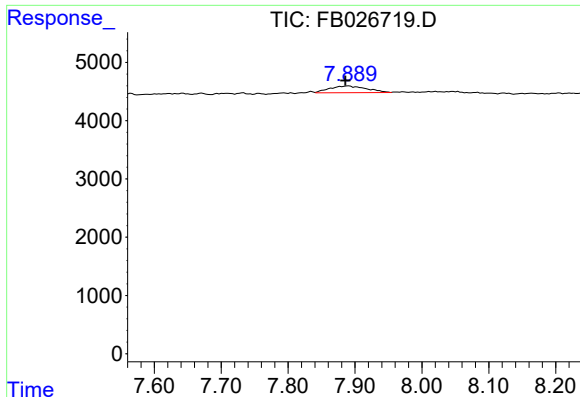

#4 Benzene


R.T.: 7.891 min
Delta R.T.: 0.005 min
Response: 4378
Conc: 0.19 ng/ml

Instrument :
FID_B
ClientSampleId :

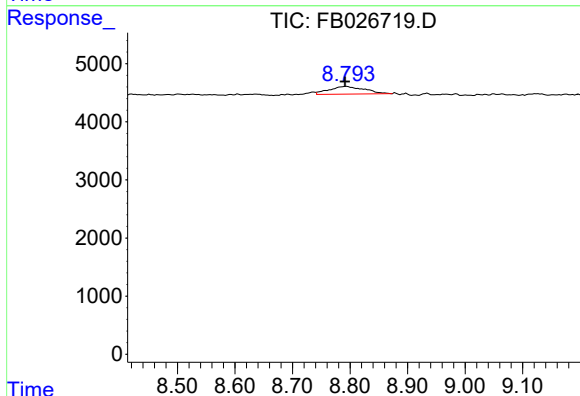


#5 AAA-TFT

R.T.: 8.794 min
Delta R.T.: 0.003 min
Response: 5651
Conc: 0.54 ng/ml

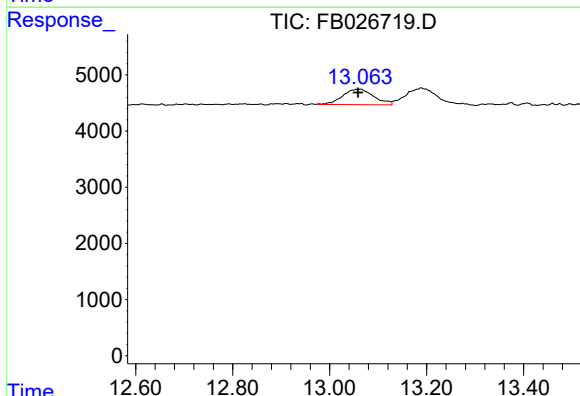


#7 Ethylbenzene

R.T.: 13.064 min
Delta R.T.: 0.005 min
Response: 12182
Conc: 0.61 ng/ml

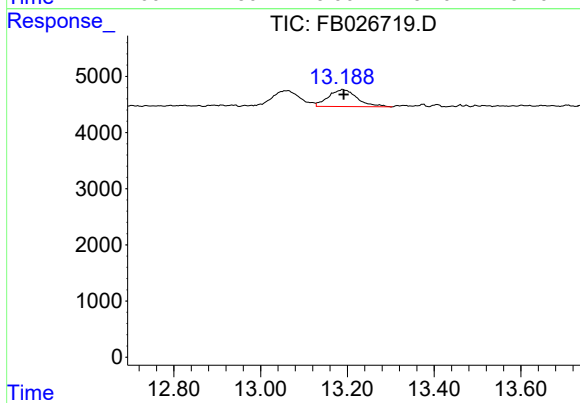

#8 m-Xylene

R.T.: 13.190 min
Delta R.T.: -0.002 min
Response: 13857
Conc: 0.69 ng/ml

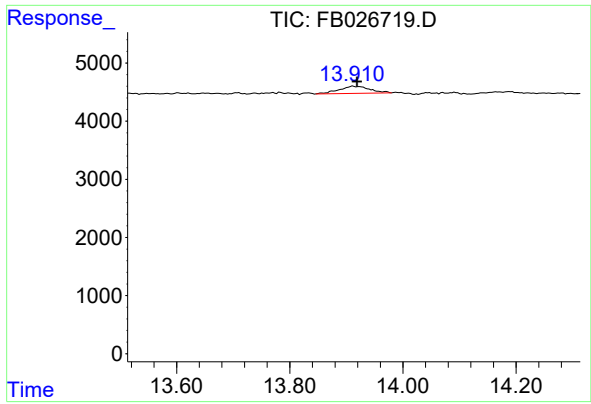

#9 O-Xylene

R.T.: 13.912 min
Delta R.T.: -0.007 min
Response: 4599
Conc: 0.23 ng/ml

Instrument :
FID_B
ClientSampleId :